

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037857.D
 Acq On : 14 Oct 2024 15:21
 Operator : SY/MD
 Sample : P4378-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV	5363	9411	0.40%	0.055%
2	1.282	68	75	92	rVB	263174	283555	12.18%	1.672%
3	1.532	146	153	172	rVB	246456	298275	12.82%	1.758%
4	2.060	307	317	335	rBV	504081	732029	31.45%	4.315%
5	3.670	816	818	823	rVB2	663	514	0.02%	0.003%
6	3.693	823	825	829	rBV2	445	385	0.02%	0.002%
7	3.728	833	836	839	rVB3	860	504	0.02%	0.003%
8	3.748	839	842	843	rBV2	402	232	0.01%	0.001%
9	3.796	849	857	890	rBV	103886	297813	12.80%	1.756%
10	4.243	979	996	1025	rBV	379314	974668	41.88%	5.746%
11	4.555	1090	1093	1094	rBV	537	287	0.01%	0.002%
12	4.715	1141	1143	1144	rBV	226	100	0.00%	0.001%
13	4.748	1151	1153	1154	rBV2	392	129	0.01%	0.001%
14	4.783	1162	1164	1166	rBV3	339	184	0.01%	0.001%
15	4.867	1188	1190	1191	rBV	458	204	0.01%	0.001%
16	4.879	1192	1194	1196	rBV	566	296	0.01%	0.002%
17	4.947	1200	1215	1247	rBV2	919442	2327295	100.00%	13.720%
18	5.529	1385	1396	1427	rBV	681533	1413346	60.73%	8.332%
19	5.982	1525	1537	1566	rBV	527407	1085523	46.64%	6.399%
20	6.497	1693	1697	1700	rVB3	935	669	0.03%	0.004%
21	6.526	1700	1706	1708	rBV4	1160	906	0.04%	0.005%
22	6.603	1728	1730	1731	rBV	367	134	0.01%	0.001%
23	6.632	1736	1739	1740	rBV3	401	226	0.01%	0.001%
24	6.664	1747	1749	1752	rBV	866	428	0.02%	0.003%
25	6.680	1752	1754	1755	rBV	426	179	0.01%	0.001%
26	6.731	1767	1770	1771	rVB3	257	108	0.00%	0.001%
27	6.741	1771	1773	1774	rBV	326	131	0.01%	0.001%
28	6.754	1774	1777	1781	rVB6	922	728	0.03%	0.004%
29	6.783	1781	1786	1793	rVB6	852	816	0.04%	0.005%
30	6.812	1793	1795	1798	rVB	354	206	0.01%	0.001%
31	6.834	1798	1802	1805	rBV2	877	662	0.03%	0.004%
32	6.850	1805	1807	1812	rVB3	473	316	0.01%	0.002%
33	6.908	1812	1825	1858	rBV	256836	506430	21.76%	2.986%
34	7.236	1916	1927	1954	rBV	1036093	1818707	78.15%	10.722%
35	7.548	2016	2024	2050	rBV	171213	328661	14.12%	1.938%
36	7.918	2136	2139	2143	rBV3	859	592	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037857.D
 Acq On : 14 Oct 2024 15:21
 Operator : SY/MD
 Sample : P4378-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.960	2151	2152	2154	rBV	517	267	0.01%	0.002%
38	8.024	2164	2172	2215	rBV2	315280	703458	30.23%	4.147%
39	8.776	2395	2406	2440	rBV	1087659	1808903	77.73%	10.664%
40	9.204	2536	2539	2545	rVB4	687	609	0.03%	0.004%
41	9.239	2545	2550	2551	rBV3	750	555	0.02%	0.003%
42	9.307	2570	2571	2574	rVB2	649	344	0.01%	0.002%
43	9.329	2576	2578	2580	rBV3	754	485	0.02%	0.003%
44	9.368	2588	2590	2592	rBV2	575	243	0.01%	0.001%
45	9.397	2598	2599	2602	rBV	582	403	0.02%	0.002%
46	9.461	2615	2619	2621	rBV3	723	510	0.02%	0.003%
47	9.474	2621	2623	2624	rBV	645	281	0.01%	0.002%
48	9.532	2638	2641	2644	rBV4	842	615	0.03%	0.004%
49	9.580	2654	2656	2660	rBV3	627	375	0.02%	0.002%
50	9.625	2669	2670	2674	rVB2	683	333	0.01%	0.002%
51	9.654	2676	2679	2681	rBV3	543	394	0.02%	0.002%
52	9.680	2686	2687	2688	rBV3	277	79	0.00%	0.000%
53	9.693	2688	2691	2692	rBV2	297	127	0.01%	0.001%
54	9.706	2692	2695	2697	rBV2	807	482	0.02%	0.003%
55	9.760	2709	2712	2717	rBV3	871	852	0.04%	0.005%
56	9.831	2729	2734	2737	rBV5	815	687	0.03%	0.004%
57	9.850	2738	2740	2742	rVV3	589	328	0.01%	0.002%
58	9.886	2746	2751	2753	rBV2	910	652	0.03%	0.004%
59	9.915	2758	2760	2763	rVB2	632	275	0.01%	0.002%
60	9.976	2776	2779	2780	rBV	614	349	0.01%	0.002%
61	9.995	2783	2785	2788	rBV4	645	512	0.02%	0.003%
62	10.046	2799	2801	2803	rBV2	104	46	0.00%	0.000%
63	10.056	2803	2804	2805	rBV2	431	158	0.01%	0.001%
64	10.146	2818	2832	2853	rBV	621591	994198	42.72%	5.861%
65	10.371	2897	2902	2903	rBV2	692	477	0.02%	0.003%
66	10.384	2903	2906	2913	rVB4	910	969	0.04%	0.006%
67	10.416	2913	2916	2918	rBV2	769	534	0.02%	0.003%
68	10.493	2938	2940	2942	rVB2	545	245	0.01%	0.001%
69	10.606	2974	2975	2976	rBV	233	55	0.00%	0.000%
70	10.657	2987	2991	2993	rBV3	698	491	0.02%	0.003%
71	10.702	3003	3005	3006	rBV	527	147	0.01%	0.001%
72	10.757	3019	3022	3026	rVB4	986	896	0.04%	0.005%
73	10.780	3026	3029	3032	rBV3	1052	712	0.03%	0.004%
74	10.818	3037	3041	3044	rBV4	543	604	0.03%	0.004%
75	10.850	3050	3051	3054	rBV2	434	211	0.01%	0.001%
76	10.902	3064	3067	3071	rVB2	696	424	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
 Data File : VV037857.D
 Acq On : 14 Oct 2024 15:21
 Operator : SY/MD
 Sample : P4378-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.940	3074	3079	3084	rBV3	688	719	0.03%	0.004%
78	10.963	3084	3086	3089	rBV	317	184	0.01%	0.001%
79	11.008	3095	3100	3103	rBV2	769	951	0.04%	0.006%
80	11.043	3108	3111	3117	rVV3	592	609	0.03%	0.004%
81	11.178	3142	3153	3189	rBV	1003906	1627802	69.94%	9.596%
82	11.551	3258	3269	3301	rBV	1062525	1720489	73.93%	10.143%
83	11.943	3389	3391	3394	rBV	690	533	0.02%	0.003%
84	12.091	3435	3437	3445	rBV5	1045	1006	0.04%	0.006%
85	12.210	3471	3474	3483	rBV5	917	1213	0.05%	0.007%
86	12.278	3493	3495	3498	rBV2	1041	555	0.02%	0.003%
87	12.538	3572	3576	3579	rBV2	626	543	0.02%	0.003%
88	12.567	3584	3585	3587	rBV2	629	312	0.01%	0.002%
89	12.911	3690	3692	3697	rBV4	758	544	0.02%	0.003%
90	13.037	3729	3731	3732	rBV2	840	418	0.02%	0.002%




Sum of corrected areas: 16962812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037857.D
Acq On : 14 Oct 2024 15:21
Operator : SY/MD
Sample : P4378-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

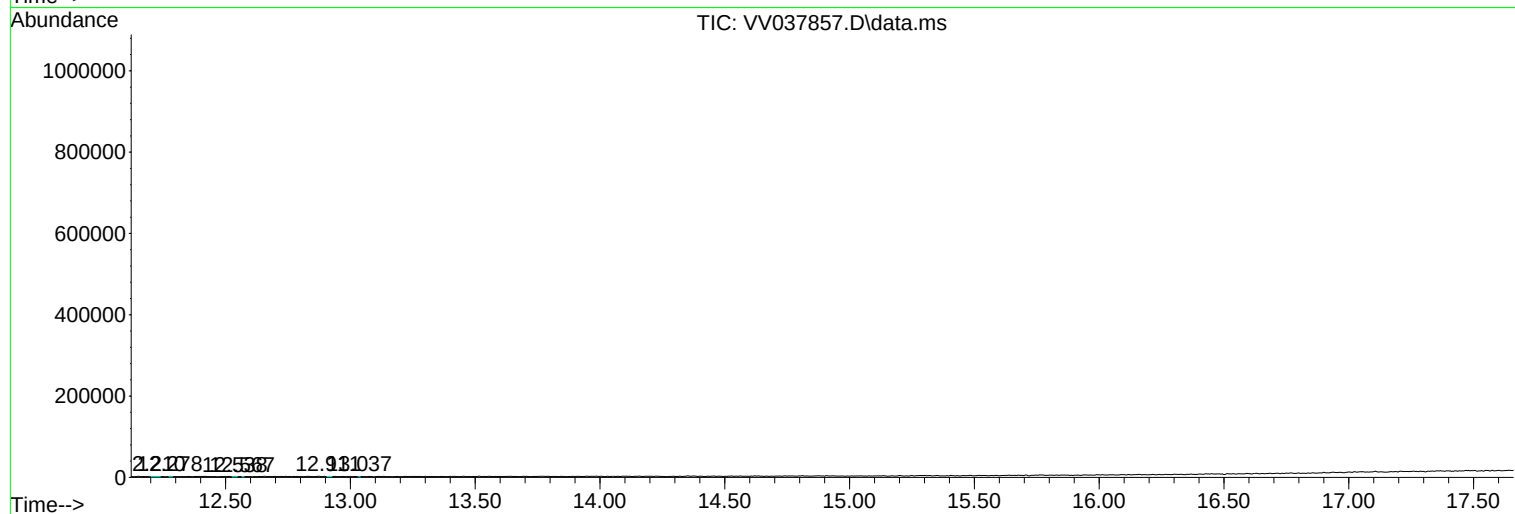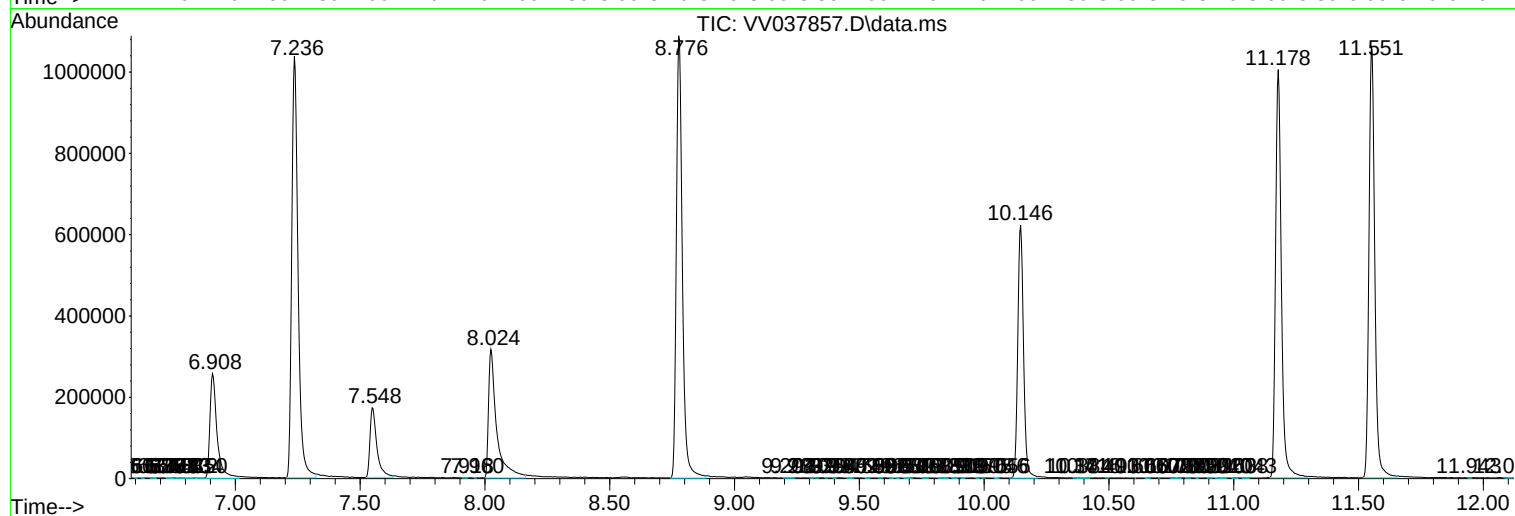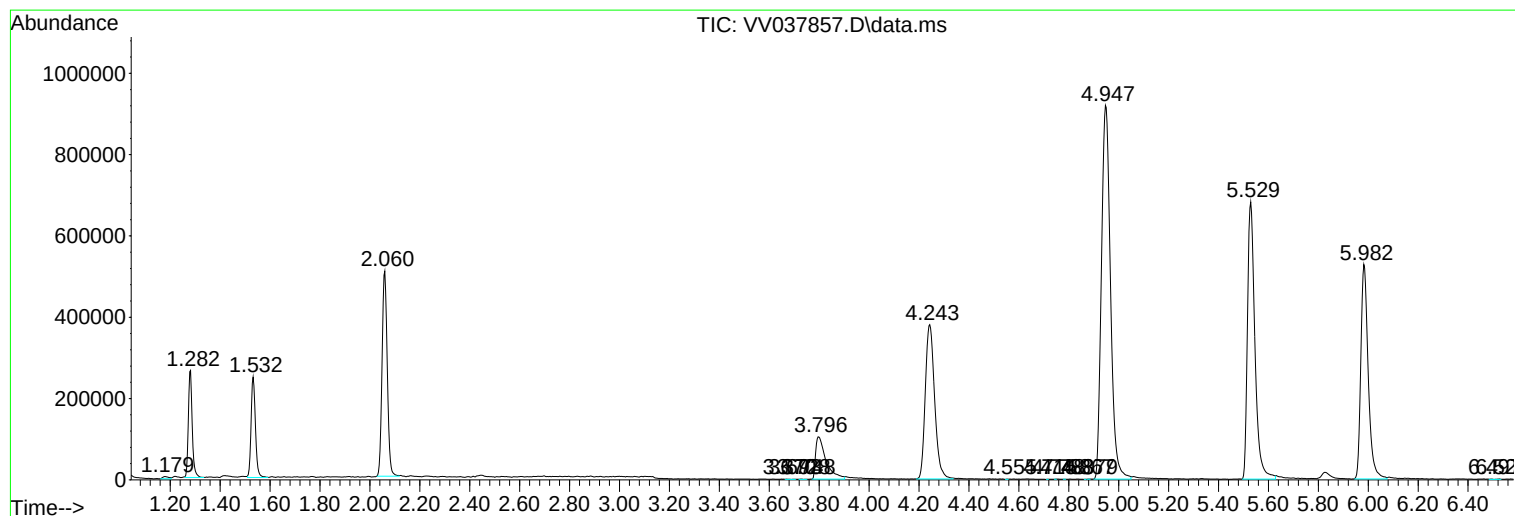

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037857.D
Acq On : 14 Oct 2024 15:21
Operator : SY/MD
Sample : P4378-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037857.D
Acq On : 14 Oct 2024 15:21
Operator : SY/MD
Sample : P4378-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------