


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101424\
Data File : VV037841.D
Acq On : 14 Oct 2024 08:41
Operator : SY/MD
Sample : BFB393
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB393

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Tue Oct 15 02:19:17 2024

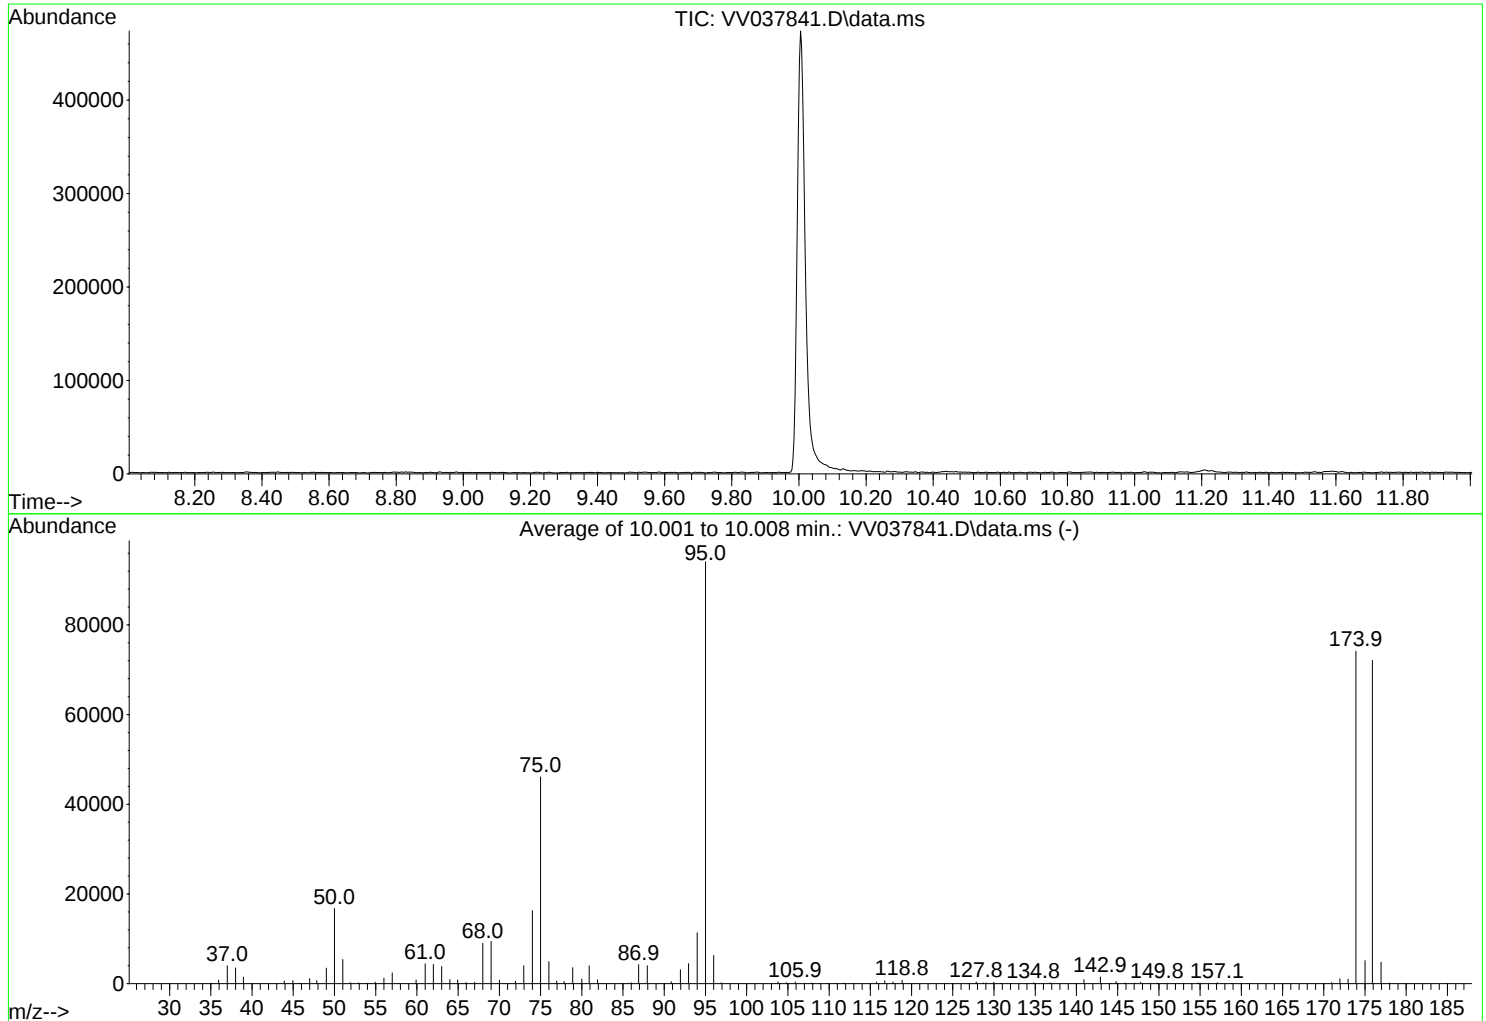

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	16741	PASS
75	95	30	80	49.0	46112	PASS
95	95	100	100	100.0	94075	PASS
96	95	5	9	6.7	6297	PASS
173	174	0.00	2	1.4	1014	PASS
174	95	50	120	78.8	74157	PASS
175	174	5	9	6.9	5135	PASS
176	174	95	105	97.2	72085	PASS
177	176	5	10	6.7	4796	PASS

m/z	Abundance
39.90	577.0
44.00	779.0
76.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.10	125.0
35.90	691.0
37.00	3998.0
38.00	3367.0
38.90	1492.0
39.90	552.0
43.90	1414.0
44.90	712.0
45.80	105.0
47.00	1074.0
47.90	712.0
49.00	3536.0
50.00	16271.0
51.00	5416.0
51.90	186.0
52.90	181.0
54.00	134.0
55.00	313.0
56.00	1207.0
57.00	2310.0
59.90	828.0
61.00	4440.0
62.00	4597.0
63.00	3699.0
64.00	946.0
65.00	703.0
65.90	218.0
67.00	368.0
68.00	8953.0
69.00	9242.0
70.00	826.0
71.90	501.0
72.90	4043.0
74.00	15828.0
75.00	44632.0
76.00	4687.0
77.00	803.0
77.90	483.0
78.90	3400.0
80.00	944.0
80.90	3857.0
81.90	842.0
86.00	205.0
86.90	4243.0
88.00	3966.0
90.90	418.0
92.00	3108.0
93.00	4283.0
94.00	11169.0
95.00	91072.0
96.00	6195.0
96.90	178.0
103.80	351.0
104.80	234.0
105.90	388.0
107.90	110.0
111.80	104.0
115.70	362.0
116.80	677.0
117.70	406.0
118.90	747.0
127.80	360.0
128.70	242.0
130.00	189.0
134.80	159.0
136.80	150.0
140.90	830.0
142.90	1398.0
144.80	530.0
145.90	189.0
147.10	162.0
147.80	330.0
149.80	191.0
154.70	264.0
157.10	202.0
171.00	300.0
171.90	898.0
173.00	990.0
173.90	70512.0
175.00	4874.0
175.90	67368.0
177.00	4524.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.10	113.0
35.90	807.0
37.00	4125.0
38.00	3706.0
39.00	1469.0
39.90	556.0
43.90	1415.0
45.00	699.0
45.80	123.0
47.00	1232.0
47.80	719.0
49.00	3510.0
50.00	17400.0
51.00	5522.0
51.90	224.0
52.90	178.0
54.00	118.0
55.00	348.0
56.00	1285.0
57.00	2437.0
59.90	825.0
61.00	4601.0
62.00	4328.0
63.00	3983.0
64.00	904.0
65.00	854.0
65.90	268.0
67.00	353.0
68.00	9370.0
69.00	9792.0
70.00	768.0
72.00	516.0
73.00	4082.0
74.00	16808.0
75.00	47600.0
76.00	5182.0
77.00	722.0
77.90	530.0
78.90	3681.0
80.00	1073.0
80.90	4176.0
81.90	890.0
85.70	167.0
86.00	184.0
86.90	4378.0
88.00	4166.0
90.90	439.0
92.00	3272.0
93.00	4586.0
94.00	11744.0
95.00	97192.0
96.00	6410.0
96.90	171.0
103.80	382.0
104.80	232.0
105.90	442.0
107.90	155.0
109.80	108.0
110.70	115.0
111.80	159.0
112.90	119.0
115.70	414.0
116.70	667.0
117.70	406.0
118.90	784.0
127.90	395.0
128.70	221.0
129.00	214.0
129.90	269.0
130.80	110.0
134.80	165.0
136.80	176.0
140.90	931.0
142.90	1593.0
144.80	519.0
145.90	167.0
147.10	139.0
147.80	338.0
149.80	173.0
154.80	237.0
157.10	210.0
158.80	107.0
171.00	249.0
172.00	1155.0
173.00	1034.0
173.90	76536.0
175.00	5261.0
175.90	74672.0
176.90	4980.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
36.00	896.0
37.00	3842.0
38.00	3466.0
39.00	1389.0
39.90	587.0
43.00	124.0
43.90	1286.0
44.90	679.0
45.80	141.0
47.00	1163.0
47.80	630.0
49.00	3309.0
50.00	16552.0
51.00	5180.0
51.90	256.0
52.90	142.0
54.90	337.0
56.00	1237.0
57.00	2451.0
57.80	130.0
59.90	840.0
61.00	4217.0
62.00	3941.0
63.00	3775.0
64.00	797.0
64.90	935.0
66.00	237.0
67.00	278.0
68.00	8697.0
69.00	9297.0
70.00	653.0
72.00	574.0
73.00	3894.0
74.00	16232.0
75.00	46104.0
76.00	4945.0
77.00	651.0
77.80	493.0
78.90	3652.0
80.00	1100.0
80.90	3902.0
81.90	798.0
86.00	169.0
86.90	4119.0
87.90	3868.0
90.80	444.0
91.90	2980.0
92.90	4541.0
94.00	11189.0
95.00	93960.0
96.00	6286.0
96.90	156.0
103.80	401.0
104.80	184.0
105.90	399.0
107.90	150.0
110.70	141.0
111.80	156.0
112.90	124.0
115.80	369.0
116.80	573.0
117.80	371.0
118.80	753.0
127.90	375.0
129.10	195.0
129.90	377.0
130.80	135.0
134.80	180.0
136.80	198.0
140.90	919.0
142.90	1562.0
144.10	115.0
144.80	467.0
146.00	116.0
147.70	258.0
149.80	121.0
155.00	233.0
157.10	210.0
158.80	156.0
160.80	136.0
170.90	211.0
172.00	1211.0
172.90	1019.0
173.90	75424.0
175.00	5269.0
175.90	74216.0
177.00	4884.0
178.00	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393