


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101518\
Data File : VV008268.D
Acq On : 15 Oct 2018 09:40
Operator : SY/MD
Sample : BFB86
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB86

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 16 05:17:07 2018

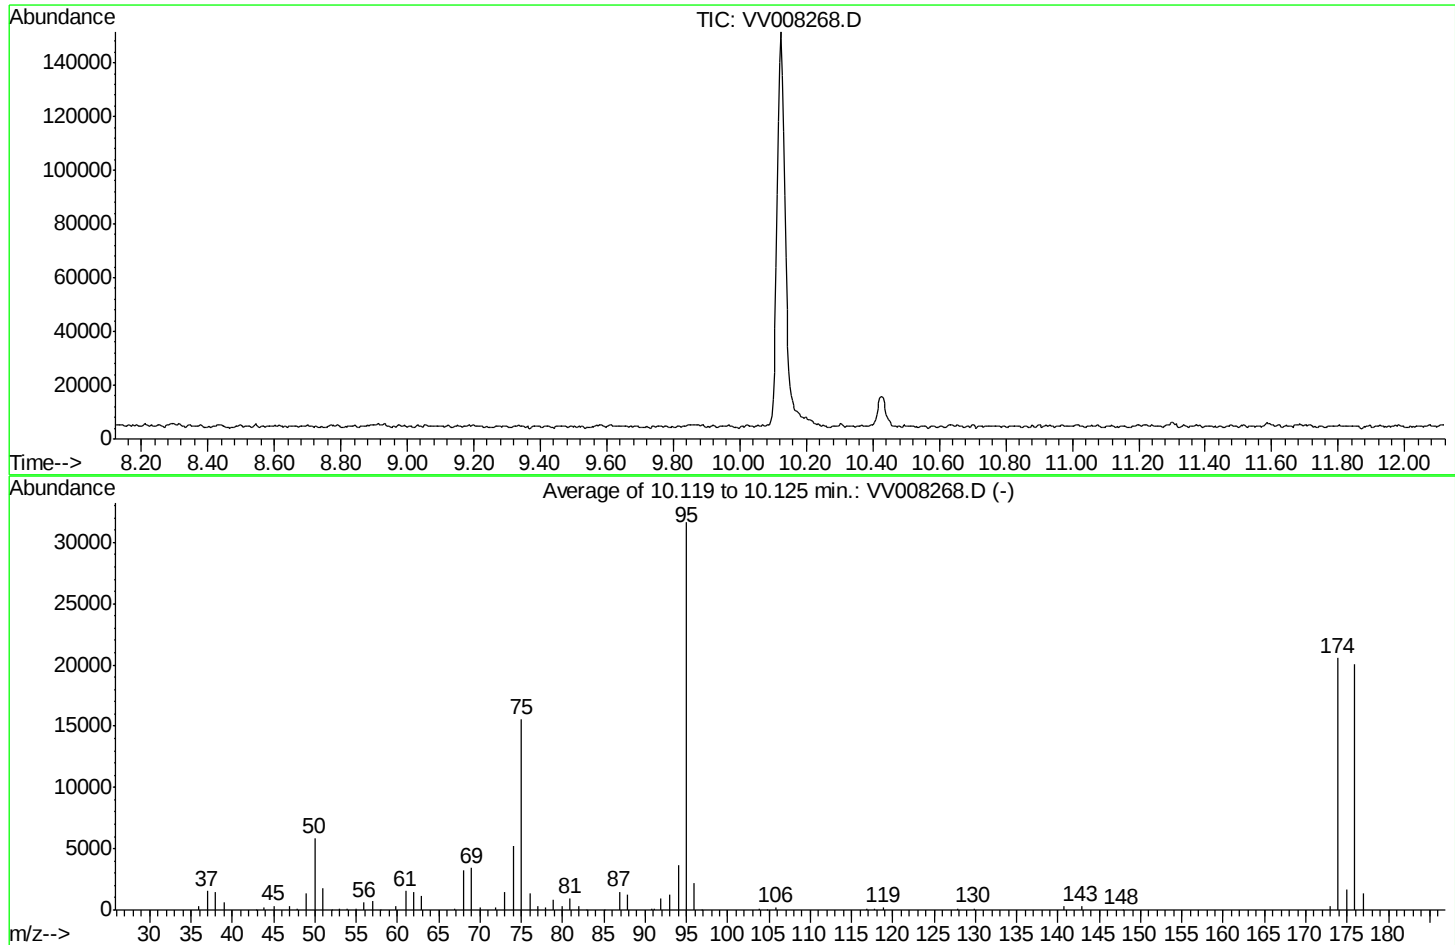

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5820	PASS
75	95	30	80	49.1	15545	PASS
95	95	100	100	100.0	31635	PASS
96	95	5	9	6.8	2156	PASS
173	174	0.00	2	1.3	267	PASS
174	95	50	120	65.0	20565	PASS
175	174	5	9	8.1	1661	PASS
176	174	95	101	97.7	20101	PASS
177	176	5	9	7.0	1410	PASS

m/z	Abundance
39.00	192.0
39.80	200.0
40.90	456.0
42.00	214.0
42.90	421.0
43.90	679.0
55.00	324.0
55.90	188.0
57.00	376.0
57.90	104.0
66.90	109.0
68.00	108.0
69.00	206.0
70.00	167.0
70.90	186.0
78.90	102.0
81.10	132.0
83.00	127.0
85.10	124.0
90.90	105.0
95.00	101.0
95.90	118.0
97.00	104.0
98.00	113.0
206.90	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	332.0
37.00	1435.0
38.00	1414.0
39.00	686.0
39.90	200.0
41.00	418.0
41.90	150.0
43.00	486.0
43.90	934.0
45.00	357.0
47.00	405.0
47.80	122.0
49.00	1273.0
50.00	5699.0
51.00	1616.0
52.00	101.0
53.00	120.0
53.90	122.0
55.00	393.0
56.00	774.0
57.00	1034.0
58.10	123.0
59.80	308.0
61.00	1492.0
62.00	1347.0
62.90	1174.0
67.00	222.0
68.00	3220.0
69.00	3479.0
70.00	334.0
70.90	166.0
71.90	177.0
73.00	1435.0
74.00	5013.0
75.00	14925.0
76.00	1293.0
77.00	353.0
77.90	151.0
78.90	907.0
79.90	328.0
80.90	1067.0
82.00	320.0
82.90	120.0
85.00	131.0
86.90	1373.0
87.90	1277.0
90.80	150.0
91.10	129.0
91.90	948.0
93.00	1259.0
94.00	3459.0
95.00	30304.0
96.00	2238.0
96.90	146.0
105.90	157.0
116.80	161.0
117.80	101.0
118.90	197.0
129.80	127.0
140.70	266.0
142.80	299.0
173.00	295.0
173.90	19128.0
174.90	1577.0
175.90	18824.0
176.90	1389.0
207.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	342.0
37.00	1589.0
38.00	1526.0
38.90	795.0
40.00	182.0
41.00	435.0
41.90	157.0
43.00	438.0
43.90	894.0
45.00	327.0
46.90	360.0
47.90	143.0
49.00	1381.0
50.00	5993.0
51.00	1791.0
52.90	128.0
53.90	119.0
55.00	423.0
56.00	804.0
57.00	1111.0
58.10	130.0
59.90	334.0
61.00	1572.0
62.00	1489.0
63.00	1201.0
66.90	245.0
68.00	3494.0
69.00	3738.0
70.00	339.0
70.90	170.0
71.90	192.0
73.00	1505.0
74.00	5395.0
75.00	15997.0
76.00	1348.0
77.00	338.0
77.90	174.0
78.90	954.0
79.90	336.0
80.90	1065.0
82.00	289.0
82.90	123.0
85.00	134.0
86.90	1549.0
87.90	1283.0
90.80	170.0
91.00	164.0
91.90	1006.0
93.00	1339.0
94.00	3810.0
95.00	32752.0
96.00	2388.0
96.90	147.0
97.90	113.0
103.90	103.0
105.90	167.0
116.80	151.0
117.80	114.0
118.90	202.0
127.80	103.0
129.80	157.0
140.70	283.0
142.80	310.0
147.80	106.0
173.00	285.0
173.90	21144.0
174.90	1757.0
175.90	20784.0
176.90	1457.0
207.00	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	353.0
37.00	1558.0
38.00	1481.0
38.90	860.0
40.00	179.0
41.00	415.0
41.90	180.0
42.90	411.0
43.90	847.0
45.00	273.0
46.90	309.0
47.90	197.0
49.00	1315.0
50.00	5769.0
51.00	1805.0
52.90	114.0
53.90	108.0
55.00	491.0
56.00	789.0
57.00	1112.0
58.10	126.0
59.90	342.0
61.00	1501.0
62.00	1503.0
63.00	1073.0
66.90	247.0
68.00	3405.0
69.00	3624.0
70.00	312.0
70.90	177.0
72.00	181.0
73.00	1526.0
74.00	5307.0
75.00	15713.0
76.00	1334.0
77.00	339.0
78.00	206.0
78.90	963.0
79.90	329.0
80.90	967.0
82.00	248.0
83.00	149.0
85.10	127.0
86.90	1475.0
87.90	1277.0
90.90	209.0
91.90	885.0
93.00	1329.0
94.00	3816.0
95.00	32152.0
96.00	2197.0
96.90	158.0
97.90	135.0
103.80	134.0
104.80	106.0
105.90	182.0
116.80	152.0
117.80	114.0
118.90	185.0
127.80	112.0
129.80	150.0
140.80	263.0
142.90	296.0
173.00	222.0
173.90	21424.0
174.90	1650.0
175.90	20696.0
176.90	1384.0
207.00	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86