


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101519\
 Data File : VV013156.D
 Acq On : 15 Oct 2019 09:24
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101119WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 15 18:13:27 2019

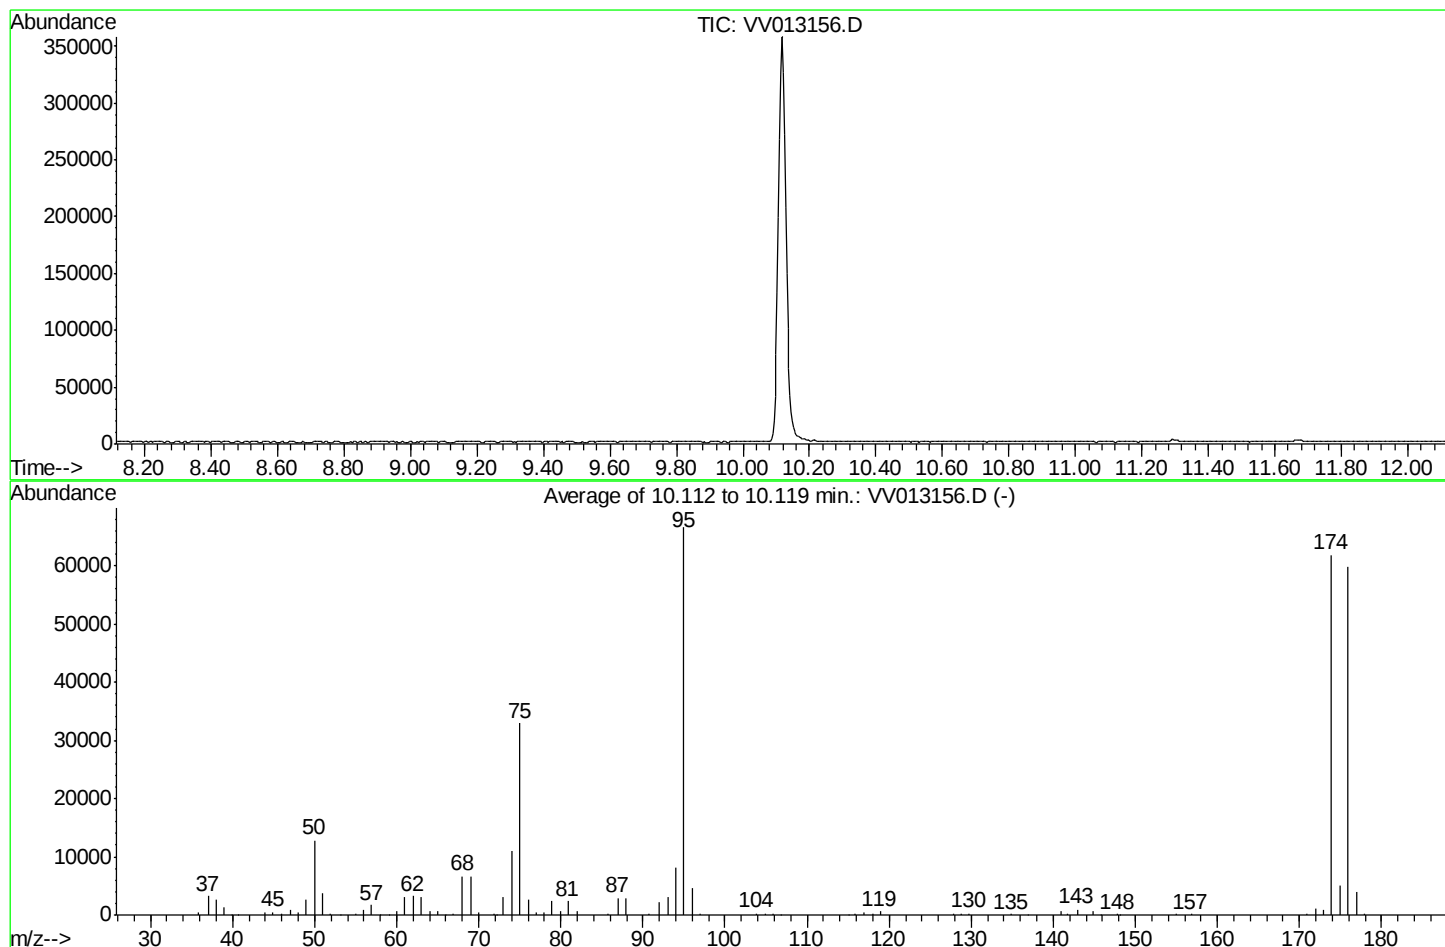

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	12772	PASS
75	95	30	80	49.4	32912	PASS
95	95	100	100	100.0	66597	PASS
96	95	5	9	7.1	4724	PASS
173	174	0.00	2	1.4	890	PASS
174	95	50	120	92.8	61797	PASS
175	174	5	9	8.2	5039	PASS
176	174	95	101	96.8	59810	PASS
177	176	5	9	6.5	3889	PASS

m/z	Abundance
35.90	574.0
37.00	3135.0
38.00	2672.0
39.00	1363.0
39.90	1037.0
44.00	1343.0
44.90	509.0
45.80	120.0
47.00	834.0
48.00	432.0
49.00	2447.0
50.00	12461.0
51.00	3656.0
52.00	224.0
53.20	147.0
55.00	277.0
56.00	901.0
56.90	1672.0
59.10	106.0
59.90	508.0
61.00	2811.0
62.00	3043.0
63.00	3153.0
64.00	559.0
65.00	599.0
66.80	131.0
68.00	6487.0
69.00	6229.0
70.00	474.0
71.90	306.0
73.00	2819.0
74.00	10533.0
75.00	31160.0
76.00	2474.0
77.00	466.0
78.00	326.0
78.90	2227.0
79.90	653.0
80.90	2312.0
81.90	625.0
85.80	124.0
87.00	2737.0
87.90	2620.0
90.80	210.0
92.00	1940.0
93.00	2908.0
94.00	7657.0
95.00	63264.0
96.00	4550.0
96.90	141.0
103.90	341.0
104.80	158.0
105.90	183.0
106.80	104.0
115.80	280.0
116.90	443.0
117.90	218.0
118.90	532.0
127.90	196.0
128.80	205.0
129.80	241.0
134.90	203.0
140.90	646.0
141.80	117.0
142.90	898.0
144.90	550.0
145.80	118.0
148.10	128.0
155.00	100.0
156.80	113.0
171.00	245.0
172.00	882.0
173.00	835.0
173.90	56472.0
174.90	4692.0
175.90	54632.0
176.90	3706.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	474.0
37.00	3283.0
38.00	2804.0
39.00	1369.0
40.00	1013.0
40.60	124.0
43.90	1566.0
44.90	563.0
45.90	137.0
47.00	890.0
47.90	534.0
49.00	2723.0
50.00	13224.0
51.00	3774.0
51.90	248.0
53.20	112.0
55.00	305.0
56.00	925.0
57.00	1800.0
58.10	112.0
60.00	588.0
61.00	3182.0
62.00	3295.0
63.00	3296.0
64.00	605.0
65.10	667.0
66.00	120.0
66.80	157.0
68.00	6882.0
69.00	6824.0
70.00	484.0
71.90	290.0
73.00	3138.0
74.00	11416.0
75.00	33928.0
76.00	2754.0
76.90	478.0
78.00	392.0
78.90	2501.0
80.00	716.0
80.90	2483.0
82.00	653.0
85.80	166.0
86.90	3020.0
87.90	2854.0
90.80	246.0
92.00	2202.0
93.00	3295.0
94.00	8351.0
95.00	68616.0
96.00	4833.0
97.00	144.0
103.90	331.0
104.90	170.0
105.90	209.0
106.80	110.0
115.00	113.0
115.90	333.0
116.90	479.0
118.00	270.0
118.90	607.0
127.90	230.0
128.80	195.0
129.70	292.0
134.90	173.0
140.90	671.0
141.70	131.0
142.90	1008.0
144.90	601.0
145.80	122.0
147.80	167.0
155.00	117.0
156.80	157.0
170.90	222.0
171.90	1045.0
173.00	938.0
173.90	63624.0
174.90	5238.0
175.90	61776.0
176.90	3991.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	410.0
37.00	3197.0
38.00	2713.0
39.00	1301.0
40.00	964.0
44.00	1552.0
44.90	562.0
46.00	169.0
47.00	847.0
47.90	499.0
49.00	2671.0
50.00	12633.0
51.00	3618.0
51.90	256.0
55.00	288.0
56.00	884.0
57.00	1744.0
58.00	126.0
60.00	669.0
61.00	3089.0
62.00	3290.0
63.00	3006.0
64.00	576.0
65.10	713.0
66.00	118.0
66.80	169.0
68.00	6775.0
69.00	6781.0
70.00	536.0
72.10	283.0
73.00	3162.0
74.00	11244.0
75.00	33648.0
76.00	2824.0
76.90	454.0
78.00	399.0
78.90	2598.0
80.00	723.0
80.90	2399.0
82.00	616.0
85.80	204.0
86.90	3044.0
87.90	2833.0
90.80	251.0
92.00	2229.0
93.00	3326.0
94.00	8323.0
95.00	67912.0
96.00	4789.0
97.00	162.0
103.90	315.0
104.80	178.0
105.90	225.0
106.80	103.0
115.00	140.0
115.90	311.0
116.90	482.0
118.00	278.0
118.90	633.0
127.90	229.0
128.80	172.0
129.70	316.0
134.90	125.0
136.90	111.0
140.90	592.0
141.70	152.0
142.90	1032.0
144.90	563.0
145.90	107.0
147.90	213.0
155.00	156.0
156.80	165.0
170.90	220.0
171.90	1151.0
173.00	898.0
173.90	65296.0
174.90	5189.0
175.90	63024.0
176.90	3970.0
177.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

Scan 2794 (10.074 min): VV013156.D
BFB73

m/z	Abundance
39.90	894.0
44.00	966.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73