

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018918.D
 Acq On : 15 Oct 2020 18:14
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	201164	203015	14.44%	1.933%
2	1.579	145	152	166	rVB	167181	187893	13.37%	1.789%
3	2.122	311	321	352	rVB	333235	514829	36.63%	4.901%
4	2.527	439	447	453	rBV5	2324	3187	0.23%	0.030%
5	2.794	528	530	535	rVB2	485	324	0.02%	0.003%
6	3.016	594	599	601	rBV2	357	265	0.02%	0.003%
7	3.032	602	604	605	rBV	251	99	0.01%	0.001%
8	3.064	610	614	619	rVV3	508	527	0.04%	0.005%
9	3.116	628	630	633	rVB2	408	191	0.01%	0.002%
10	3.383	711	713	716	rVB3	565	326	0.02%	0.003%
11	3.531	752	759	761	rBV2	504	523	0.04%	0.005%
12	3.547	762	764	767	rVV2	296	166	0.01%	0.002%
13	3.579	772	774	777	rVB2	504	254	0.02%	0.002%
14	3.605	779	782	783	rBV2	149	71	0.01%	0.001%
15	3.614	783	785	789	rBV3	314	225	0.02%	0.002%
16	3.672	800	803	805	rBV	329	244	0.02%	0.002%
17	3.743	823	825	826	rBV2	208	111	0.01%	0.001%
18	3.778	833	836	839	rBV2	271	242	0.02%	0.002%
19	3.875	864	866	867	rBV	206	83	0.01%	0.001%
20	3.910	867	877	914	rBV	96745	295806	21.04%	2.816%
21	4.376	1007	1022	1048	rVB	219927	537765	38.26%	5.120%
22	4.833	1159	1164	1167	rBV3	616	470	0.03%	0.004%
23	4.859	1167	1172	1173	rBV2	654	381	0.03%	0.004%
24	4.907	1185	1187	1190	rBV2	366	243	0.02%	0.002%
25	4.990	1211	1213	1215	rBV2	169	82	0.01%	0.001%
26	5.003	1215	1217	1220	rBV2	274	163	0.01%	0.002%
27	5.071	1220	1238	1265	rBV2	545321	1405630	100.00%	13.382%
28	5.559	1387	1390	1394	rBV2	406	290	0.02%	0.003%
29	5.595	1397	1401	1403	rBV2	628	382	0.03%	0.004%
30	5.640	1403	1415	1444	rBV	402072	812335	57.79%	7.734%
31	5.929	1493	1505	1530	rBV3	50712	112355	7.99%	1.070%
32	6.093	1542	1556	1580	rBV	321485	644060	45.82%	6.132%
33	6.357	1635	1638	1642	rVB3	459	267	0.02%	0.003%
34	6.376	1642	1644	1645	rBV3	314	108	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018918.D
 Acq On : 15 Oct 2020 18:14
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.424	1657	1659	1663	rBV3	323	210	0.01%	0.002%
36	6.495	1679	1681	1684	rBV	272	157	0.01%	0.001%
37	6.518	1686	1688	1689	rBV	290	94	0.01%	0.001%
38	6.572	1704	1705	1708	rBV2	270	96	0.01%	0.001%
39	6.768	1762	1766	1770	rBV3	517	456	0.03%	0.004%
40	6.923	1812	1814	1816	rVB	155	61	0.00%	0.001%
41	6.955	1821	1824	1828	rBV2	340	274	0.02%	0.003%
42	7.006	1828	1840	1864	rBV	169795	308455	21.94%	2.937%
43	7.338	1928	1943	1971	rBV	633931	1089480	77.51%	10.372%
44	7.643	2027	2038	2073	rBV	121491	217259	15.46%	2.068%
45	7.929	2121	2127	2128	rBV2	371	319	0.02%	0.003%
46	8.000	2139	2149	2164	rVB2	24265	41314	2.94%	0.393%
47	8.064	2166	2169	2171	rBV2	469	251	0.02%	0.002%
48	8.109	2173	2183	2226	rBV2	304899	636763	45.30%	6.062%
49	8.730	2373	2376	2378	rBV3	253	165	0.01%	0.002%
50	8.784	2390	2393	2394	rBV2	460	245	0.02%	0.002%
51	8.871	2406	2420	2449	rBV	633062	1023114	72.79%	9.740%
52	9.096	2485	2490	2494	rVB5	924	1087	0.08%	0.010%
53	9.122	2494	2498	2501	rBV3	625	559	0.04%	0.005%
54	9.376	2574	2577	2581	rBV2	460	317	0.02%	0.003%
55	9.550	2629	2631	2633	rVB	175	75	0.01%	0.001%
56	9.582	2634	2641	2644	rBV3	497	642	0.05%	0.006%
57	9.627	2653	2655	2656	rBV	154	71	0.01%	0.001%
58	9.759	2692	2696	2697	rBV2	358	216	0.02%	0.002%
59	9.781	2701	2703	2707	rVB	531	282	0.02%	0.003%
60	9.817	2709	2714	2716	rBV	540	444	0.03%	0.004%
61	9.887	2733	2736	2740	rVB3	564	456	0.03%	0.004%
62	9.907	2740	2742	2743	rBV3	537	226	0.02%	0.002%
63	9.952	2751	2756	2761	rVB3	511	492	0.04%	0.005%
64	10.035	2779	2782	2785	rVB	405	247	0.02%	0.002%
65	10.087	2796	2798	2799	rBV	257	101	0.01%	0.001%
66	10.138	2812	2814	2815	rBV	235	98	0.01%	0.001%
67	10.238	2832	2845	2865	rBV	322597	518719	36.90%	4.938%
68	10.466	2912	2916	2918	rBV2	377	330	0.02%	0.003%
69	10.508	2926	2929	2932	rBV	384	251	0.02%	0.002%
70	10.617	2961	2963	2965	rBV	281	135	0.01%	0.001%
71	10.823	3020	3027	3030	rBV2	651	758	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018918.D
Acq On : 15 Oct 2020 18:14
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	11.080	3103	3107	3111	rBV2	517	426	0.03%	0.004%
73	11.215	3147	3149	3152	rBV2	408	256	0.02%	0.002%
74	11.270	3155	3166	3188	rBV	605293	935173	66.53%	8.903%
75	11.646	3271	3283	3306	rBV	634160	999389	71.10%	9.514%
76	12.222	3458	3462	3466	rBV3	637	657	0.05%	0.006%
77	12.386	3511	3513	3518	rBV2	433	271	0.02%	0.003%
78	12.456	3533	3535	3539	rBV2	479	262	0.02%	0.002%
79	12.771	3630	3633	3636	rBV2	496	308	0.02%	0.003%


Sum of corrected areas: 10503873

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018918.D
Acq On : 15 Oct 2020 18:14
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

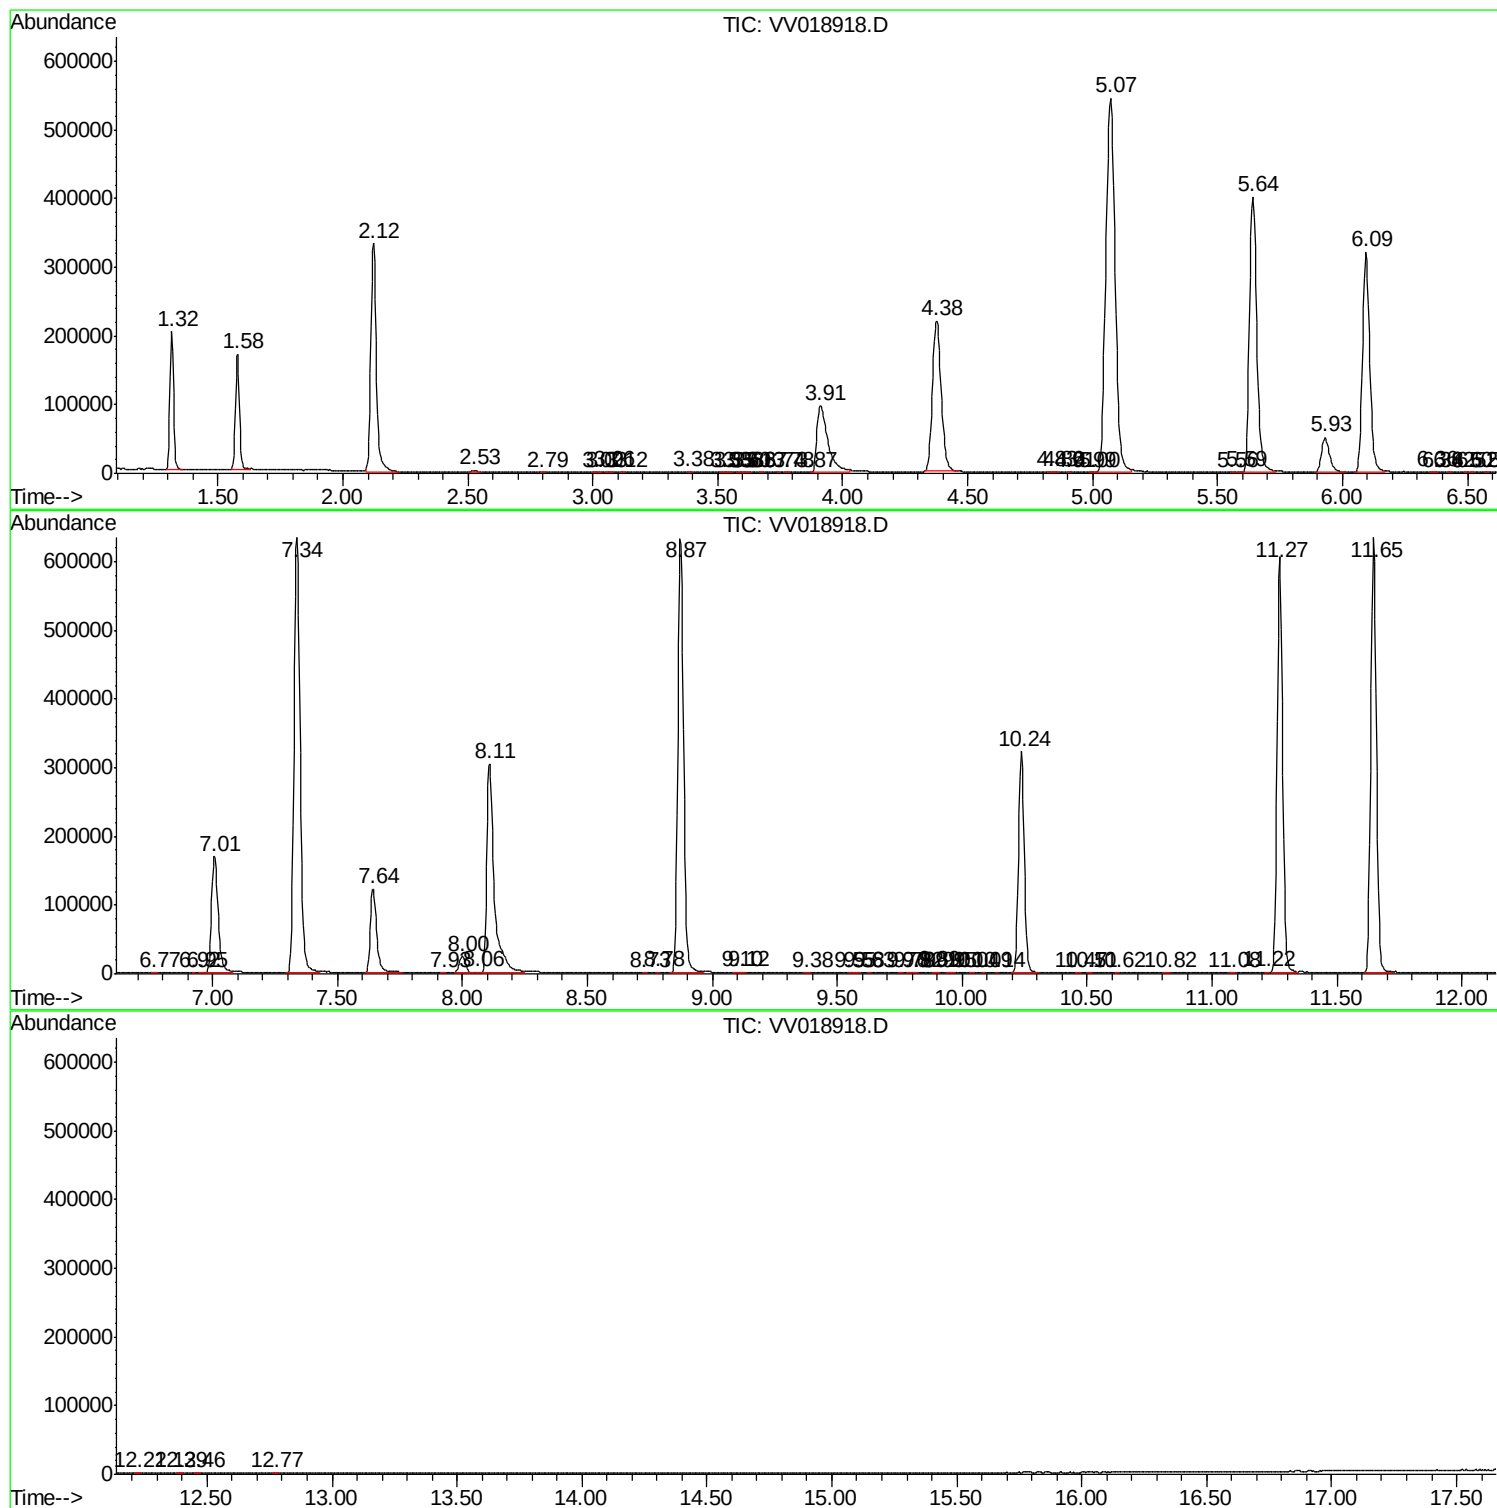

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018918.D
Acq On : 15 Oct 2020 18:14
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101520\
Data File : VV018918.D
Acq On : 15 Oct 2020 18:14
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc