

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018920.D
 Acq On : 15 Oct 2020 19:01
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rBV	199361	200899	14.30%	1.926%
2	1.579	145	152	164	rVB	159728	183814	13.09%	1.762%
3	2.122	311	321	351	rVB	328986	506874	36.09%	4.859%
4	2.376	396	400	403	rBV2	610	411	0.03%	0.004%
5	2.528	438	447	455	rBV6	2592	4462	0.32%	0.043%
6	2.692	496	498	503	rVB3	497	310	0.02%	0.003%
7	2.897	555	562	565	rBV2	534	652	0.05%	0.006%
8	2.965	581	583	586	rVB	326	133	0.01%	0.001%
9	2.981	586	588	590	rBV2	359	146	0.01%	0.001%
10	3.039	605	606	610	rBV	306	159	0.01%	0.002%
11	3.100	622	625	631	rVB3	351	239	0.02%	0.002%
12	3.135	633	636	639	rBV	405	250	0.02%	0.002%
13	3.184	647	651	653	rBV2	355	192	0.01%	0.002%
14	3.238	663	668	670	rBV2	551	444	0.03%	0.004%
15	3.280	680	681	684	rBV	177	77	0.01%	0.001%
16	3.296	684	686	688	rBV	292	140	0.01%	0.001%
17	3.547	761	764	767	rBV2	262	203	0.01%	0.002%
18	3.640	792	793	795	rBV2	183	74	0.01%	0.001%
19	3.733	817	822	826	rBV2	357	455	0.03%	0.004%
20	3.791	837	840	843	rBV2	340	209	0.01%	0.002%
21	3.913	867	878	917	rBV	94993	299965	21.36%	2.875%
22	4.376	1007	1022	1045	rBV	217069	536891	38.23%	5.146%
23	4.601	1089	1092	1094	rBV2	671	401	0.03%	0.004%
24	4.650	1105	1107	1110	rBV2	630	445	0.03%	0.004%
25	4.817	1157	1159	1161	rBV	557	254	0.02%	0.002%
26	4.897	1182	1184	1185	rBV	476	212	0.02%	0.002%
27	5.071	1221	1238	1269	rBV2	546966	1404398	100.00%	13.462%
28	5.351	1321	1325	1326	rBV2	607	399	0.03%	0.004%
29	5.421	1344	1347	1352	rBV4	762	828	0.06%	0.008%
30	5.544	1382	1385	1389	rVB2	549	382	0.03%	0.004%
31	5.640	1403	1415	1450	rBV	403457	810406	57.70%	7.768%
32	5.929	1492	1505	1528	rBV	46040	98812	7.04%	0.947%
33	6.093	1542	1556	1586	rBV	318040	643398	45.81%	6.167%
34	6.476	1671	1675	1678	rVB	601	409	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018920.D
 Acq On : 15 Oct 2020 19:01
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.495	1678	1681	1682	rBV	242	147	0.01%	0.001%
36	6.534	1692	1693	1697	rVB	321	83	0.01%	0.001%
37	6.556	1697	1700	1702	rBV2	215	135	0.01%	0.001%
38	6.662	1731	1733	1735	rBV	357	147	0.01%	0.001%
39	6.675	1735	1737	1739	rVV2	549	257	0.02%	0.002%
40	6.753	1760	1761	1764	rBV2	169	114	0.01%	0.001%
41	6.772	1764	1767	1769	rBV2	457	307	0.02%	0.003%
42	6.830	1784	1785	1793	rVB	583	648	0.05%	0.006%
43	6.868	1793	1797	1799	rBV2	470	344	0.02%	0.003%
44	6.933	1813	1817	1822	rVB2	363	294	0.02%	0.003%
45	7.007	1829	1840	1867	rBV	168586	307844	21.92%	2.951%
46	7.338	1931	1943	1968	rBV	634888	1081533	77.01%	10.367%
47	7.643	2028	2038	2064	rBV	118958	212127	15.10%	2.033%
48	7.878	2109	2111	2115	rBV2	364	276	0.02%	0.003%
49	7.920	2122	2124	2127	rBV2	511	280	0.02%	0.003%
50	8.003	2141	2150	2160	rVB6	6145	10965	0.78%	0.105%
51	8.109	2172	2183	2221	rBV2	307890	634779	45.20%	6.085%
52	8.669	2355	2357	2360	rBV	434	336	0.02%	0.003%
53	8.791	2392	2395	2396	rBV	195	108	0.01%	0.001%
54	8.871	2408	2420	2450	rBV	626743	1023049	72.85%	9.806%
55	9.106	2491	2493	2498	rVB3	646	460	0.03%	0.004%
56	9.129	2498	2500	2504	rBV3	584	336	0.02%	0.003%
57	9.151	2504	2507	2508	rBV	488	251	0.02%	0.002%
58	9.235	2531	2533	2538	rBV2	336	233	0.02%	0.002%
59	9.260	2539	2541	2546	rBV3	368	248	0.02%	0.002%
60	9.322	2558	2560	2565	rBV2	399	325	0.02%	0.003%
61	9.518	2619	2621	2625	rVB	365	242	0.02%	0.002%
62	9.534	2625	2626	2628	rBV	277	151	0.01%	0.001%
63	9.640	2656	2659	2660	rBV2	476	274	0.02%	0.003%
64	9.749	2691	2693	2695	rBV	230	101	0.01%	0.001%
65	9.781	2700	2703	2705	rBV2	434	281	0.02%	0.003%
66	9.810	2710	2712	2719	rVB2	520	431	0.03%	0.004%
67	9.884	2730	2735	2737	rBV3	324	331	0.02%	0.003%
68	9.939	2746	2752	2756	rBV3	622	648	0.05%	0.006%
69	10.238	2833	2845	2868	rBV	335105	517794	36.87%	4.963%
70	10.405	2895	2897	2898	rBV	270	83	0.01%	0.001%
71	10.553	2939	2943	2946	rBV2	357	368	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018920.D
Acq On : 15 Oct 2020 19:01
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.685	2980	2984	2986	rBV2	528	432	0.03%	0.004%
73	10.929	3058	3060	3063	rVB	325	170	0.01%	0.002%
74	10.948	3063	3066	3069	rBV2	405	319	0.02%	0.003%
75	11.270	3155	3166	3192	rBV	618469	939581	66.90%	9.006%
76	11.646	3271	3283	3310	rBV	644829	996261	70.94%	9.549%
77	11.829	3338	3340	3344	rBV4	442	355	0.03%	0.003%
78	11.868	3349	3352	3355	rBV2	638	562	0.04%	0.005%
79	12.508	3548	3551	3553	rBV2	542	285	0.02%	0.003%
80	13.325	3802	3805	3810	rVB2	565	418	0.03%	0.004%
81	14.193	4072	4075	4078	rBV2	751	594	0.04%	0.006%


Sum of corrected areas: 10432650

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV018920\
Data File : VV018920.D
Acq On : 15 Oct 2020 19:01
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

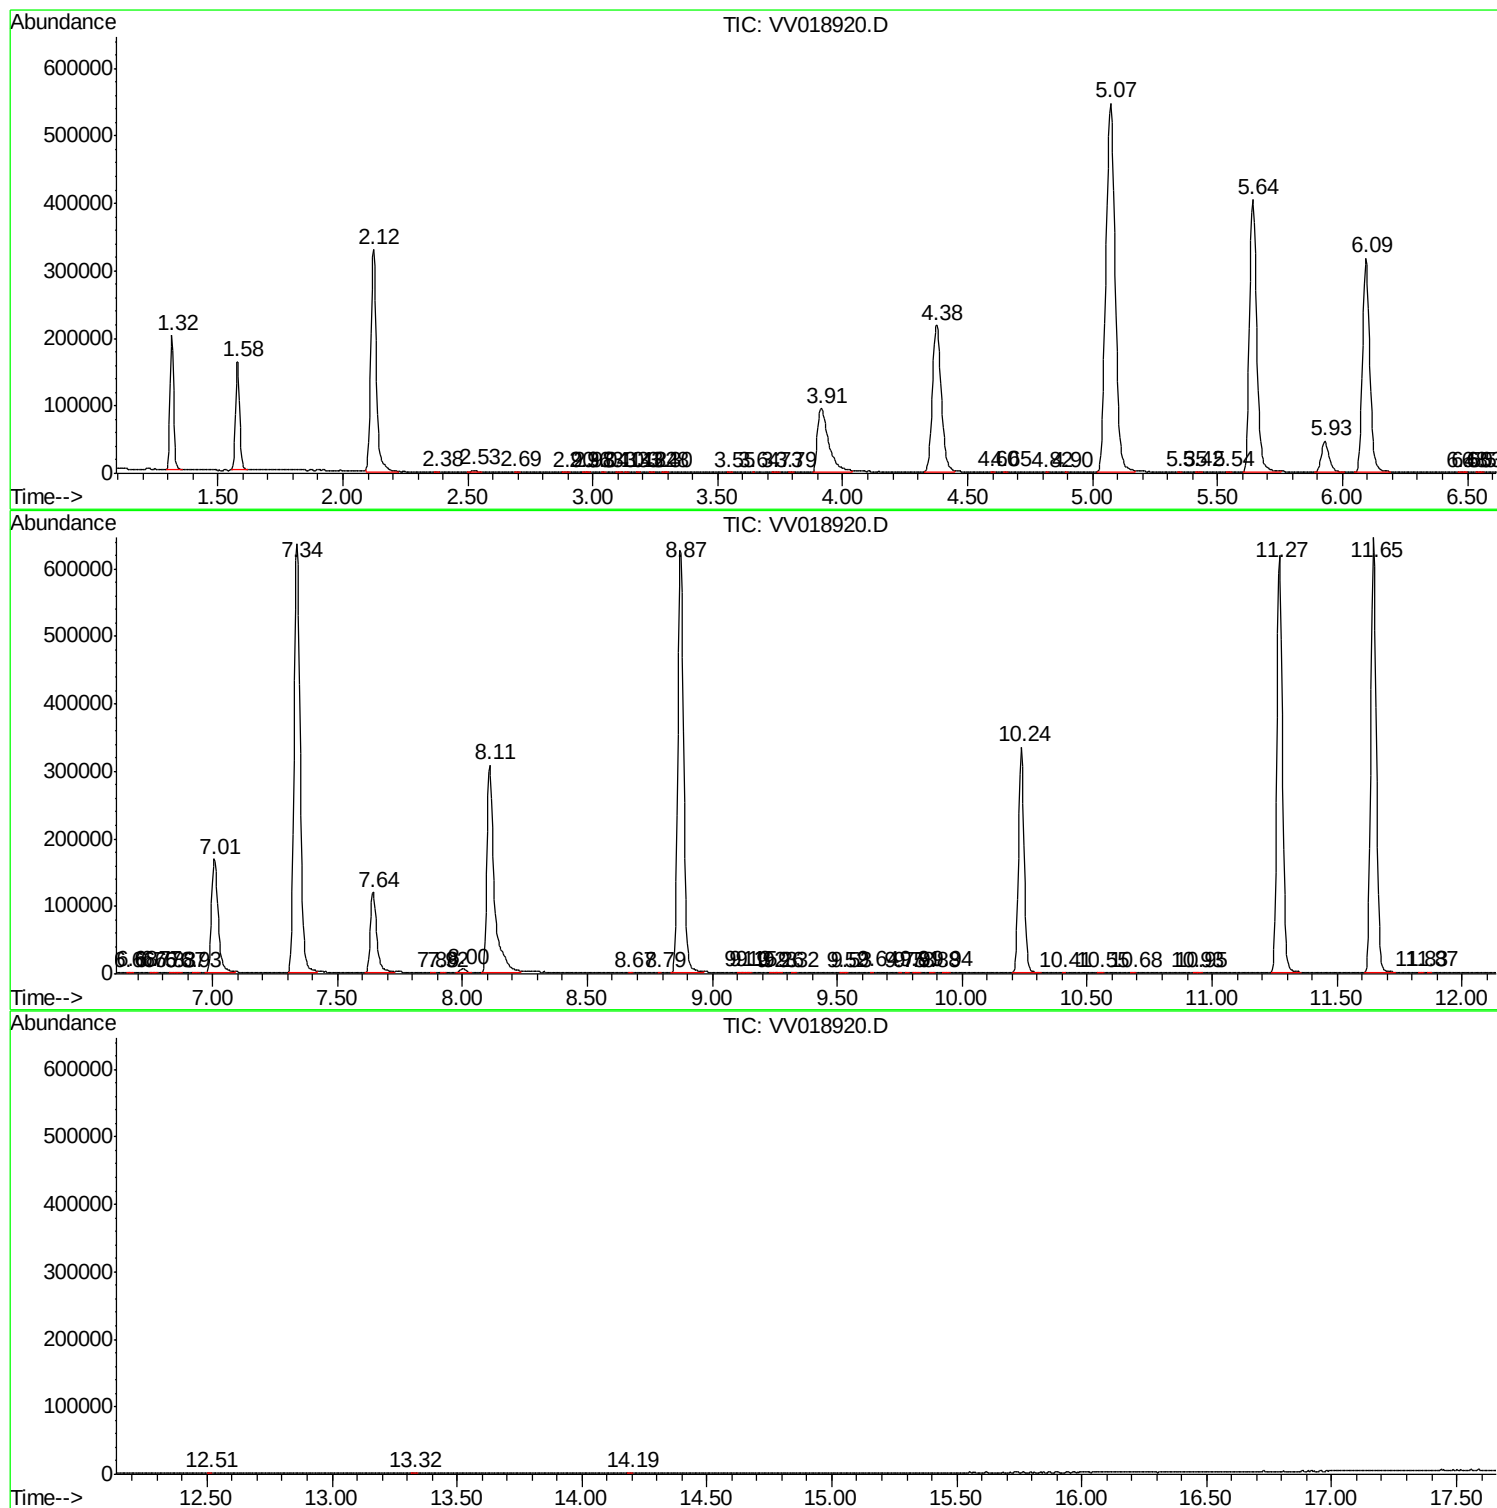

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018920.D
Acq On : 15 Oct 2020 19:01
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018920.D
Acq On : 15 Oct 2020 19:01
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc