

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018923.D
 Acq On : 15 Oct 2020 20:12
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	205897	208710	14.82%	1.999%
2	1.579	145	152	167	rVB	171343	192290	13.65%	1.842%
3	2.123	311	321	344	rBV	334633	502791	35.70%	4.817%
4	2.643	480	483	487	rBV	532	357	0.03%	0.003%
5	2.766	519	521	523	rVB2	340	102	0.01%	0.001%
6	2.791	527	529	532	rBV	302	194	0.01%	0.002%
7	2.814	532	536	539	rBV2	451	382	0.03%	0.004%
8	2.930	570	572	574	rBV	350	220	0.02%	0.002%
9	3.029	600	603	607	rBV3	471	399	0.03%	0.004%
10	3.077	615	618	620	rVB	636	335	0.02%	0.003%
11	3.261	670	675	679	rVB4	376	399	0.03%	0.004%
12	3.290	681	684	686	rVB2	318	195	0.01%	0.002%
13	3.306	686	689	690	rBV2	226	93	0.01%	0.001%
14	3.335	695	698	700	rBV2	313	186	0.01%	0.002%
15	3.348	700	702	704	rVV2	359	137	0.01%	0.001%
16	3.431	724	728	731	rBV3	422	401	0.03%	0.004%
17	3.479	741	743	747	rVB	318	111	0.01%	0.001%
18	3.540	759	762	763	rBV2	191	130	0.01%	0.001%
19	3.586	773	776	777	rBV	369	217	0.02%	0.002%
20	3.627	785	789	792	rBV2	481	340	0.02%	0.003%
21	3.666	799	801	804	rVB2	369	165	0.01%	0.002%
22	3.685	804	807	809	rBV	235	171	0.01%	0.002%
23	3.698	809	811	814	rVB	263	158	0.01%	0.002%
24	3.717	815	817	819	rVV2	296	83	0.01%	0.001%
25	3.775	833	835	836	rBV2	100	44	0.00%	0.000%
26	3.785	836	838	839	rBV2	183	95	0.01%	0.001%
27	3.820	847	849	851	rVB	253	75	0.01%	0.001%
28	3.878	863	867	868	rBV	403	241	0.02%	0.002%
29	3.913	868	878	911	rBV	89817	278109	19.74%	2.664%
30	4.376	1005	1022	1053	rBV	220603	549260	39.00%	5.262%
31	4.557	1075	1078	1080	rBV	454	327	0.02%	0.003%
32	4.721	1127	1129	1132	rBV4	307	149	0.01%	0.001%
33	4.846	1165	1168	1171	rVB	403	236	0.02%	0.002%
34	4.878	1175	1178	1179	rBV2	476	204	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018923.D
 Acq On : 15 Oct 2020 20:12
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	4.907	1185	1187	1188	rBV2	165	58	0.00%	0.001%
36	4.923	1190	1192	1193	rBV	219	75	0.01%	0.001%
37	5.071	1221	1238	1269	rBV2	549487	1408525	100.00%	13.494%
38	5.457	1353	1358	1361	rBV3	444	341	0.02%	0.003%
39	5.476	1361	1364	1368	rBV2	491	384	0.03%	0.004%
40	5.550	1384	1387	1390	rBV2	632	407	0.03%	0.004%
41	5.579	1394	1396	1397	rBV	281	139	0.01%	0.001%
42	5.640	1403	1415	1441	rBV	409231	813667	57.77%	7.795%
43	5.926	1493	1504	1525	rBV	55835	116663	8.28%	1.118%
44	6.093	1543	1556	1577	rBV	317410	641507	45.54%	6.146%
45	6.447	1662	1666	1670	rBV2	478	433	0.03%	0.004%
46	6.495	1678	1681	1683	rBV3	423	313	0.02%	0.003%
47	6.566	1701	1703	1704	rBV	512	230	0.02%	0.002%
48	6.595	1711	1712	1714	rVB	354	112	0.01%	0.001%
49	6.643	1724	1727	1728	rBV2	199	103	0.01%	0.001%
50	6.785	1766	1771	1776	rVB	495	402	0.03%	0.004%
51	6.807	1776	1778	1779	rBV	197	105	0.01%	0.001%
52	6.868	1792	1797	1798	rBV	208	160	0.01%	0.002%
53	6.926	1812	1815	1817	rBV2	351	241	0.02%	0.002%
54	7.007	1829	1840	1860	rBV	166358	303597	21.55%	2.908%
55	7.338	1931	1943	1962	rBV	641027	1093478	77.63%	10.475%
56	7.640	2028	2037	2062	rBV	118567	210447	14.94%	2.016%
57	7.949	2131	2133	2138	rBV3	442	330	0.02%	0.003%
58	8.003	2141	2150	2160	rVB4	3742	5952	0.42%	0.057%
59	8.109	2172	2183	2227	rBV2	287574	631916	44.86%	6.054%
60	8.637	2345	2347	2351	rVB2	702	433	0.03%	0.004%
61	8.720	2370	2373	2376	rBV	377	210	0.01%	0.002%
62	8.778	2388	2391	2394	rBV3	379	250	0.02%	0.002%
63	8.871	2408	2420	2448	rBV	629856	1027971	72.98%	9.848%
64	9.125	2497	2499	2500	rBV2	232	94	0.01%	0.001%
65	9.158	2507	2509	2513	rVB3	510	266	0.02%	0.003%
66	9.174	2513	2514	2516	rBV3	338	134	0.01%	0.001%
67	9.450	2597	2600	2604	rBV3	385	313	0.02%	0.003%
68	9.572	2631	2638	2640	rBV3	588	637	0.05%	0.006%
69	9.630	2649	2656	2660	rBV	257	305	0.02%	0.003%
70	9.662	2664	2666	2670	rBV2	327	237	0.02%	0.002%
71	9.714	2679	2682	2683	rBV	307	196	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018923.D
 Acq On : 15 Oct 2020 20:12
 Operator : SY/MD
 Sample : L4382-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG409

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.791	2703	2706	2707	rBV	227	130	0.01%	0.001%
73	9.932	2746	2750	2751	rBV	391	257	0.02%	0.002%
74	9.949	2754	2755	2759	rVB	490	163	0.01%	0.002%
75	9.971	2760	2762	2770	rVB3	541	637	0.05%	0.006%
76	10.006	2770	2773	2777	rBV3	238	206	0.01%	0.002%
77	10.035	2777	2782	2784	rBV3	494	475	0.03%	0.005%
78	10.132	2809	2812	2814	rBV	318	185	0.01%	0.002%
79	10.170	2822	2824	2826	rBV3	225	117	0.01%	0.001%
80	10.235	2832	2844	2872	rVB	303703	480742	34.13%	4.605%
81	10.338	2873	2876	2882	rBV4	438	456	0.03%	0.004%
82	10.408	2888	2898	2900	rBV3	943	1382	0.10%	0.013%
83	10.441	2906	2908	2912	rBV3	544	420	0.03%	0.004%
84	10.643	2969	2971	2973	rBV	273	145	0.01%	0.001%
85	10.704	2989	2990	2996	rVB	308	172	0.01%	0.002%
86	10.775	3009	3012	3015	rBV	367	192	0.01%	0.002%
87	11.016	3084	3087	3089	rBV	400	243	0.02%	0.002%
88	11.084	3104	3108	3111	rBV3	571	379	0.03%	0.004%
89	11.270	3154	3166	3191	rBV	620366	947466	67.27%	9.077%
90	11.569	3254	3259	3262	rBV4	731	842	0.06%	0.008%
91	11.646	3271	3283	3301	rBV	648826	1004783	71.34%	9.626%
92	11.926	3366	3370	3373	rBV	603	531	0.04%	0.005%
93	13.569	3879	3881	3883	rBV	525	244	0.02%	0.002%
94	13.804	3950	3954	3956	rBV2	466	339	0.02%	0.003%


Sum of corrected areas: 10438443

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018923.D
Acq On : 15 Oct 2020 20:12
Operator : SY/MD
Sample : L4382-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG409

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

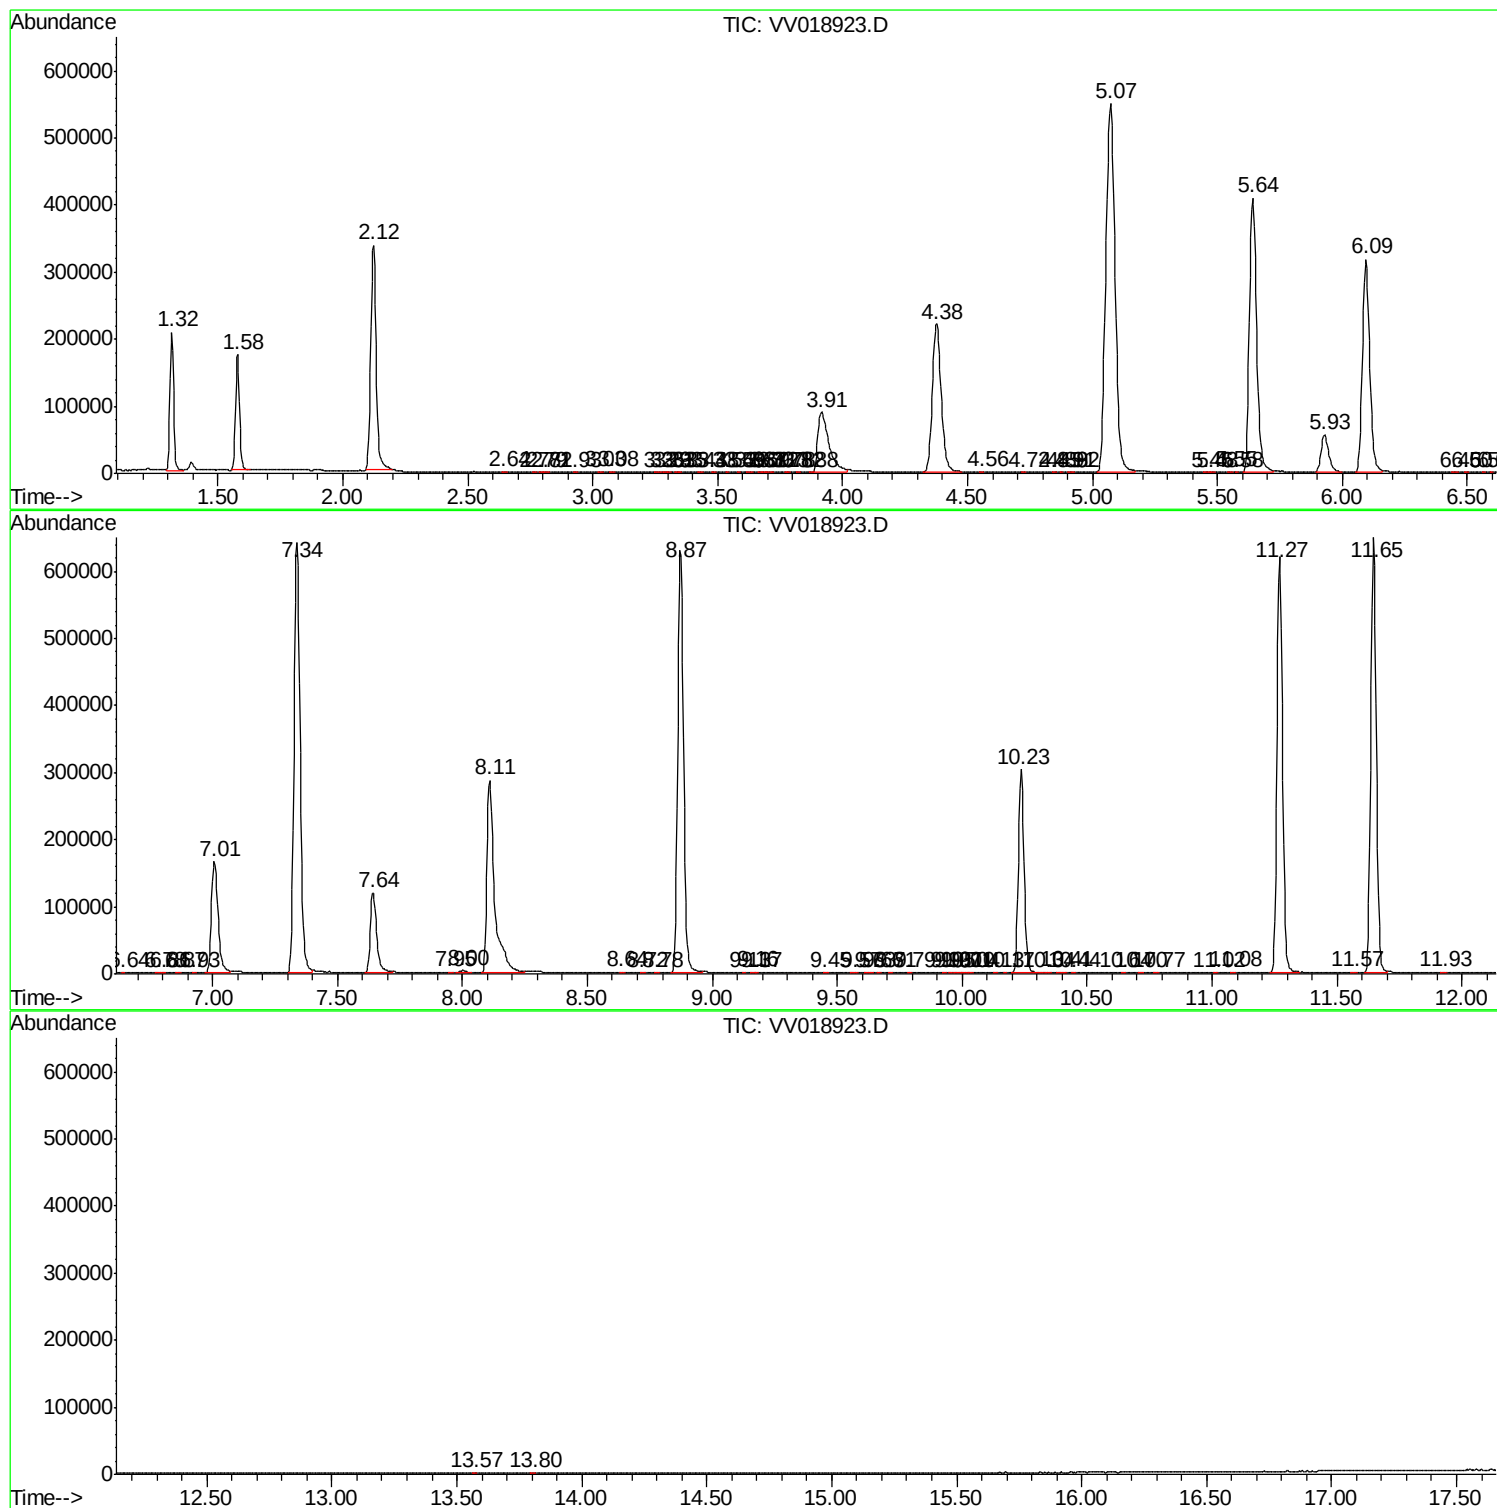

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018923.D
Acq On : 15 Oct 2020 20:12
Operator : SY/MD
Sample : L4382-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG409

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018923.D
Acq On : 15 Oct 2020 20:12
Operator : SY/MD
Sample : L4382-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG409

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc