

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018928.D
 Acq On : 15 Oct 2020 22:10
 Operator : SY/MD
 Sample : L4382-15 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	204794	199631	3.35%	1.247%
2	1.579	144	152	164	rBV	165454	186783	3.13%	1.167%
3	2.122	311	321	351	rVB	317895	491863	8.25%	3.073%
4	2.527	439	447	459	rBV4	2530	3802	0.06%	0.024%
5	2.704	500	502	506	rBV2	343	234	0.00%	0.001%
6	2.936	571	574	576	rBV2	186	135	0.00%	0.001%
7	2.987	588	590	591	rBV	224	68	0.00%	0.000%
8	3.010	595	597	598	rBV	267	101	0.00%	0.001%
9	3.042	605	607	609	rBV	193	94	0.00%	0.001%
10	3.074	615	617	622	rVB3	518	412	0.01%	0.003%
11	3.216	656	661	663	rBV	355	388	0.01%	0.002%
12	3.254	668	673	679	rBV3	469	563	0.01%	0.004%
13	3.354	697	704	706	rBV2	460	509	0.01%	0.003%
14	3.415	720	723	729	rBV2	356	308	0.01%	0.002%
15	3.466	736	739	741	rVB2	369	207	0.00%	0.001%
16	3.486	742	745	750	rVV3	412	251	0.00%	0.002%
17	3.508	750	752	757	rVB2	302	234	0.00%	0.001%
18	3.540	758	762	768	rBV2	364	330	0.01%	0.002%
19	3.585	774	776	779	rBV2	231	179	0.00%	0.001%
20	3.611	782	784	786	rVB	204	84	0.00%	0.001%
21	3.624	786	788	792	rVB2	311	148	0.00%	0.001%
22	3.656	796	798	801	rBV3	251	183	0.00%	0.001%
23	3.720	814	818	821	rBV2	368	269	0.00%	0.002%
24	3.743	823	825	829	rBV2	332	236	0.00%	0.001%
25	3.765	829	832	835	rBV2	282	213	0.00%	0.001%
26	3.830	846	852	855	rBV3	349	386	0.01%	0.002%
27	3.865	859	863	865	rBV	365	246	0.00%	0.002%
28	3.916	868	879	914	rBV	91656	288664	4.84%	1.804%
29	4.376	1005	1022	1051	rBV	208513	522000	8.76%	3.262%
30	4.746	1135	1137	1138	rBV	217	85	0.00%	0.001%
31	4.775	1143	1146	1148	rVV2	328	248	0.00%	0.002%
32	4.801	1151	1154	1162	rVB2	377	482	0.01%	0.003%
33	4.849	1162	1169	1170	rBV	370	342	0.01%	0.002%
34	4.875	1174	1177	1179	rBV2	370	195	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018928.D
 Acq On : 15 Oct 2020 22:10
 Operator : SY/MD
 Sample : L4382-15 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	4.891	1179	1182	1184	rBV2	266	167	0.00%	0.001%
36	4.949	1197	1200	1202	rBV2	397	263	0.00%	0.002%
37	4.984	1209	1211	1213	rBV2	224	112	0.00%	0.001%
38	5.071	1221	1238	1274	rBV2	512302	1323165	22.20%	8.268%
39	5.293	1305	1307	1312	rBV2	573	516	0.01%	0.003%
40	5.402	1337	1341	1344	rBV3	496	436	0.01%	0.003%
41	5.492	1365	1369	1372	rBV3	404	397	0.01%	0.002%
42	5.540	1382	1384	1387	rVB2	242	93	0.00%	0.001%
43	5.595	1398	1401	1402	rBV	201	101	0.00%	0.001%
44	5.640	1402	1415	1443	rBV	378706	760373	12.75%	4.751%
45	5.932	1493	1506	1526	rBV3	64142	148294	2.49%	0.927%
46	6.093	1541	1556	1583	rBV	308059	617313	10.36%	3.857%
47	6.318	1623	1626	1628	rVB2	691	371	0.01%	0.002%
48	6.341	1628	1633	1638	rVB4	546	476	0.01%	0.003%
49	6.363	1638	1640	1644	rBV3	245	176	0.00%	0.001%
50	6.457	1665	1669	1671	rBV2	420	321	0.01%	0.002%
51	6.495	1680	1681	1682	rVB2	278	54	0.00%	0.000%
52	6.505	1682	1684	1686	rBV2	163	55	0.00%	0.000%
53	6.521	1687	1689	1691	rBV	195	119	0.00%	0.001%
54	6.624	1716	1721	1723	rBV2	396	304	0.01%	0.002%
55	6.672	1733	1736	1737	rBV	362	217	0.00%	0.001%
56	6.691	1740	1742	1745	rVB3	413	168	0.00%	0.001%
57	6.736	1753	1756	1757	rBV	382	215	0.00%	0.001%
58	6.830	1783	1785	1786	rBV	166	63	0.00%	0.000%
59	6.904	1803	1808	1811	rBV2	467	450	0.01%	0.003%
60	7.006	1829	1840	1873	rBV	160786	295414	4.96%	1.846%
61	7.338	1931	1943	1965	rBV	602157	1034831	17.36%	6.466%
62	7.643	2028	2038	2063	rBV2	114427	204865	3.44%	1.280%
63	7.910	2116	2121	2123	rBV2	542	469	0.01%	0.003%
64	7.997	2134	2148	2173	rBV	3584113	5961418	100.00%	37.249%
65	8.109	2174	2183	2224	rVB2	313490	639053	10.72%	3.993%
66	8.801	2397	2398	2399	rBV2	428	111	0.00%	0.001%
67	8.871	2409	2420	2445	rBV	591135	971983	16.30%	6.073%
68	9.174	2511	2514	2515	rBV2	429	240	0.00%	0.001%
69	9.415	2586	2589	2590	rBV	530	275	0.00%	0.002%
70	9.514	2616	2620	2624	rBV3	436	377	0.01%	0.002%
71	9.566	2634	2636	2637	rBV	348	158	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018928.D
 Acq On : 15 Oct 2020 22:10
 Operator : SY/MD
 Sample : L4382-15 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.723	2682	2685	2689	rBV	342	268	0.00%	0.002%
73	9.772	2698	2700	2704	rVB2	292	137	0.00%	0.001%
74	9.820	2713	2715	2718	rVB2	263	127	0.00%	0.001%
75	9.887	2733	2736	2738	rBV	272	182	0.00%	0.001%
76	10.141	2813	2815	2821	rVB	656	474	0.01%	0.003%
77	10.167	2821	2823	2825	rBV3	184	107	0.00%	0.001%
78	10.238	2833	2845	2865	rBV	318568	499544	8.38%	3.121%
79	10.521	2931	2933	2935	rBV	259	119	0.00%	0.001%
80	10.582	2949	2952	2955	rBV3	334	216	0.00%	0.001%
81	10.636	2967	2969	2971	rVB	351	106	0.00%	0.001%
82	10.865	3036	3040	3042	rBV	333	245	0.00%	0.002%
83	10.942	3062	3064	3069	rBV2	570	459	0.01%	0.003%
84	10.990	3076	3079	3081	rBV2	313	227	0.00%	0.001%
85	11.206	3144	3146	3152	rVB	566	381	0.01%	0.002%
86	11.270	3154	3166	3190	rBV	581097	893263	14.98%	5.581%
87	11.646	3271	3283	3307	rBV	612392	943488	15.83%	5.895%
88	12.540	3558	3561	3562	rBV	477	270	0.00%	0.002%
89	13.964	3999	4004	4011	rBV4	562	877	0.01%	0.005%
90	14.369	4127	4130	4134	rBV2	732	630	0.01%	0.004%


Sum of corrected areas: 16004406

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018928.D
Acq On : 15 Oct 2020 22:10
Operator : SY/MD
Sample : L4382-15 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

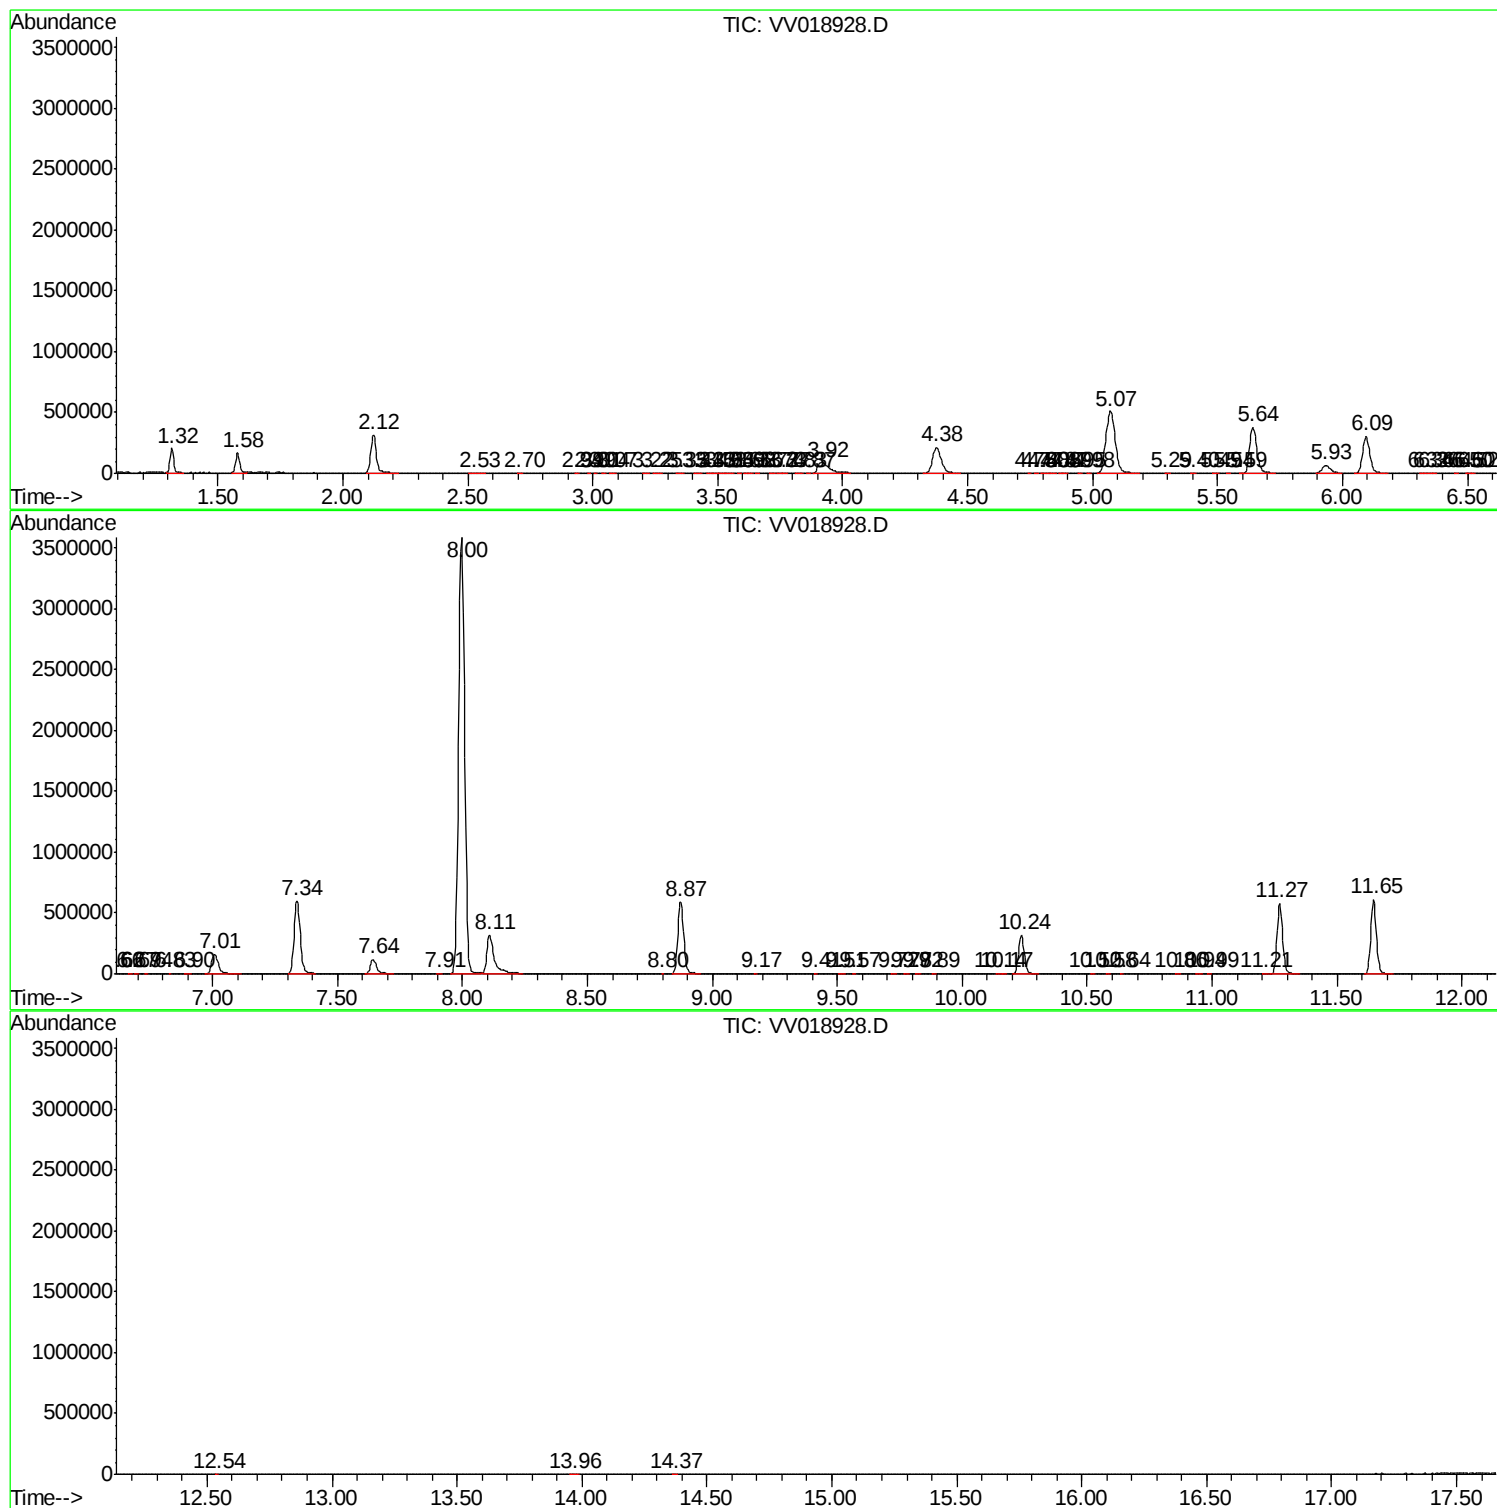

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018928.D
Acq On : 15 Oct 2020 22:10
Operator : SY/MD
Sample : L4382-15 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018928.D
Acq On : 15 Oct 2020 22:10
Operator : SY/MD
Sample : L4382-15 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc