

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018931.D
 Acq On : 15 Oct 2020 23:21
 Operator : SY/MD
 Sample : L4382-14 40X
 Misc : 5.51µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Y2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	194636	195278	15.62%	2.033%
2	1.579	144	152	164	rBV	164732	185474	14.84%	1.931%
3	2.122	311	321	350	rVB	318037	491295	39.31%	5.114%
4	2.399	404	407	412	rVB3	738	677	0.05%	0.007%
5	2.933	565	573	574	rBV2	515	593	0.05%	0.006%
6	3.190	646	653	655	rBV2	295	375	0.03%	0.004%
7	3.306	685	689	691	rBV2	503	285	0.02%	0.003%
8	3.479	740	743	744	rBV	270	135	0.01%	0.001%
9	3.675	801	804	806	rBV2	221	119	0.01%	0.001%
10	3.798	840	842	847	rBV2	372	279	0.02%	0.003%
11	3.917	868	879	916	rBV	87920	276729	22.14%	2.881%
12	4.376	1004	1022	1048	rBV	202536	503770	40.30%	5.244%
13	4.595	1087	1090	1093	rVB2	506	320	0.03%	0.003%
14	4.646	1104	1106	1112	rVB2	538	360	0.03%	0.004%
15	4.714	1125	1127	1130	rBV2	242	127	0.01%	0.001%
16	4.778	1145	1147	1148	rBV	286	101	0.01%	0.001%
17	4.859	1169	1172	1175	rBV2	381	278	0.02%	0.003%
18	4.949	1198	1200	1203	rBV	397	208	0.02%	0.002%
19	4.974	1206	1208	1209	rBV	226	82	0.01%	0.001%
20	5.071	1220	1238	1263	rBV2	490358	1249938	100.00%	13.011%
21	5.389	1336	1337	1341	rBV	197	110	0.01%	0.001%
22	5.408	1341	1343	1344	rBV2	225	120	0.01%	0.001%
23	5.476	1360	1364	1371	rVB2	470	460	0.04%	0.005%
24	5.505	1371	1373	1375	rBV2	231	82	0.01%	0.001%
25	5.521	1375	1378	1380	rBV3	419	267	0.02%	0.003%
26	5.553	1384	1388	1392	rVB2	452	438	0.04%	0.005%
27	5.640	1402	1415	1439	rBV	381809	757816	60.63%	7.888%
28	5.926	1490	1504	1525	rBV2	44634	94506	7.56%	0.984%
29	6.032	1536	1537	1542	rBV2	491	297	0.02%	0.003%
30	6.093	1542	1556	1584	rBV	280205	567087	45.37%	5.903%
31	6.318	1625	1626	1629	rVB2	468	195	0.02%	0.002%
32	6.344	1629	1634	1635	rBV	111	93	0.01%	0.001%
33	6.357	1635	1638	1639	rBV	367	245	0.02%	0.003%
34	6.441	1661	1664	1665	rBV	307	185	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018931.D
 Acq On : 15 Oct 2020 23:21
 Operator : SY/MD
 Sample : L4382-14 40X
 Misc : 5.51µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Y2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.453	1665	1668	1670	rVV	348	210	0.02%	0.002%
36	6.598	1709	1713	1719	rBV3	453	497	0.04%	0.005%
37	6.736	1753	1756	1763	rVB2	517	455	0.04%	0.005%
38	6.775	1763	1768	1772	rBV2	345	355	0.03%	0.004%
39	6.797	1772	1775	1776	rVV	240	137	0.01%	0.001%
40	6.817	1780	1781	1785	rVB	383	227	0.02%	0.002%
41	6.881	1798	1801	1804	rBV2	377	286	0.02%	0.003%
42	6.900	1804	1807	1810	rVB	409	271	0.02%	0.003%
43	6.949	1820	1822	1827	rVB	309	205	0.02%	0.002%
44	7.006	1827	1840	1862	rBV	154385	278609	22.29%	2.900%
45	7.219	1902	1906	1907	rBV	422	307	0.02%	0.003%
46	7.338	1930	1943	1975	rBV	566941	978633	78.29%	10.187%
47	7.643	2027	2038	2061	rBV	106538	188129	15.05%	1.958%
48	7.997	2138	2148	2164	rVB2	40526	68828	5.51%	0.716%
49	8.109	2173	2183	2218	rBV2	268523	558567	44.69%	5.814%
50	8.508	2304	2307	2310	rVB2	533	337	0.03%	0.004%
51	8.598	2333	2335	2337	rVB	572	229	0.02%	0.002%
52	8.614	2338	2340	2342	rBV	249	133	0.01%	0.001%
53	8.682	2359	2361	2365	rBV4	357	225	0.02%	0.002%
54	8.746	2379	2381	2382	rBV4	371	144	0.01%	0.001%
55	8.797	2392	2397	2401	rBV	356	442	0.04%	0.005%
56	8.833	2406	2408	2409	rBV	303	130	0.01%	0.001%
57	8.871	2409	2420	2442	rBV	582813	955541	76.45%	9.947%
58	9.170	2510	2513	2516	rVB3	294	144	0.01%	0.001%
59	9.196	2516	2521	2524	rBV	470	429	0.03%	0.004%
60	9.354	2567	2570	2572	rBV3	394	228	0.02%	0.002%
61	9.389	2579	2581	2584	rBV2	378	195	0.02%	0.002%
62	9.444	2595	2598	2602	rBV	397	339	0.03%	0.004%
63	9.527	2621	2624	2626	rBV	324	222	0.02%	0.002%
64	9.608	2646	2649	2650	rBV	234	117	0.01%	0.001%
65	9.666	2664	2667	2669	rBV	240	129	0.01%	0.001%
66	9.746	2690	2692	2694	rBV	235	76	0.01%	0.001%
67	9.865	2723	2729	2732	rBV2	437	509	0.04%	0.005%
68	9.913	2740	2744	2749	rBV2	351	334	0.03%	0.003%
69	10.100	2799	2802	2804	rBV2	341	207	0.02%	0.002%
70	10.238	2833	2845	2862	rBV	279801	446061	35.69%	4.643%
71	10.608	2957	2960	2962	rVB	357	233	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101520\
 Data File : VV018931.D
 Acq On : 15 Oct 2020 23:21
 Operator : SY/MD
 Sample : L4382-14 40X
 Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Y2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.932	3059	3061	3063	rBV	185	99	0.01%	0.001%
73	11.013	3080	3086	3091	rBV3	445	589	0.05%	0.006%
74	11.038	3091	3094	3099	rVB2	330	250	0.02%	0.003%
75	11.064	3099	3102	3104	rBV	302	201	0.02%	0.002%
76	11.112	3114	3117	3121	rBV2	358	313	0.03%	0.003%
77	11.199	3140	3144	3150	rBV4	419	447	0.04%	0.005%
78	11.270	3154	3166	3191	rVV	580134	887633	71.01%	9.240%
79	11.646	3271	3283	3309	rBV	581345	904946	72.40%	9.420%
80	11.971	3382	3384	3385	rBV	261	84	0.01%	0.001%
81	12.199	3453	3455	3457	rBV	276	135	0.01%	0.001%
82	12.264	3473	3475	3478	rBV2	221	124	0.01%	0.001%
83	12.460	3532	3536	3538	rBV	486	391	0.03%	0.004%
84	12.627	3586	3588	3589	rBV	295	123	0.01%	0.001%
85	12.791	3637	3639	3642	rVB	418	186	0.01%	0.002%
86	12.810	3643	3645	3646	rBV	339	132	0.01%	0.001%
87	12.948	3686	3688	3691	rBV2	308	175	0.01%	0.002%
88	13.788	3946	3949	3951	rBV2	609	351	0.03%	0.004%


Sum of corrected areas: 9606623

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101520\
Data File : VV018931.D
Acq On : 15 Oct 2020 23:21
Operator : SY/MD
Sample : L4382-14 40X
Misc : 5.51µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Y2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

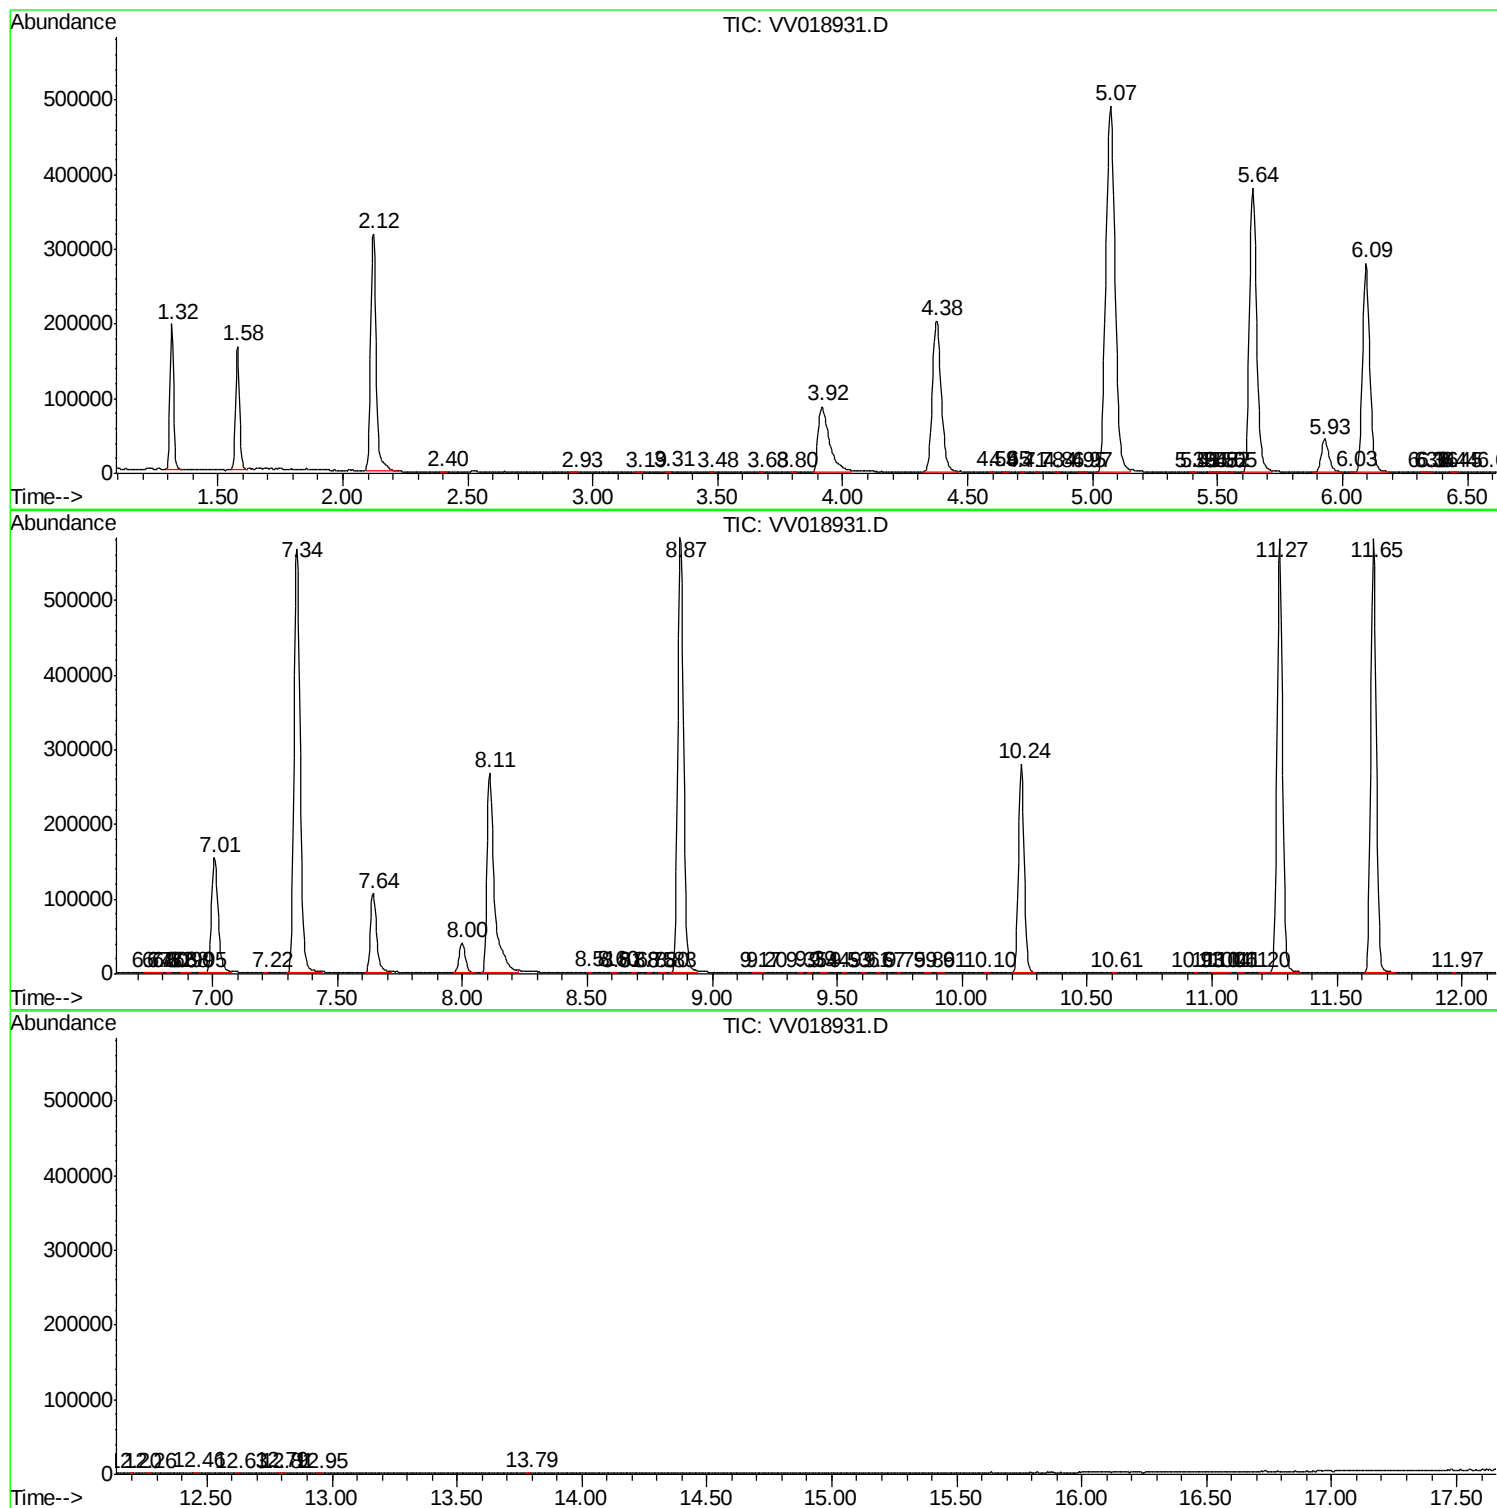

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101520\
Data File : VV018931.D
Acq On : 15 Oct 2020 23:21
Operator : SY/MD
Sample : L4382-14 40X
Misc : 5.51g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3Y2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101520\
Data File : VV018931.D
Acq On : 15 Oct 2020 23:21
Operator : SY/MD
Sample : L4382-14 40X
Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Y2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc