


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101520\
 Data File : VV018908.D
 Acq On : 15 Oct 2020 13:41
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 16 10:34:27 2020

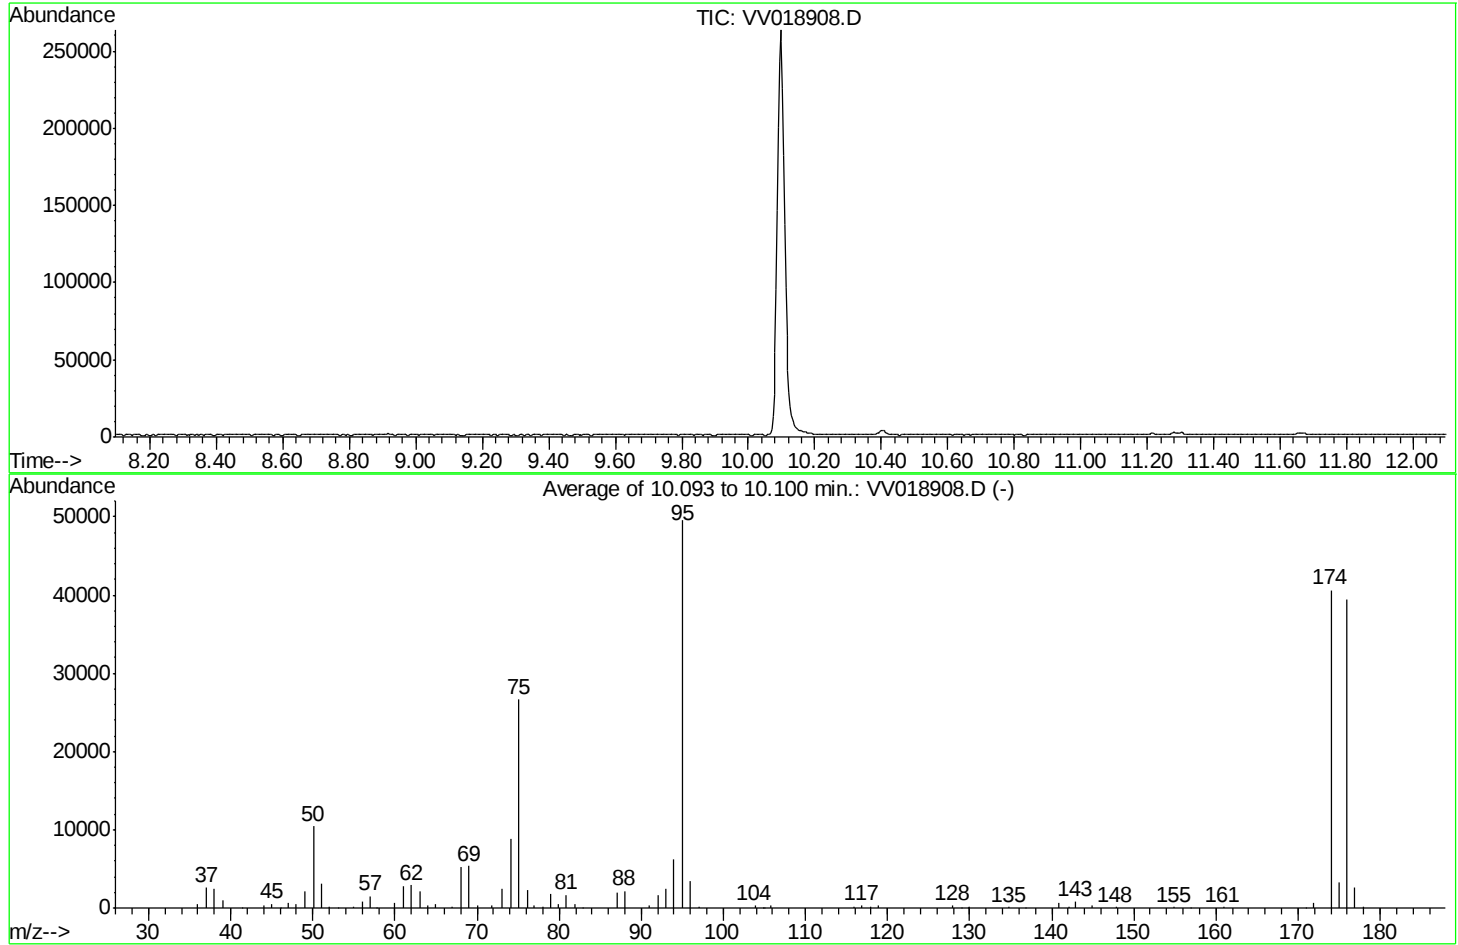

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	10454	PASS
75	95	30	80	53.7	26621	PASS
95	95	100	100	100.0	49552	PASS
96	95	5	9	7.1	3496	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.0	40653	PASS
175	174	5	9	8.0	3268	PASS
176	174	95	101	97.1	39477	PASS
177	176	5	9	6.5	2570	PASS

m/z	Abundance
36.00	542.0
37.10	2567.0
38.00	2339.0
39.10	1103.0
40.00	328.0
41.30	117.0
44.00	1483.0
45.00	552.0
47.10	636.0
48.00	478.0
49.00	2142.0
50.00	10157.0
51.00	3100.0
52.00	193.0
55.00	159.0
56.00	850.0
57.00	1409.0
57.80	123.0
60.00	641.0
61.00	2763.0
62.00	2744.0
63.10	1997.0
64.10	388.0
65.00	443.0
67.00	183.0
68.00	4886.0
69.00	5209.0
70.00	410.0
71.90	259.0
73.00	2445.0
74.00	8474.0
75.10	25784.0
76.10	2539.0
77.00	325.0
78.00	250.0
78.90	1779.0
79.90	512.0
80.90	1628.0
81.90	508.0
87.00	1871.0
88.00	1906.0
91.00	281.0
92.00	1536.0
93.00	2291.0
94.00	6115.0
95.10	47472.0
96.00	3485.0
97.00	144.0
103.80	323.0
105.80	295.0
115.90	197.0
116.90	306.0
117.90	223.0
118.90	299.0
128.00	265.0
129.80	161.0
134.80	132.0
140.90	547.0
142.10	131.0
143.00	714.0
144.90	272.0
147.80	120.0
154.90	112.0
160.90	112.0
171.90	551.0
174.00	37888.0
175.00	3185.0
176.00	37096.0
176.90	2473.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	611.0
37.00	2710.0
38.00	2459.0
39.00	1092.0
39.90	325.0
41.40	101.0
44.00	1432.0
45.00	580.0
46.00	113.0
47.10	695.0
48.00	531.0
49.00	2250.0
50.10	10904.0
51.10	3300.0
52.00	162.0
53.10	102.0
55.00	188.0
56.00	945.0
57.00	1572.0
60.00	627.0
61.00	2891.0
62.00	2990.0
63.10	2128.0
64.00	399.0
65.00	549.0
67.00	192.0
68.00	5376.0
69.00	5550.0
70.00	421.0
71.90	339.0
73.00	2633.0
74.00	9180.0
75.10	27576.0
76.10	2429.0
77.00	384.0
77.90	246.0
78.90	1914.0
79.80	543.0
80.90	1745.0
81.90	547.0
87.00	1942.0
88.00	2264.0
91.00	285.0
92.00	1650.0
93.00	2487.0
94.00	6485.0
95.00	51416.0
96.00	3589.0
97.00	143.0
103.80	322.0
104.80	105.0
105.90	272.0
116.00	204.0
116.90	323.0
117.90	226.0
118.90	334.0
127.90	286.0
129.00	106.0
130.00	159.0
134.80	135.0
140.80	621.0
142.10	144.0
142.90	799.0
144.90	297.0
147.80	138.0
154.90	116.0
161.00	124.0
170.90	110.0
171.90	671.0
174.00	42080.0
175.00	3382.0
176.00	40984.0
177.00	2632.0
177.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	551.0
37.00	2549.0
38.00	2375.0
39.10	1009.0
39.90	348.0
44.00	1308.0
45.00	564.0
46.00	114.0
47.00	660.0
48.00	469.0
49.00	2164.0
50.10	10302.0
51.10	3126.0
52.00	147.0
53.00	103.0
54.90	197.0
56.00	889.0
57.00	1534.0
60.00	515.0
61.00	2719.0
62.00	2921.0
63.10	2071.0
64.00	355.0
65.00	594.0
67.00	186.0
68.00	5342.0
69.00	5247.0
70.00	380.0
71.80	376.0
73.00	2501.0
74.10	8884.0
75.10	26504.0
76.10	2119.0
77.00	411.0
77.90	229.0
79.00	1901.0
79.80	526.0
80.90	1766.0
81.90	501.0
82.80	120.0
87.00	1945.0
88.00	2320.0
91.00	257.0
92.00	1550.0
93.00	2419.0
94.00	6111.0
95.00	49768.0
96.00	3414.0
97.00	119.0
103.90	300.0
105.00	122.0
105.90	283.0
116.00	180.0
116.90	338.0
117.90	231.0
118.90	315.0
127.90	275.0
129.90	196.0
134.80	138.0
136.80	111.0
140.80	621.0
142.10	120.0
142.90	788.0
144.90	254.0
147.80	119.0
154.90	118.0
156.90	109.0
160.90	128.0
170.90	121.0
171.90	687.0
174.00	41992.0
175.00	3238.0
176.00	40352.0
177.00	2607.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Scan 2790 (10.061 min): VV018908.D
BFB75

m/z	Abundance
39.90	345.0
44.00	1101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75