


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022846.D
Acq On : 15 Oct 2021 19:05
Operator : SY/MD
Sample : M4223-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG97

Manual Integrations
APPROVED

SAM
10/18/2021 1:06:12 PM

Quant Time: Oct 16 05:30:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 16 05:27:41 2021
Response via : Initial Calibration

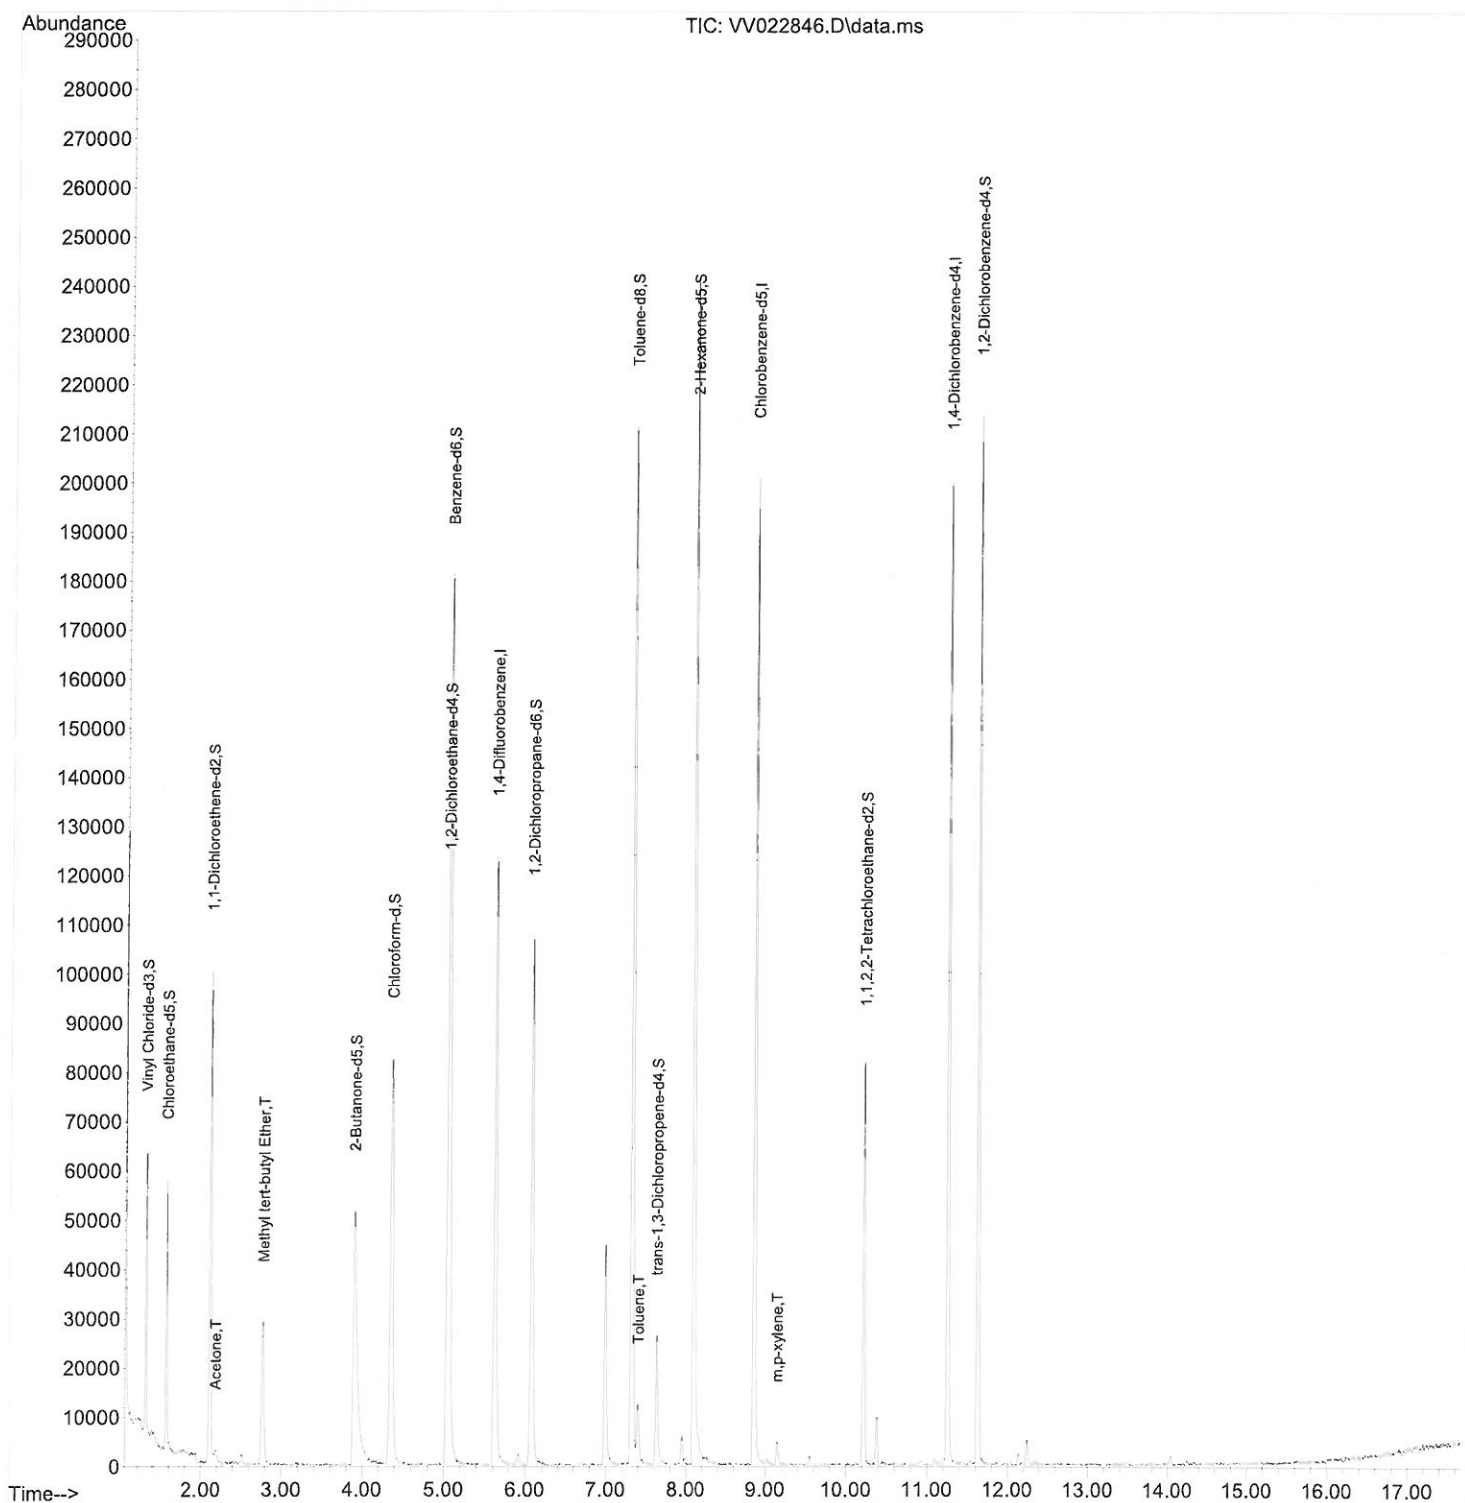

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022846.D
 Acq On : 15 Oct 2021 19:05
 Operator : SY/MD
 Sample : M4223-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG97

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:12 PM

Quant Time: Oct 16 05:30:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

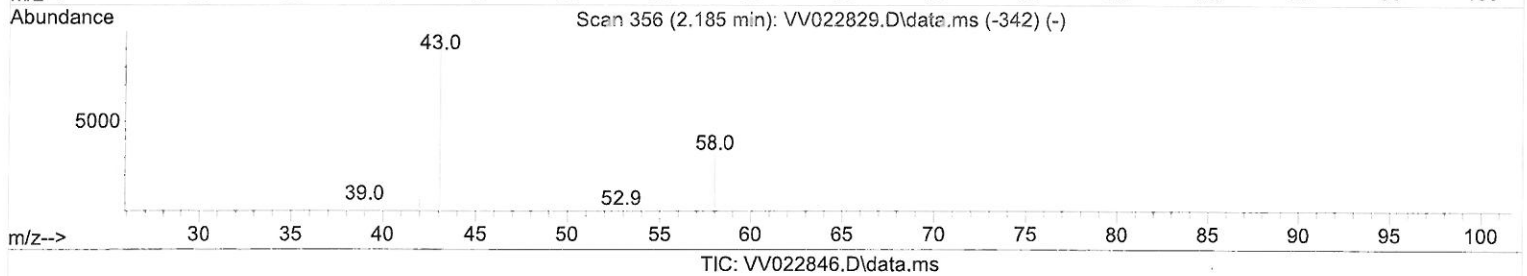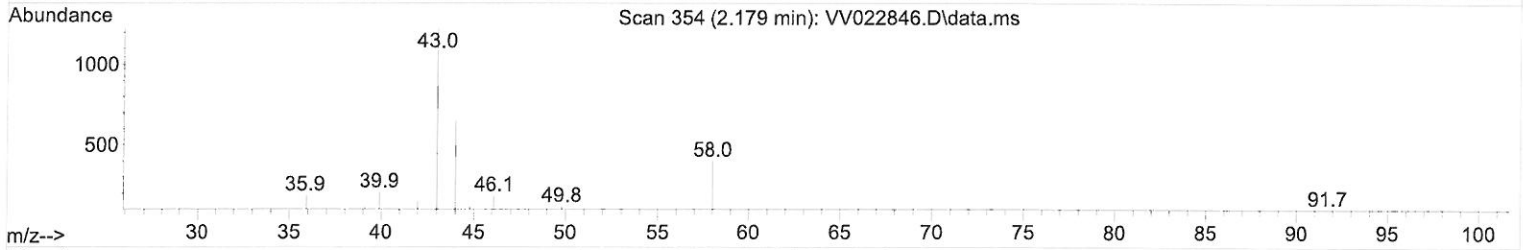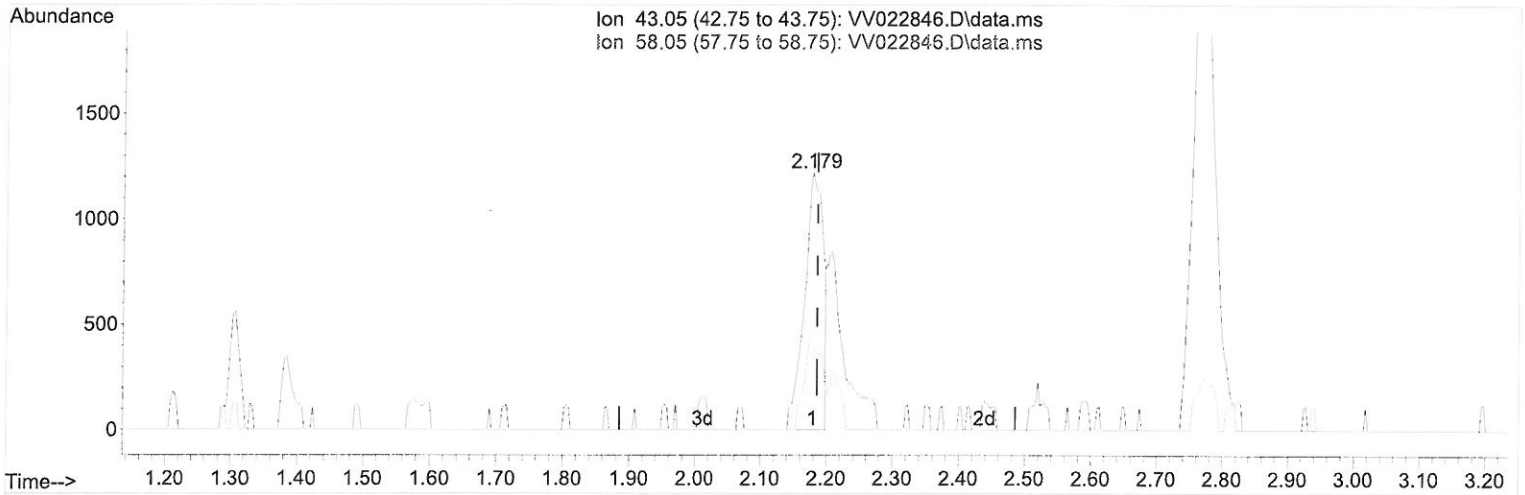

(13) Acetone (T)

2.179min (-0.006) 2.15 ug/L

response 2413

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	34.19#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022846.D
 Acq On : 15 Oct 2021 19:05
 Operator : SY/MD
 Sample : M4223-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG97

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:12 PM

Quant Time: Oct 16 05:30:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

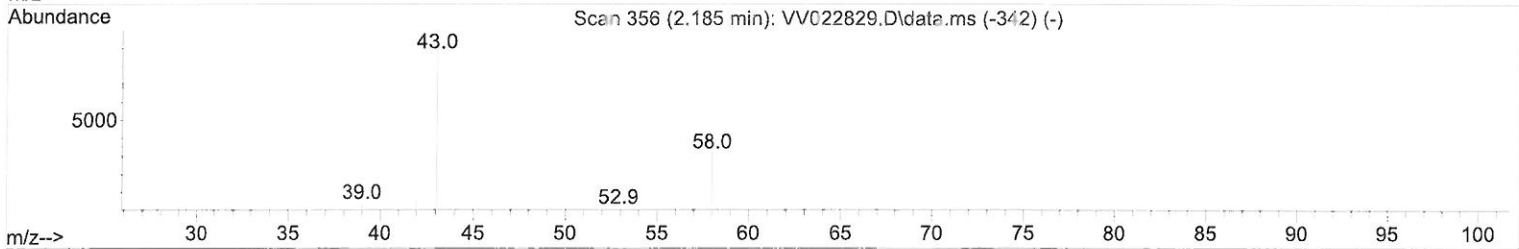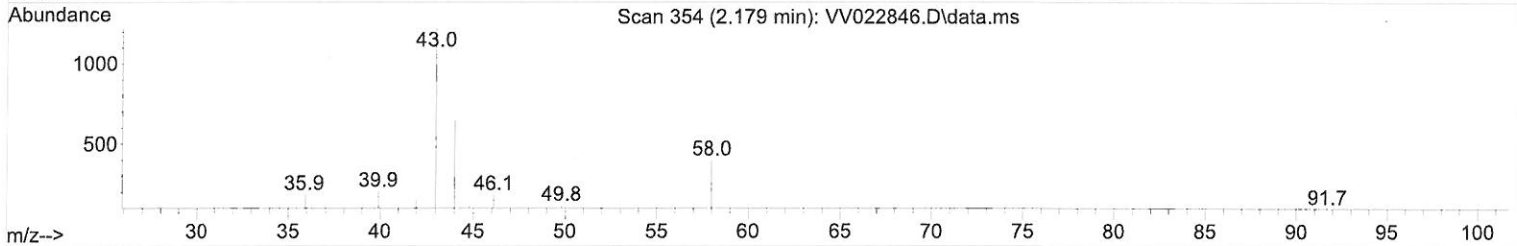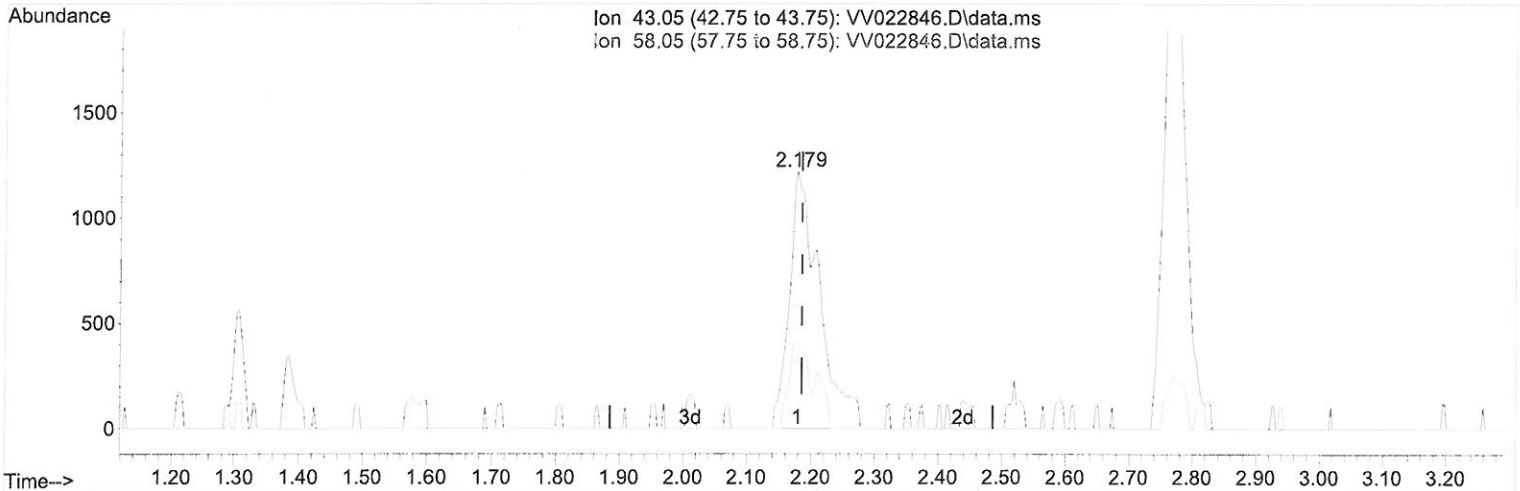

TIC: VV022846.D\data.ms

(13) Acetone (T)

2.179min (-0.006) 3.55 ug/L m

response 3991

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	20.67
0.00	0.00	0.00
0.00	0.00	0.00

MD
10/27/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101521\
 Data File : VW022846.D
 Acq On : 15 Oct 2021 19:05
 Operator : SY/MD
 Sample : M4223-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 BFG97

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:12 PM

Quant Time: Oct 16 05:30:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	111735	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	114427	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54075	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36087	4.694	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.568	69	32283	4.673	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.400%	
11) 1,1-Dichloroethene-d2	2.108	63	51126	3.390	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.800%	
20) 2-Butanone-d5	3.892	46	102645	50.923	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	101.840%	
24) Chloroform-d	4.352	84	86997	5.491	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.800%	
26) 1,2-Dichloroethane-d4	5.034	65	41047	5.338	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.800%	
32) Benzene-d6	5.053	84	167275	4.911	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.072	67	53829	5.336	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.800%	
41) Toluene-d8	7.320	98	141915	4.819	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.625	79	16749	5.005	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	100.000%	
46) 2-Hexanone-d5	8.092	63	84558	62.700	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	125.400%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	39881	5.836	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	116.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57713	5.756	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.200%	
Target Compounds						
13) Acetone	2.179	43	3991m	3.551	ug/L	Qvalue
17) Methyl tert-butyl Ether	2.770	73	28527	1.747	ug/L	98
42) Toluene	7.397	91	9344	0.299	ug/L	95
53) m,p-xylene	9.143	106	1672	0.134	ug/L	86

7 MD
 10/27/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed