


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022847.D
Acq On : 15 Oct 2021 19:29
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Manual Integrations
APPROVED

SAM
10/18/2021 1:06:40 PM

Quant Time: Oct 16 05:30:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 16 05:27:41 2021
Response via : Initial Calibration

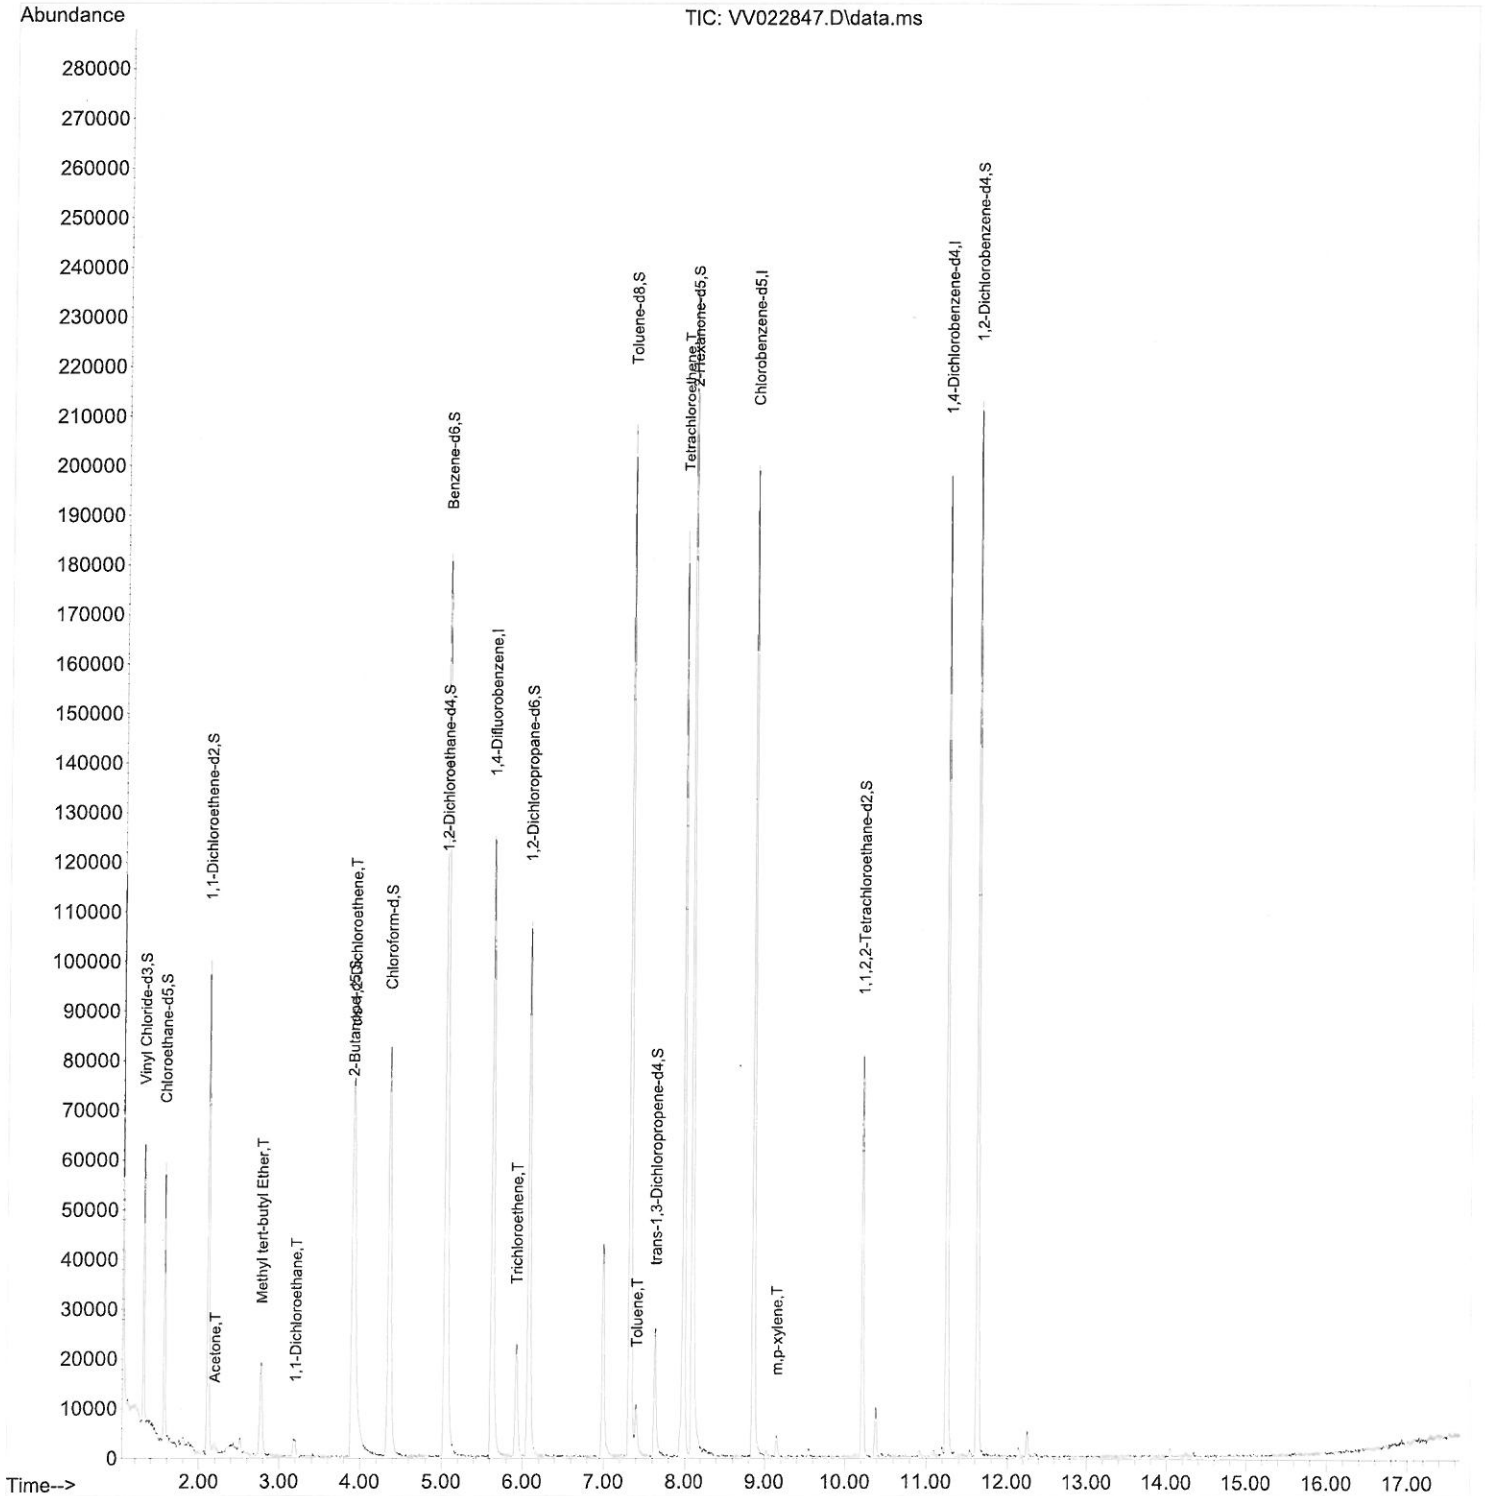

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022847.D
 Acq On : 15 Oct 2021 19:29
 Operator : SY/MD
 Sample : M4223-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG98

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:40 PM

Quant Time: Oct 16 05:30:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

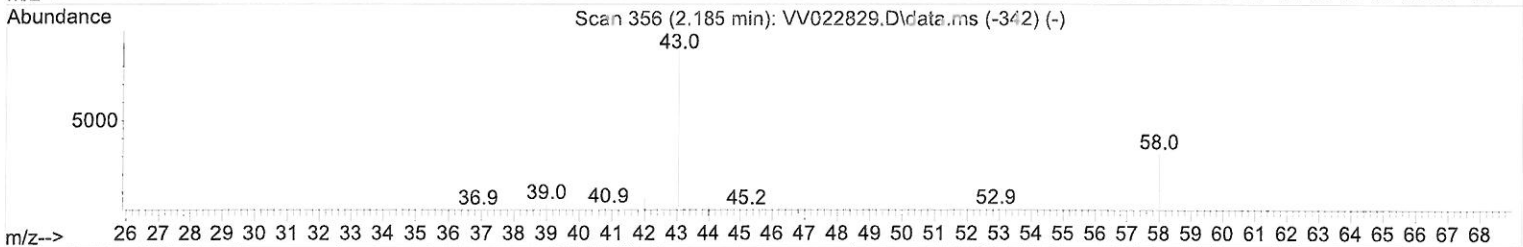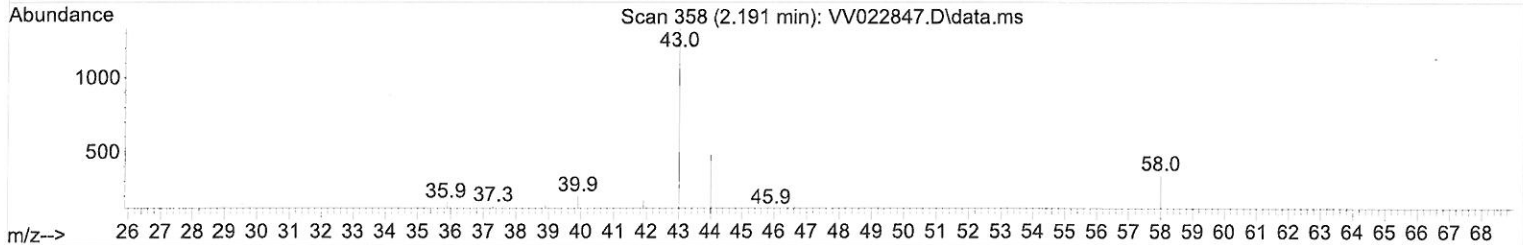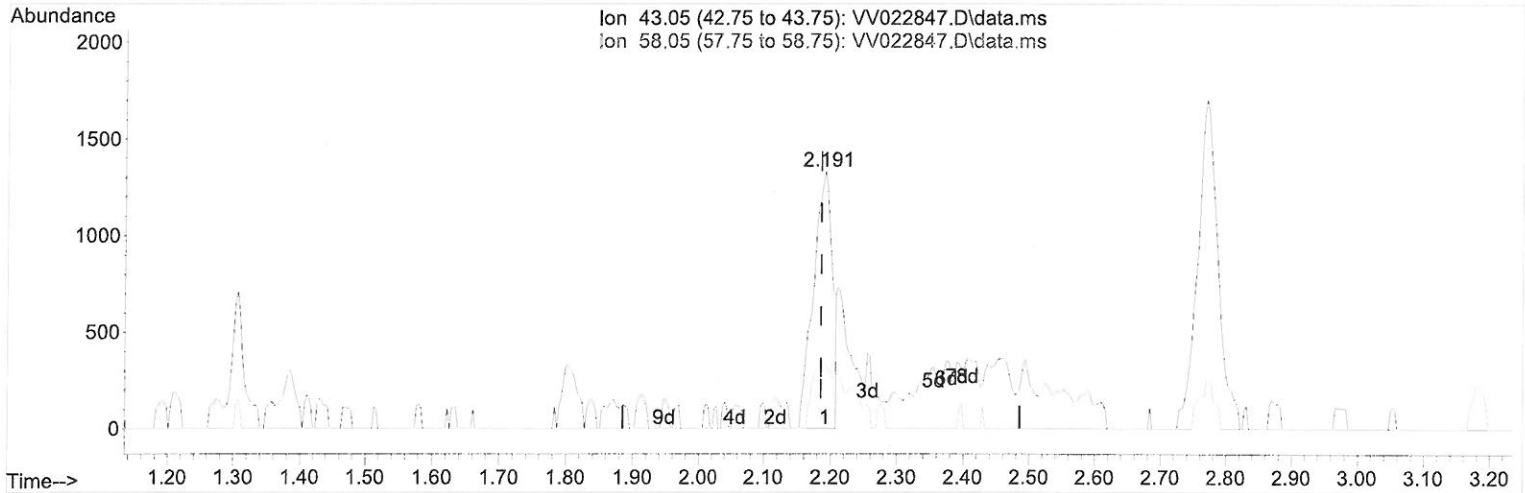

TIC: VV022847.D\data.ms

(13) Acetone (T)

2.191min (+ 0.006) 2.31 ug/L

response 2649

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	26.09#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022847.D
 Acq On : 15 Oct 2021 19:29
 Operator : SY/MD
 Sample : M4223-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG98

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:40 PM

Quant Time: Oct 16 05:30:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

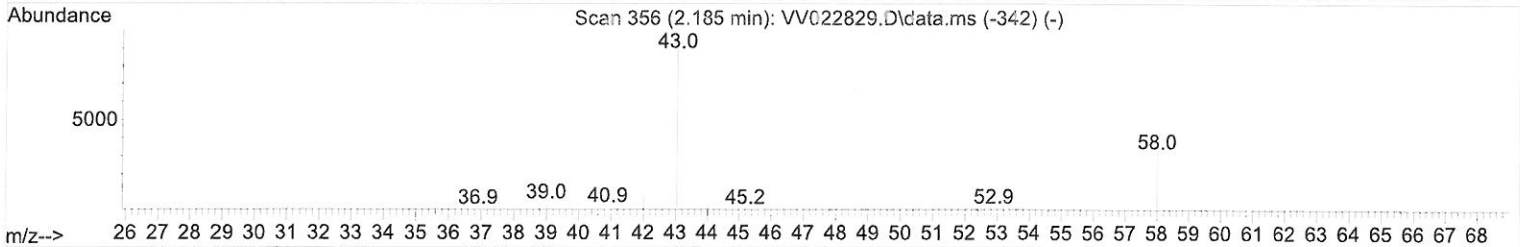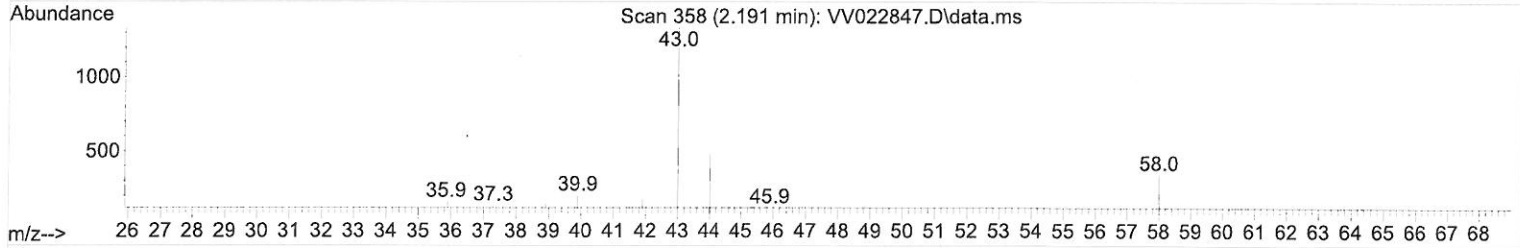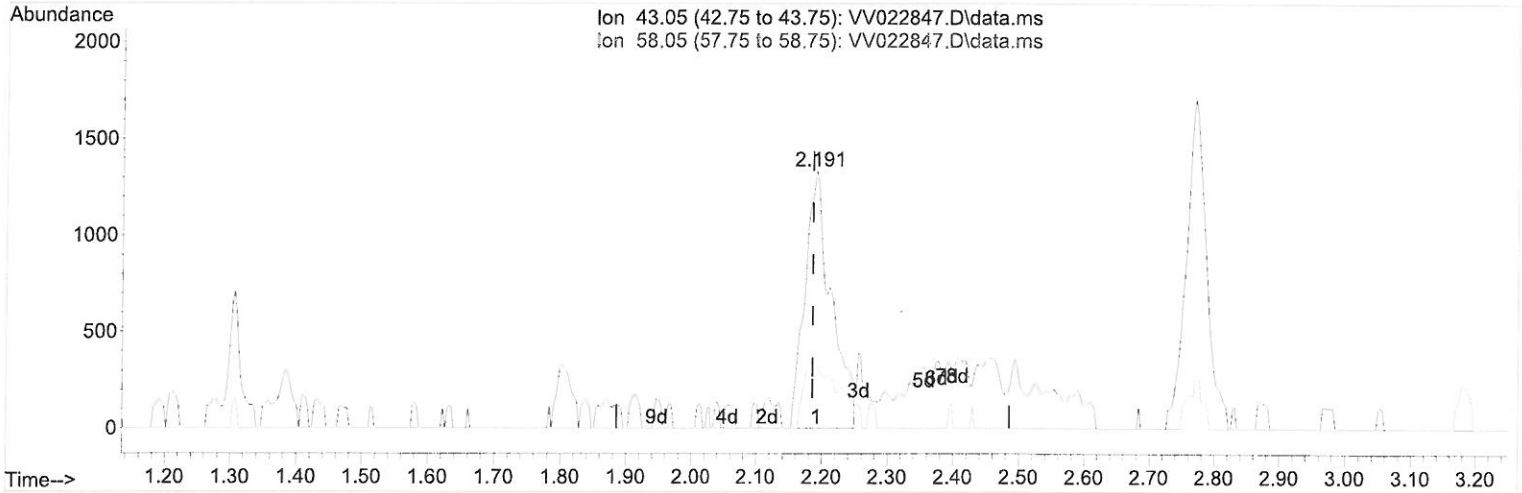

TIC: VV022847.D\data.ms

(13) Acetone (T)

2.191min (+ 0.006) 3.25 ug/L m

response 3732

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	18.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\vqasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022847.D
 Acq On : 15 Oct 2021 19:29
 Operator : SY/MD
 Sample : M4223-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG98

Manual Integrations
 APPROVED

SAM
 10/18/2021 1:06:40 PM

Quant Time: Oct 16 05:30:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	114187	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	114765	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54146	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	35301	4.493	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.800%	
7) Chloroethane-d5	1.568	69	32453	4.597	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.000%	
11) 1,1-Dichloroethane-d2	2.108	63	50252	3.261	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.200%	
20) 2-Butanone-d5	3.895	46	104903	50.925	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	101.860%	
24) Chloroform-d	4.352	84	86982	5.373	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.400%	
26) 1,2-Dichloroethane-d4	5.034	65	41048	5.224	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.053	84	166885	4.885	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.072	67	53120	5.250	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.000%	
41) Toluene-d8	7.320	98	139235	4.714	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.628	79	15723	4.685	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.600%	
46) 2-Hexanone-d5	8.091	63	82864	61.263	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	122.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39027	5.694	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	113.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	56760	5.654	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.000%	
Target Compounds						
13) Acetone	2.191	43	3732m	3.249	ug/L	Qvalue
17) Methyl tert-butyl Ether	2.770	73	17666	1.058	ug/L	97
19) 1,1-Dichloroethane	3.201	63	2092	0.155	ug/L #	78
22) cis-1,2-Dichloroethene	3.915	96	22121	2.809	ug/L	98
34) Trichloroethene	5.921	95	7961	0.947	ug/L	95
42) Toluene	7.400	91	8263	0.263	ug/L	94
47) Tetrachloroethene	7.979	164	43828	6.447	ug/L	97
53) m,p-xylene	9.146	106	1295	0.104	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 MD
 10/27/21