

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022830.D
 Acq On : 15 Oct 2021 12:44
 Operator : SY/MD
 Sample : VV1015WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK224

Quant Time: Oct 16 05:28:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	112376	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	113130	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54364	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36948	4.779	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.600%
7) Chloroethane-d5	1.568	69	32382	4.661	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.108	63	53104	3.501	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.000%
20) 2-Butanone-d5	3.905	46	84103	41.486	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.980%
24) Chloroform-d	4.355	84	86979	5.459	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.200%
26) 1,2-Dichloroethane-d4	5.040	65	39728	5.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
32) Benzene-d6	5.056	84	166270	4.937	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
36) 1,2-Dichloropropane-d6	6.075	67	51706	5.184	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.600%
41) Toluene-d8	7.320	98	141436	4.858	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
43) trans-1,3-Dichloroprop...	7.628	79	15670	4.736	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.800%
46) 2-Hexanone-d5	8.091	63	69305	51.979	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.960%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	35364	5.234	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	54812	5.438	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds					Qvalue	
42) Toluene	7.400	91	6020	0.195	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022830.D
Acq On : 15 Oct 2021 12:44
Operator : SY/MD
Sample : VV1015WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK224

Quant Time: Oct 16 05:28:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 16 05:27:41 2021
Response via : Initial Calibration

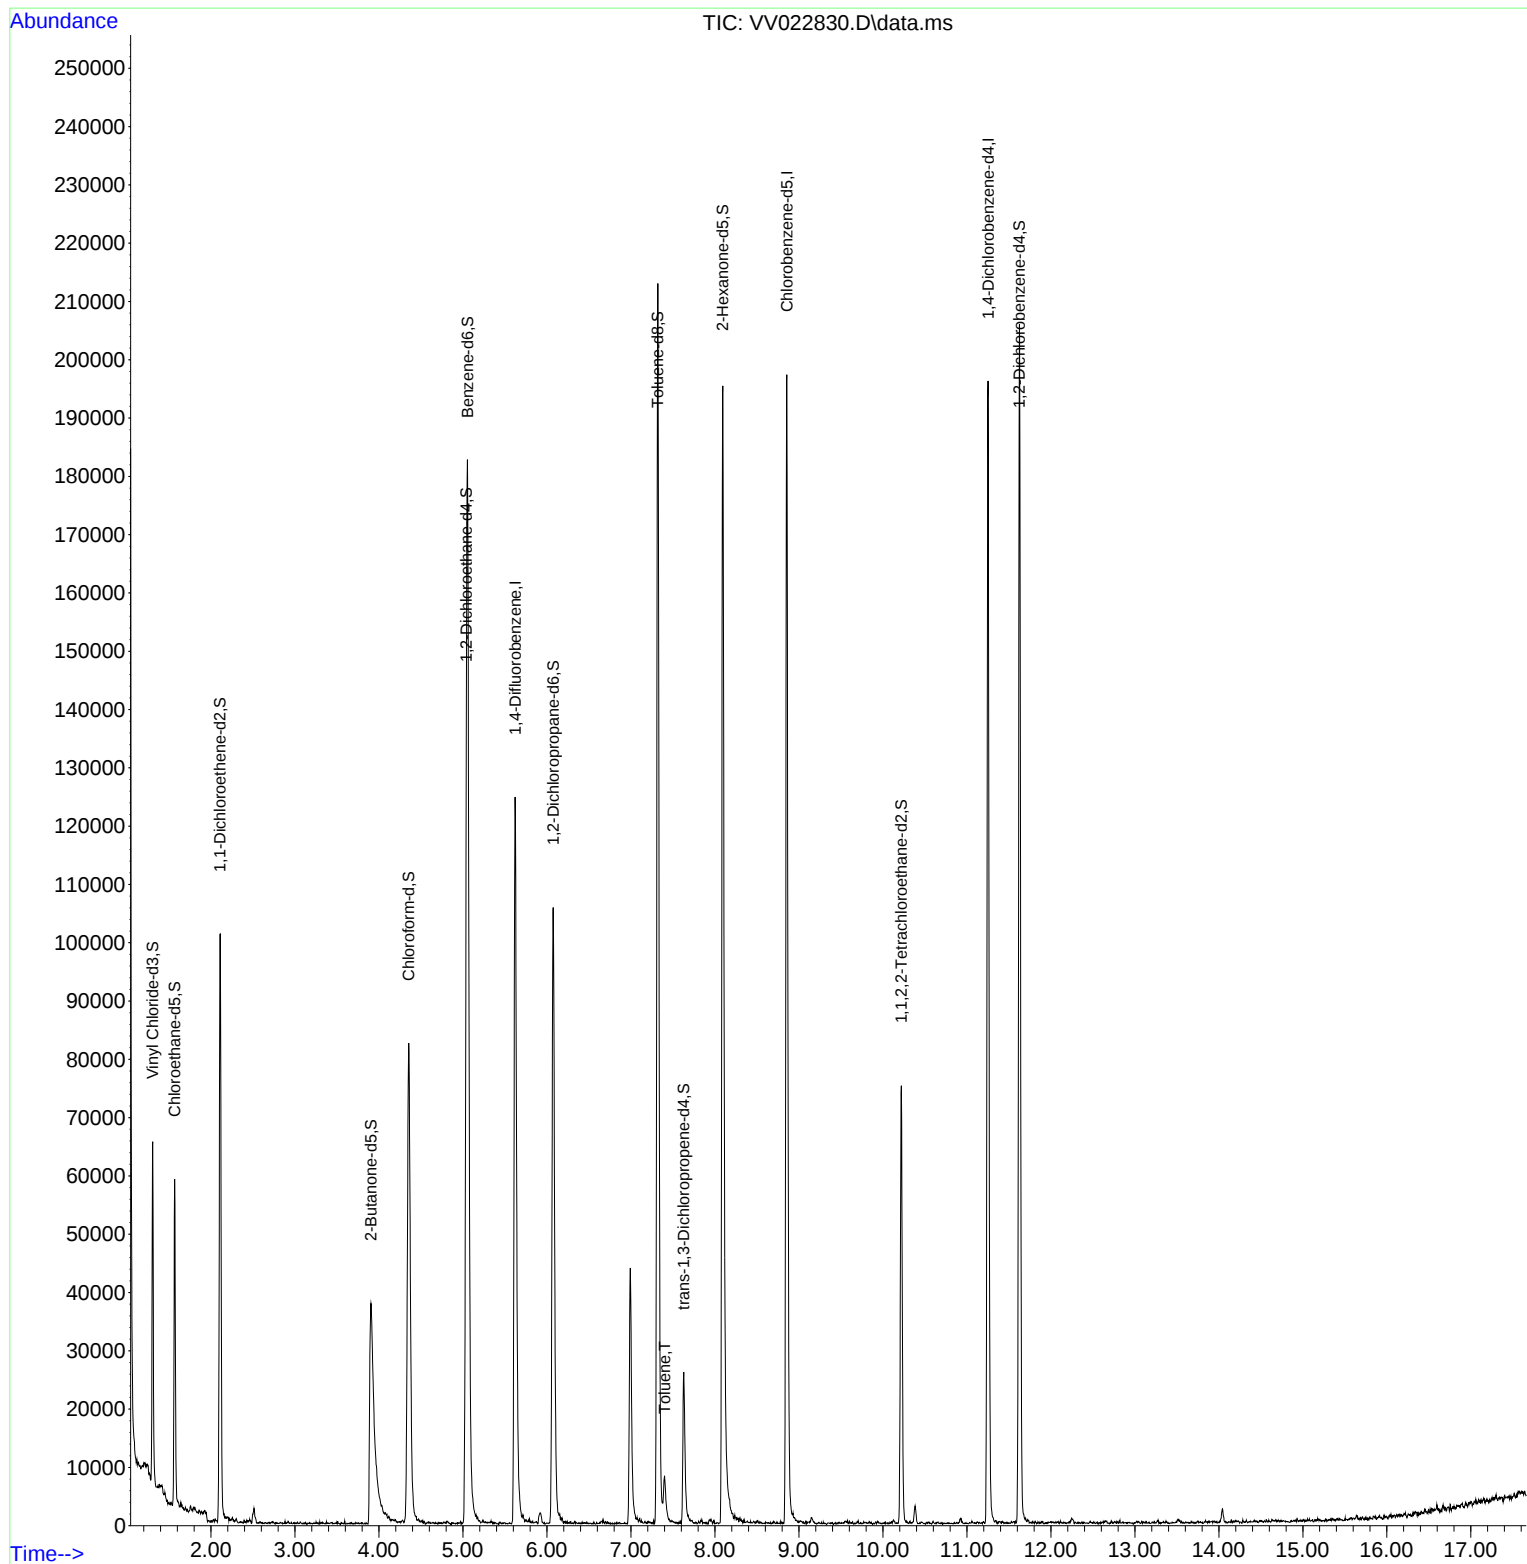

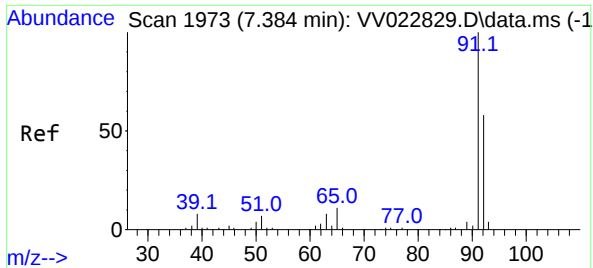

#42
Toluene
Concen: 0.195 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.016 min
Lab File: VV022830.D
Acq: 15 Oct 2021 12:44

Instrument :
MSVOA_V
ClientSampleId :
VBLK224

Tgt Ion: 91 Resp: 6020
Ion Ratio Lower Upper
91 100
92 55.0 40.7 75.7

