

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101521\
 Data File : VW022843.D
 Acq On : 15 Oct 2021 17:53
 Operator : SY/MD
 Sample : M4214-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGG2

Quant Time: Oct 16 05:29:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 16 05:27:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124375	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59447	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35999	4.207	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.200%
7) Chloroethane-d5	1.568	69	33543	4.362	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.200%
11) 1,1-Dichloroethene-d2	2.108	63	53578	3.192	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.800%
20) 2-Butanone-d5	3.895	46	102783	45.809	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.620%
24) Chloroform-d	4.352	84	87898	4.984	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.034	65	40209	4.698	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.053	84	166594	4.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.072	67	53234	4.799	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.320	98	141129	4.358	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.625	79	16894	4.591	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.800%
46) 2-Hexanone-d5	8.091	63	80490	54.274	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.540%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37569	4.999	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	56100	5.090	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.800%
Target Compounds						Qvalue
3) Chloromethane	1.240	50	1932	0.212	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022843.D
Acq On : 15 Oct 2021 17:53
Operator : SY/MD
Sample : M4214-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGG2

Quant Time: Oct 16 05:29:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 16 05:27:41 2021
Response via : Initial Calibration

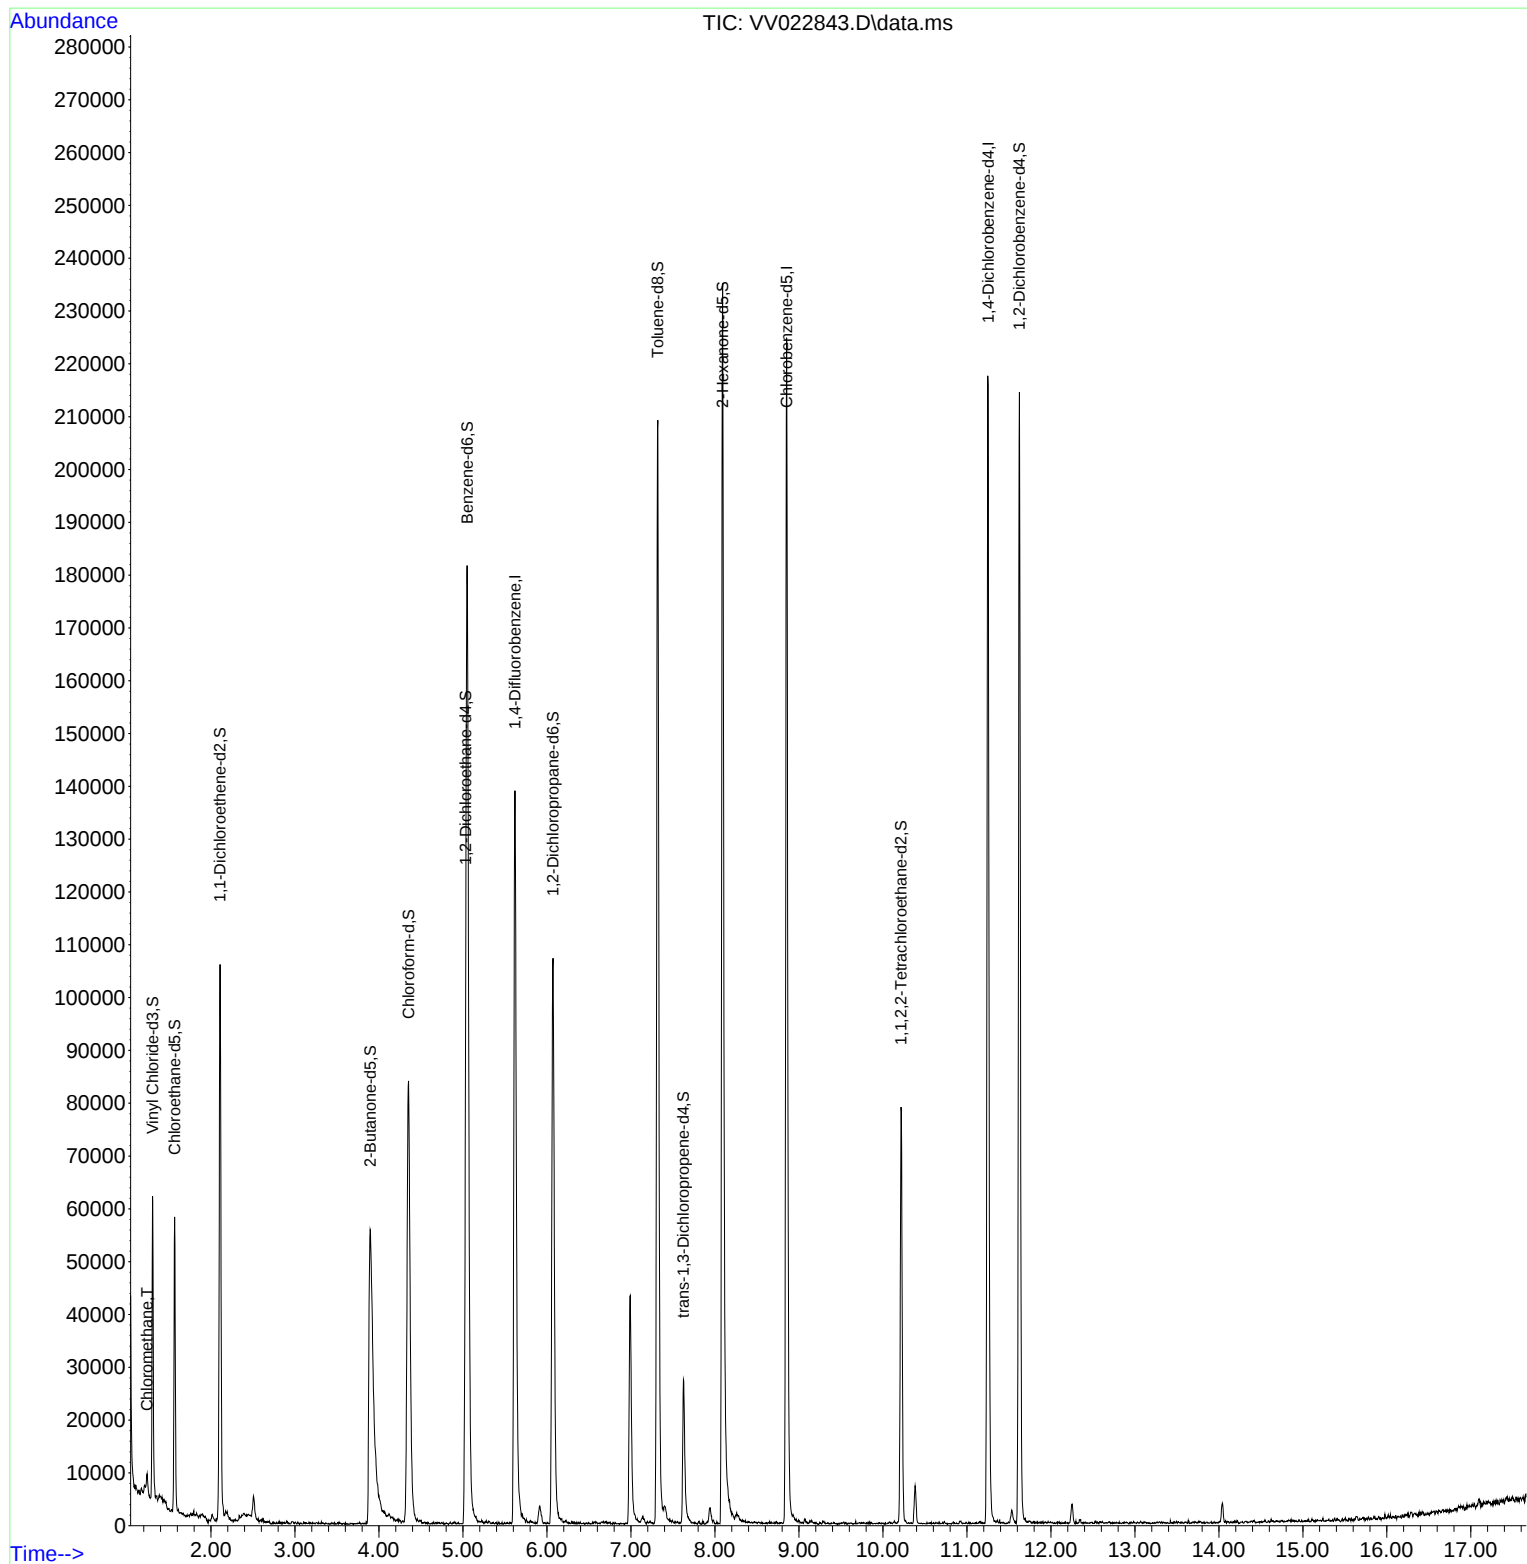

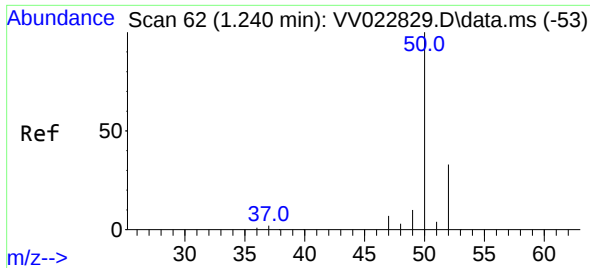

#3
 Chloromethane
 Concen: 0.212 ug/L
 RT: 1.240 min Scan# 62
 Delta R.T. -0.000 min
 Lab File: VV022843.D
 Acq: 15 Oct 2021 17:53

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGG2

Tgt Ion: 50 Resp: 1932
 Ion Ratio Lower Upper
 50 100
 52 29.9 22.9 42.5

