

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022832.D
 Acq On : 15 Oct 2021 13:35
 Operator : SY/MD
 Sample : M4182-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	27	rVB3	6820	5994	1.30%	0.169%
2	1.304	76	82	92	rVB	61394	59751	12.94%	1.684%
3	1.568	156	164	176	rVB	53212	61871	13.40%	1.744%
4	2.108	321	332	346	rBV	89872	130416	28.25%	3.677%
5	3.912	880	893	926	rBV2	32314	142446	30.85%	4.016%
6	4.352	1014	1030	1057	rBV2	81072	205028	44.41%	5.780%
7	5.050	1231	1247	1283	rBV2	184831	461686	100.00%	13.015%
8	5.619	1413	1424	1446	rBV	125576	258171	55.92%	7.278%
9	6.072	1551	1565	1589	rBV	108573	223679	48.45%	6.306%
10	6.992	1841	1851	1876	rBV	44569	86271	18.69%	2.432%
11	7.320	1939	1953	1971	rBV	210307	375073	81.24%	10.574%
12	7.397	1973	1977	1989	rVB6	3552	6532	1.41%	0.184%
13	7.628	2039	2049	2061	rBV	26208	46290	10.03%	1.305%
14	8.091	2183	2193	2230	rBV	200501	392395	84.99%	11.062%
15	8.854	2418	2430	2448	rBV	198594	327531	70.94%	9.233%
16	10.220	2844	2855	2875	rBV	74622	121417	26.30%	3.423%
17	10.384	2893	2906	2915	rBV2	4396	6601	1.43%	0.186%
18	11.249	3165	3175	3194	rBV	194022	304181	65.88%	8.575%
19	11.625	3280	3292	3312	rBV	210957	331939	71.90%	9.358%




Sum of corrected areas: 3547272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022832.D
Acq On : 15 Oct 2021 13:35
Operator : SY/MD
Sample : M4182-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

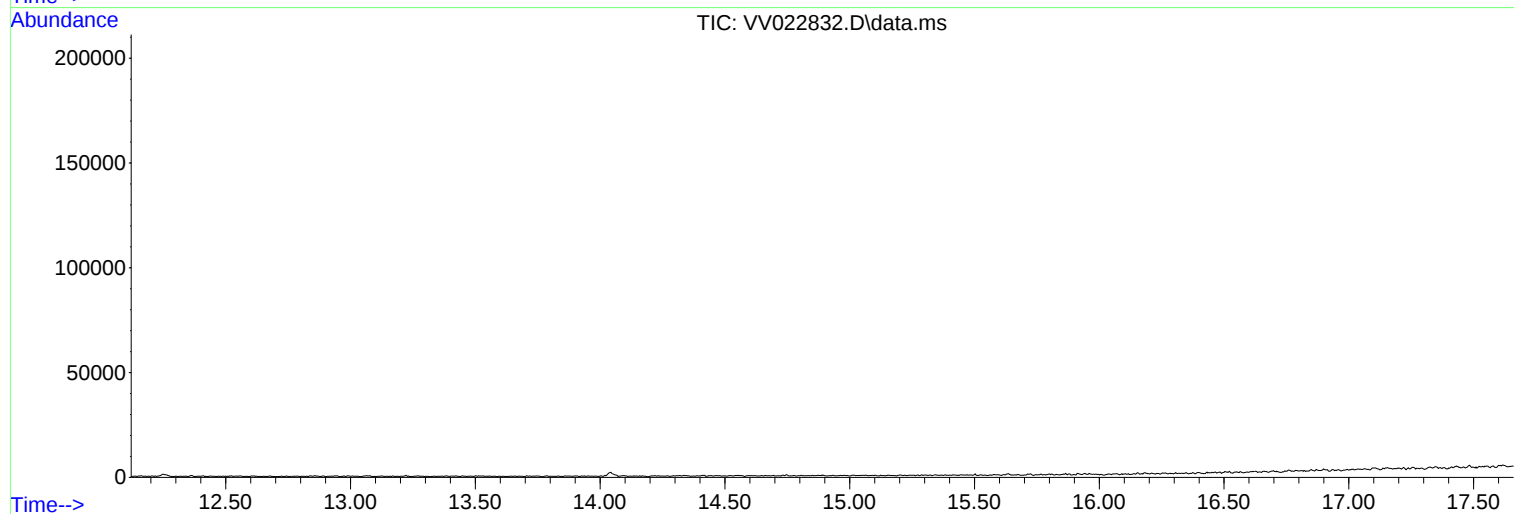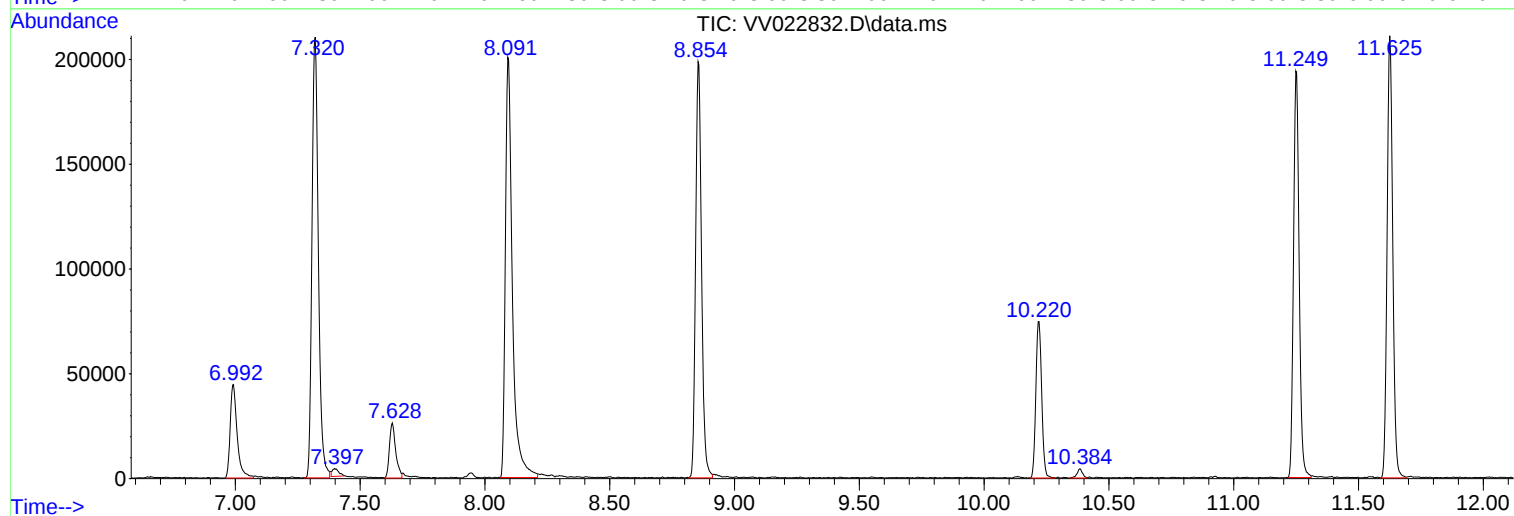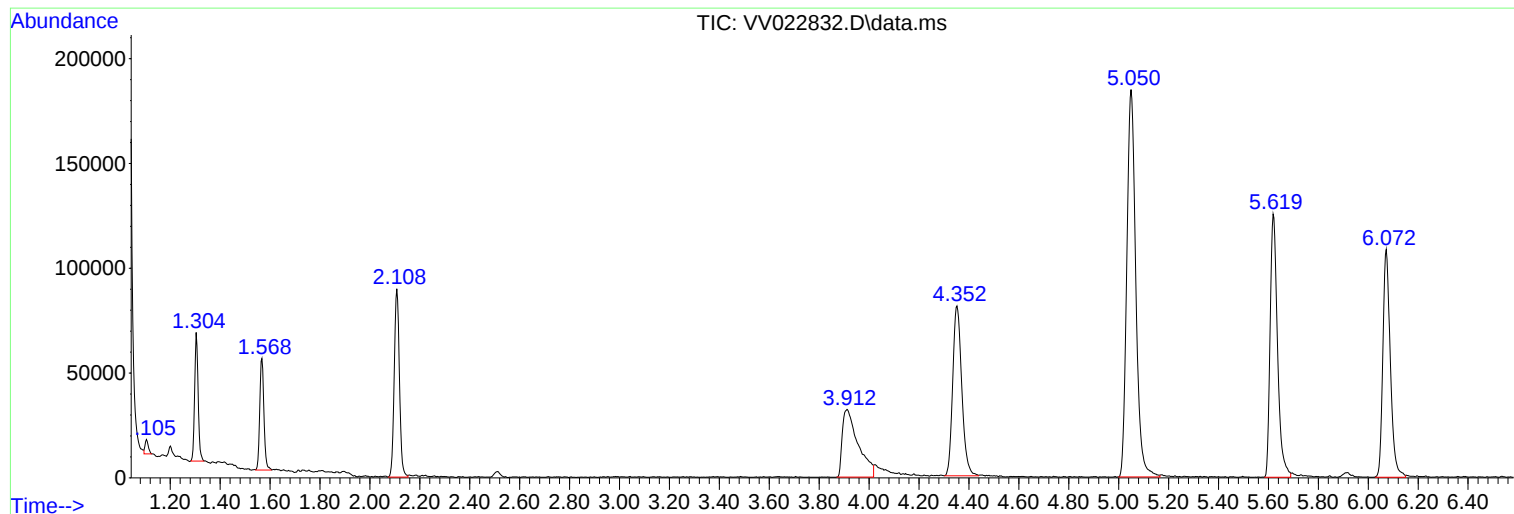

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022832.D
Acq On : 15 Oct 2021 13:35
Operator : SY/MD
Sample : M4182-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022832.D
Acq On : 15 Oct 2021 13:35
Operator : SY/MD
Sample : M4182-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
