

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022833.D
 Acq On : 15 Oct 2021 13:59
 Operator : SY/MD
 Sample : M4207-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B86

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	56028	57859	13.09%	1.642%
2	1.568	157	164	180	rVB	56030	61956	14.01%	1.759%
3	2.108	320	332	348	rBV	95065	139771	31.62%	3.967%
4	3.892	876	887	919	rBV	44361	146547	33.15%	4.160%
5	4.352	1014	1030	1058	rBV2	79771	205114	46.40%	5.822%
6	5.050	1231	1247	1271	rBV2	176314	442100	100.00%	12.549%
7	5.619	1411	1424	1444	rBV	128905	263602	59.62%	7.482%
8	5.918	1505	1517	1527	rVB9	2608	5649	1.28%	0.160%
9	6.072	1552	1565	1592	rBV2	104378	217475	49.19%	6.173%
10	6.992	1839	1851	1872	rBV	41981	80799	18.28%	2.293%
11	7.320	1941	1953	1972	rBV	205139	362533	82.00%	10.290%
12	7.628	2038	2049	2067	rBV	25677	47352	10.71%	1.344%
13	7.940	2136	2146	2157	rBV2	4756	8740	1.98%	0.248%
14	8.091	2182	2193	2223	rBV	200212	367306	83.08%	10.426%
15	8.853	2418	2430	2449	rBV	204863	337992	76.45%	9.594%
16	10.220	2844	2855	2868	rBV	72121	115056	26.02%	3.266%
17	10.384	2895	2906	2917	rBV2	10993	17193	3.89%	0.488%
18	11.249	3162	3175	3194	rBV	202472	317456	71.81%	9.011%
19	11.625	3279	3292	3308	rBV	204800	321700	72.77%	9.131%
20	12.255	3479	3488	3497	rVB2	4300	6853	1.55%	0.195%




Sum of corrected areas: 3523053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022833.D
Acq On : 15 Oct 2021 13:59
Operator : SY/MD
Sample : M4207-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

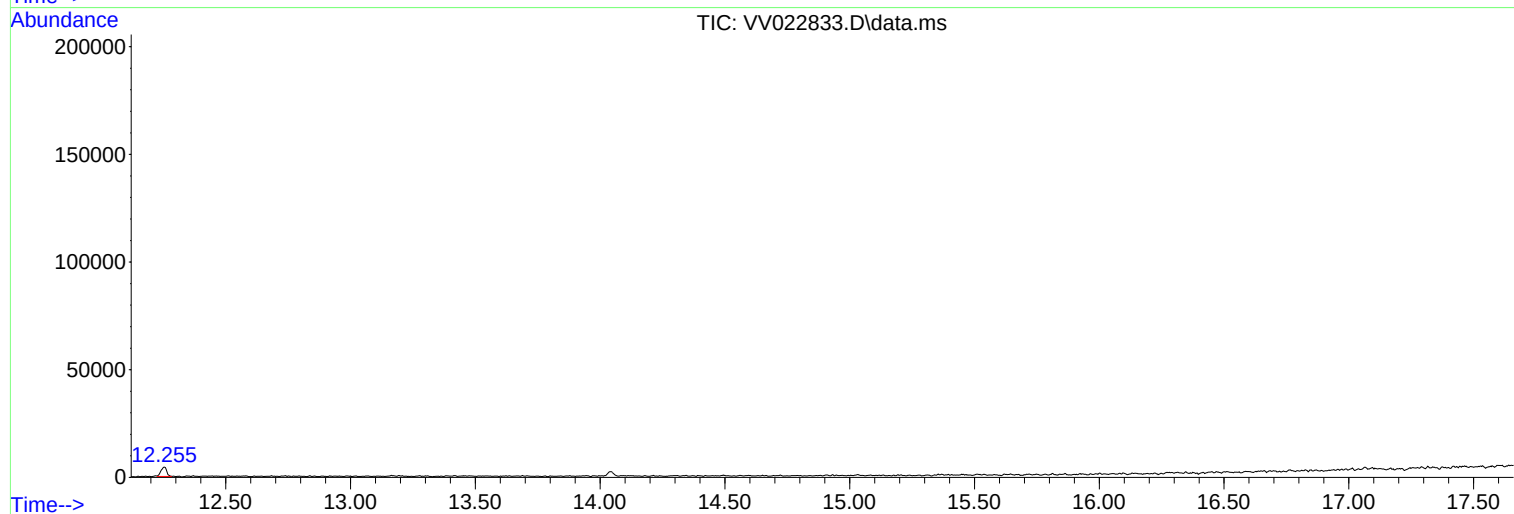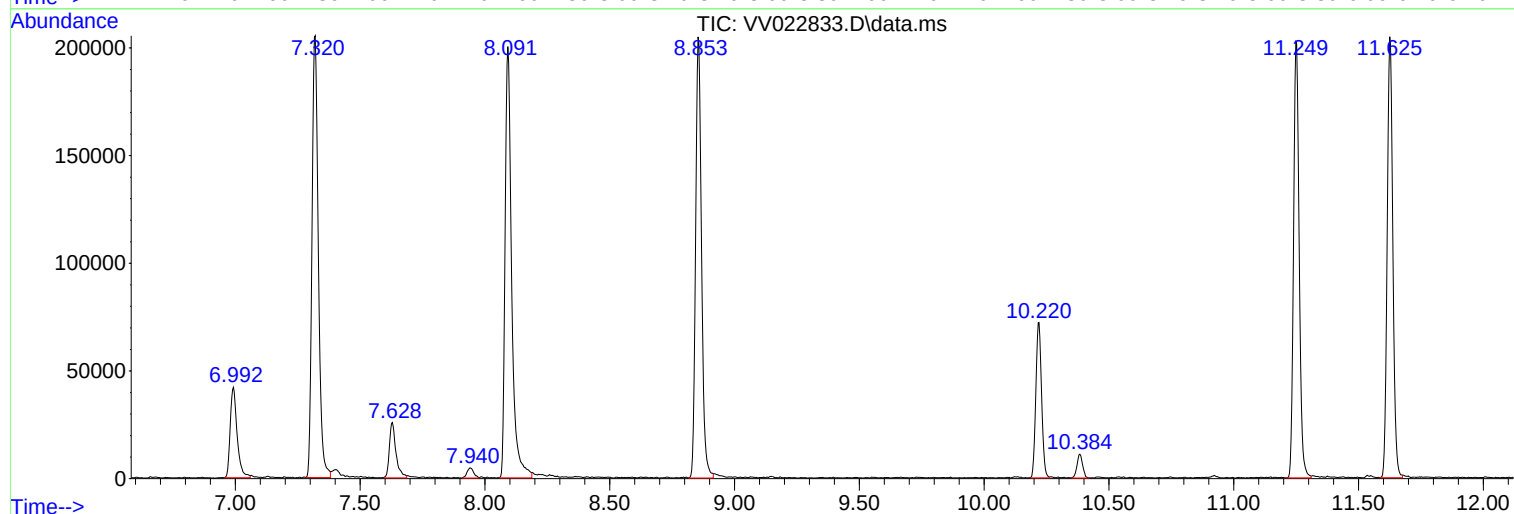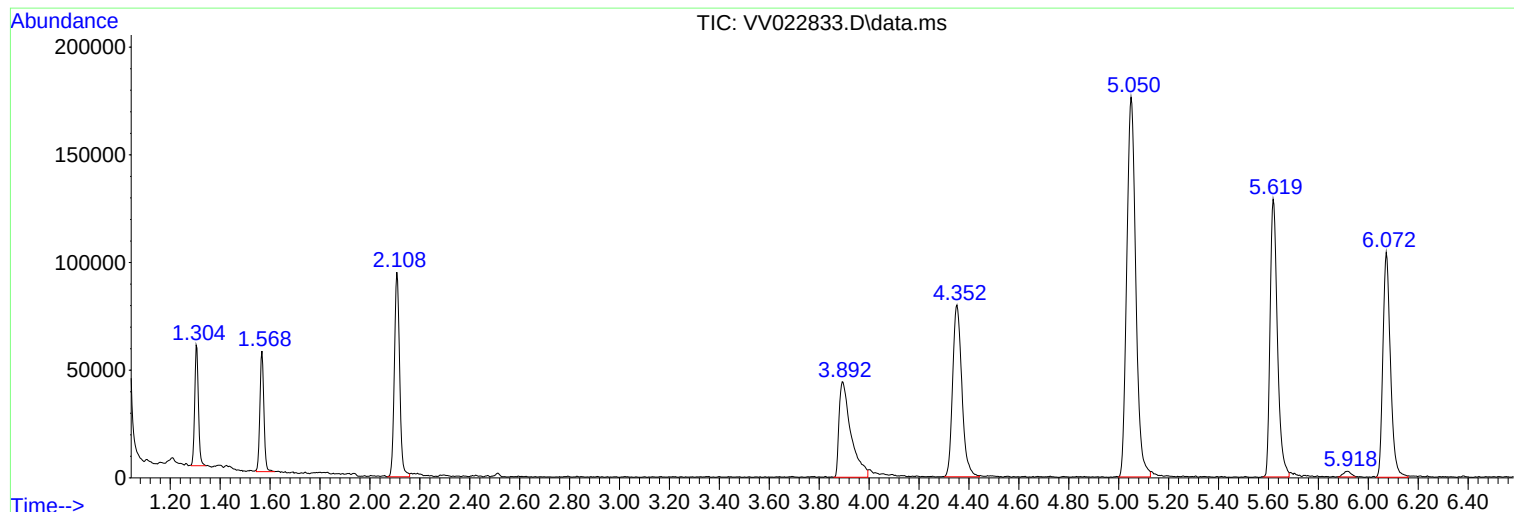

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022833.D
Acq On : 15 Oct 2021 13:59
Operator : SY/MD
Sample : M4207-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022833.D
Acq On : 15 Oct 2021 13:59
Operator : SY/MD
Sample : M4207-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
