

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022834.D
 Acq On : 15 Oct 2021 14:22
 Operator : SY/MD
 Sample : M4207-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B91

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	58180	61027	13.63%	1.747%
2	1.568	156	164	176	rBV	55086	61839	13.82%	1.770%
3	2.108	321	332	348	rBV	84972	122975	27.48%	3.520%
4	3.899	878	889	927	rBV2	40869	148741	33.23%	4.258%
5	4.352	1014	1030	1054	rBV	82120	205850	45.99%	5.893%
6	5.053	1231	1248	1274	rBV3	179310	447587	100.00%	12.813%
7	5.622	1410	1425	1450	rBV2	126485	261655	58.46%	7.490%
8	5.918	1506	1517	1529	rVB7	2872	6135	1.37%	0.176%
9	6.072	1552	1565	1594	rBV	104291	218115	48.73%	6.244%
10	6.992	1840	1851	1870	rBV	42508	81281	18.16%	2.327%
11	7.320	1941	1953	1971	rBV	205175	363943	81.31%	10.418%
12	7.397	1973	1977	1988	rVB6	3147	5265	1.18%	0.151%
13	7.629	2039	2049	2065	rBV	25895	46395	10.37%	1.328%
14	7.944	2135	2147	2159	rBV3	3298	5825	1.30%	0.167%
15	8.092	2183	2193	2224	rBV	197939	370871	82.86%	10.616%
16	8.854	2414	2430	2460	rBV	201632	332970	74.39%	9.532%
17	10.217	2843	2854	2871	rBV	71983	115090	25.71%	3.295%
18	10.384	2897	2906	2918	rVB3	7010	11188	2.50%	0.320%
19	11.249	3164	3175	3192	rBV	195564	304543	68.04%	8.718%
20	11.625	3280	3292	3313	rBV	206189	322057	71.95%	9.219%




Sum of corrected areas: 3493352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022834.D
Acq On : 15 Oct 2021 14:22
Operator : SY/MD
Sample : M4207-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

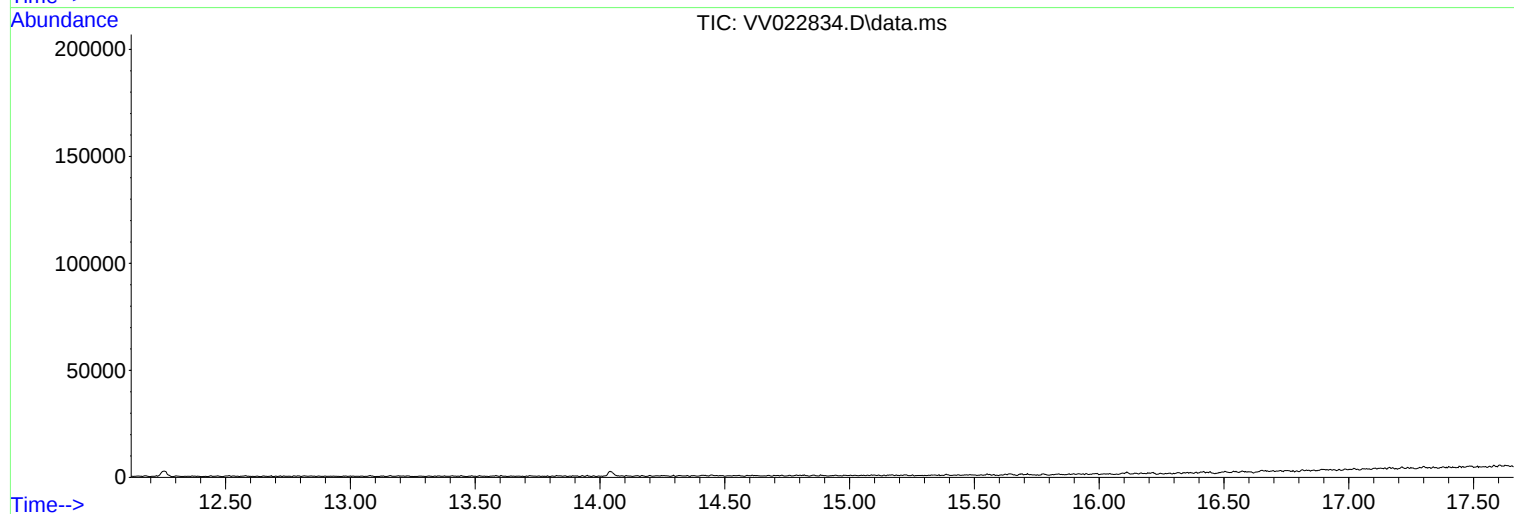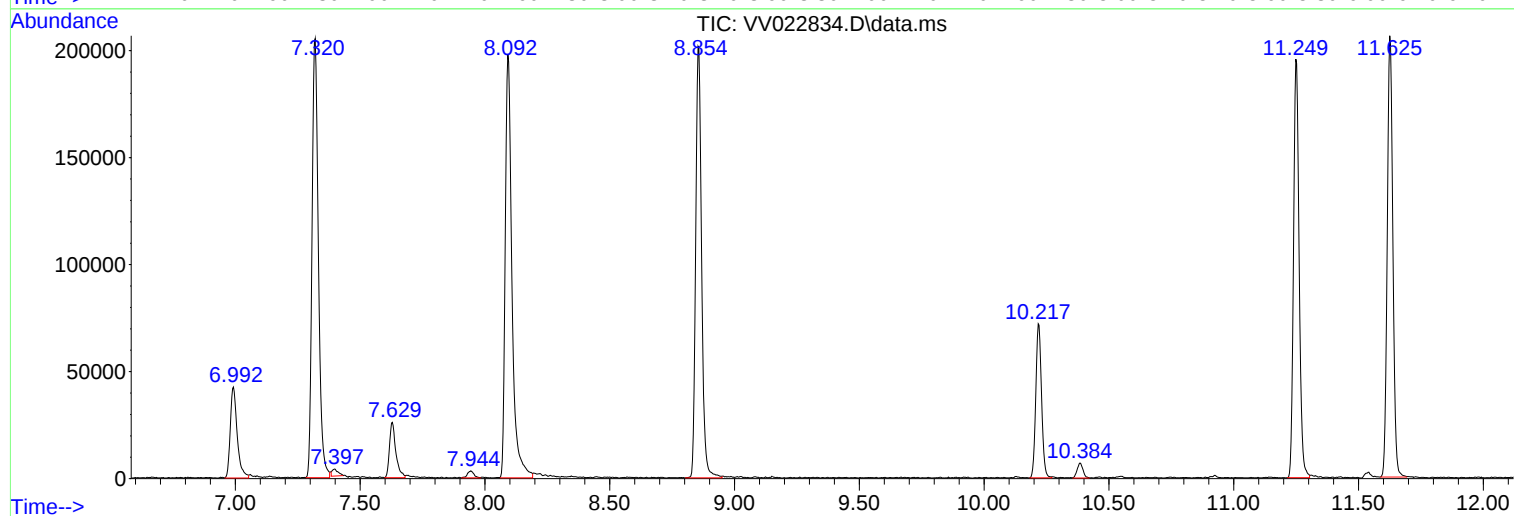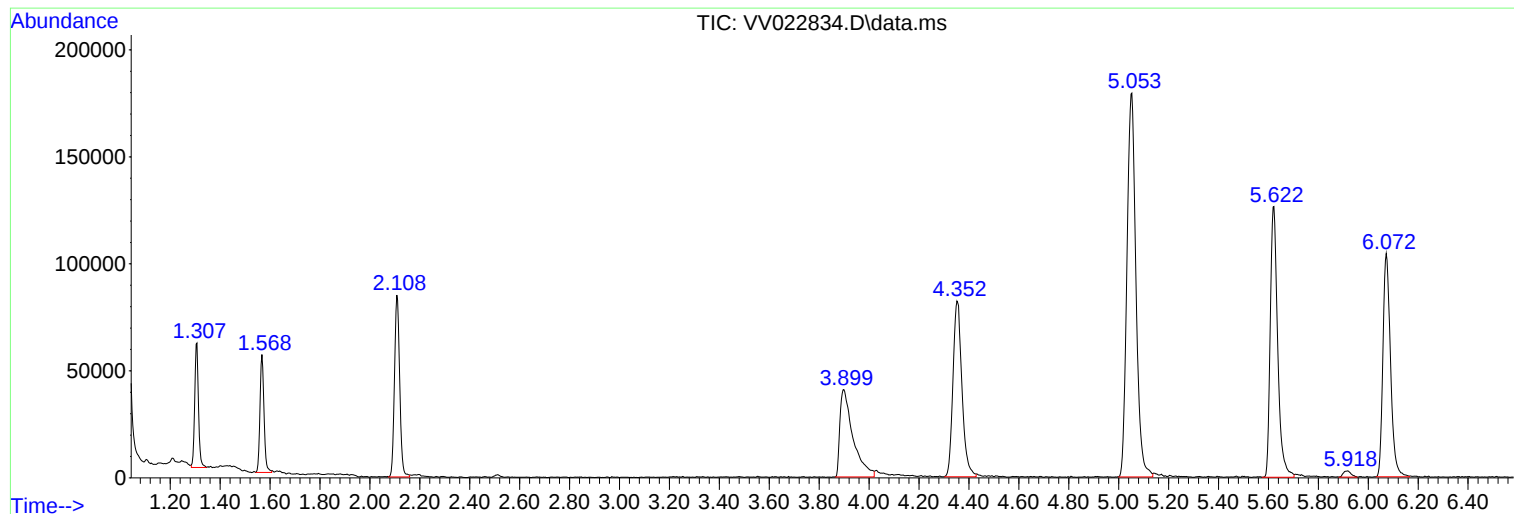

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022834.D
Acq On : 15 Oct 2021 14:22
Operator : SY/MD
Sample : M4207-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022834.D
Acq On : 15 Oct 2021 14:22
Operator : SY/MD
Sample : M4207-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
