

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022840.D
 Acq On : 15 Oct 2021 16:43
 Operator : SY/MD
 Sample : M4223-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	29	rVB	9757	8728	1.53%	0.229%
2	1.304	76	82	95	rVB	61427	63335	11.14%	1.665%
3	1.568	156	164	175	rVB	49728	56332	9.91%	1.481%
4	2.108	322	332	344	rBV	83757	120803	21.25%	3.176%
5	2.179	344	354	372	rVB	13631	31845	5.60%	0.837%
6	2.349	384	407	410	rBV6	3262	8724	1.53%	0.229%
7	2.767	522	537	561	rVB2	19753	42197	7.42%	1.110%
8	3.905	875	891	916	rBV4	50547	184840	32.51%	4.860%
9	4.352	1014	1030	1054	rBV2	64868	161848	28.46%	4.256%
10	5.050	1230	1247	1273	rBV3	142744	362504	63.75%	9.532%
11	5.619	1411	1424	1448	rBV	105295	215501	37.90%	5.666%
12	5.921	1505	1518	1537	rBV3	22355	47614	8.37%	1.252%
13	6.072	1550	1565	1586	rBV	82456	170662	30.01%	4.487%
14	6.992	1840	1851	1872	rBV	34610	67339	11.84%	1.771%
15	7.320	1941	1953	1971	rBV	170008	296487	52.14%	7.796%
16	7.397	1971	1977	1993	rVB2	6295	11756	2.07%	0.309%
17	7.629	2039	2049	2064	rBV	22133	39084	6.87%	1.028%
18	7.976	2136	2157	2183	rBV	330704	568600	100.00%	14.951%
19	8.092	2183	2193	2218	rBV	190663	335139	58.94%	8.812%
20	8.854	2420	2430	2453	rBV	170974	281611	49.53%	7.405%
21	10.217	2840	2854	2867	rBV2	66457	105673	18.58%	2.779%
22	10.384	2895	2906	2919	rVB4	11085	18931	3.33%	0.498%
23	11.249	3165	3175	3194	rBV	180502	279389	49.14%	7.346%
24	11.625	3280	3292	3315	rBV	188773	293647	51.64%	7.721%
25	12.252	3475	3487	3497	rBV	8597	13566	2.39%	0.357%
26	14.040	4033	4043	4055	rVB2	5030	8244	1.45%	0.217%
27	17.098	4987	4994	5003	rBV	6233	8724	1.53%	0.229%




Sum of corrected areas: 3803123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022840.D
Acq On : 15 Oct 2021 16:43
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

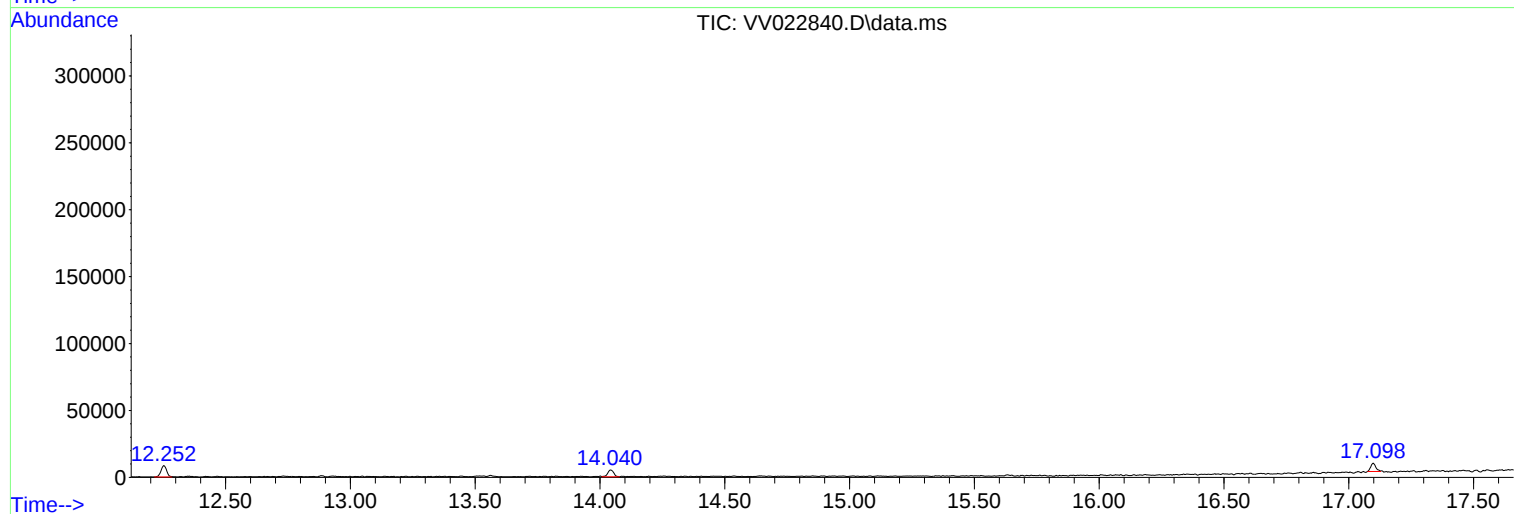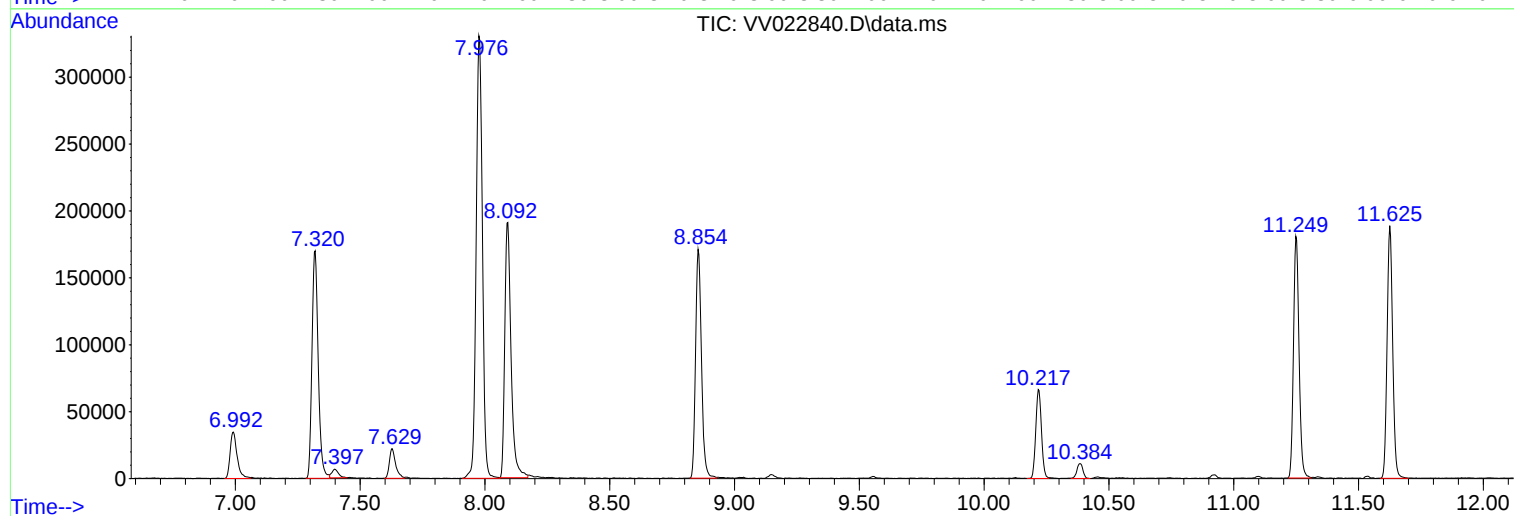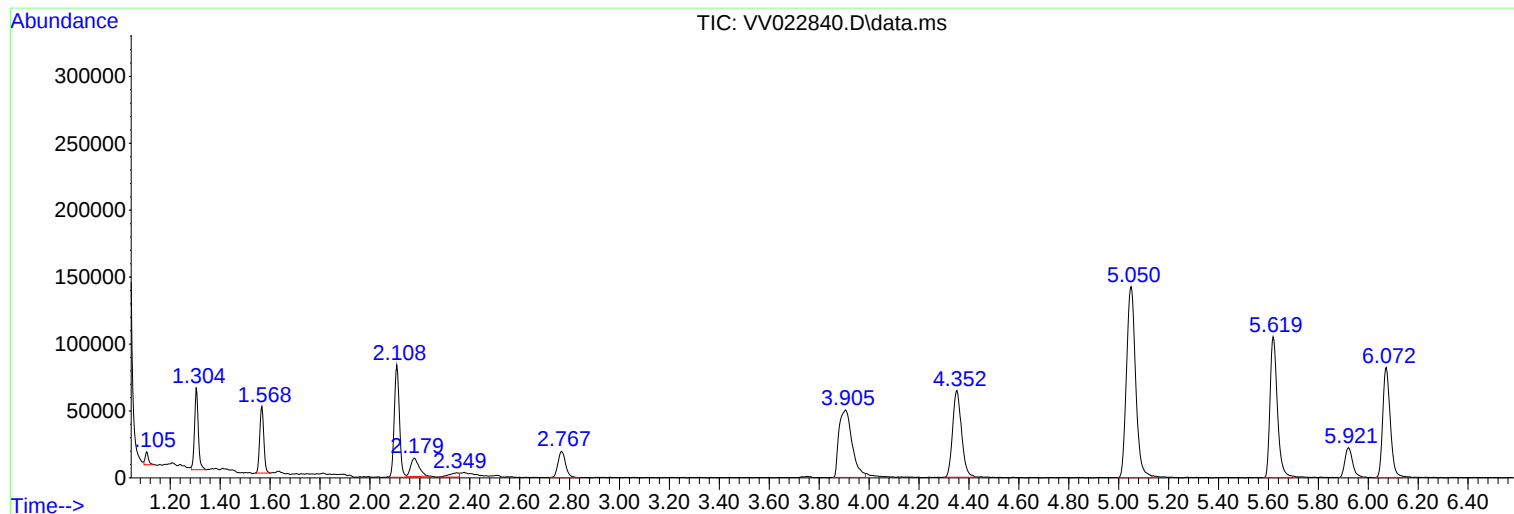

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022840.D
Acq On : 15 Oct 2021 16:43
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022840.D
Acq On : 15 Oct 2021 16:43
Operator : SY/MD
Sample : M4223-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
