

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022844.D
 Acq On : 15 Oct 2021 18:17
 Operator : SY/MD
 Sample : M4223-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG95

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB2	61896	67830	8.42%	1.268%
2	1.568	155	164	179	rBV	51471	61826	7.68%	1.156%
3	2.108	320	332	344	rBV	105330	154719	19.21%	2.892%
4	2.770	524	538	552	rBV4	10129	21598	2.68%	0.404%
5	3.191	655	669	687	rBV	32315	69555	8.64%	1.300%
6	3.291	690	700	718	rVB2	5271	13247	1.64%	0.248%
7	3.912	877	893	922	rBV2	297073	805457	100.00%	15.055%
8	4.358	1012	1032	1063	rBV4	106480	372270	46.22%	6.958%
9	5.050	1229	1247	1268	rBV2	181764	451823	56.10%	8.445%
10	5.140	1269	1275	1292	rVB5	6499	15990	1.99%	0.299%
11	5.619	1411	1424	1451	rBV	129600	264200	32.80%	4.938%
12	5.918	1505	1517	1537	rBV2	83270	167448	20.79%	3.130%
13	6.072	1553	1565	1589	rBV	105459	219830	27.29%	4.109%
14	6.992	1840	1851	1867	rBV	43144	83084	10.32%	1.553%
15	7.320	1939	1953	1970	rBV	205262	364169	45.21%	6.807%
16	7.400	1971	1978	1994	rVB2	8535	16261	2.02%	0.304%
17	7.628	2034	2049	2072	rBV2	26340	49545	6.15%	0.926%
18	7.976	2135	2157	2179	rBV	346753	594654	73.83%	11.114%
19	8.091	2183	2193	2227	rVV	238270	427220	53.04%	7.985%
20	8.853	2418	2430	2452	rBV	203647	340281	42.25%	6.360%
21	10.217	2841	2854	2870	rBV	81241	129496	16.08%	2.420%
22	10.384	2891	2906	2918	rBV2	10081	16055	1.99%	0.300%
23	11.249	3163	3175	3196	rBV	203622	313238	38.89%	5.855%
24	11.625	3281	3292	3310	rBV	208122	330460	41.03%	6.177%




Sum of corrected areas: 5350256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022844.D
Acq On : 15 Oct 2021 18:17
Operator : SY/MD
Sample : M4223-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

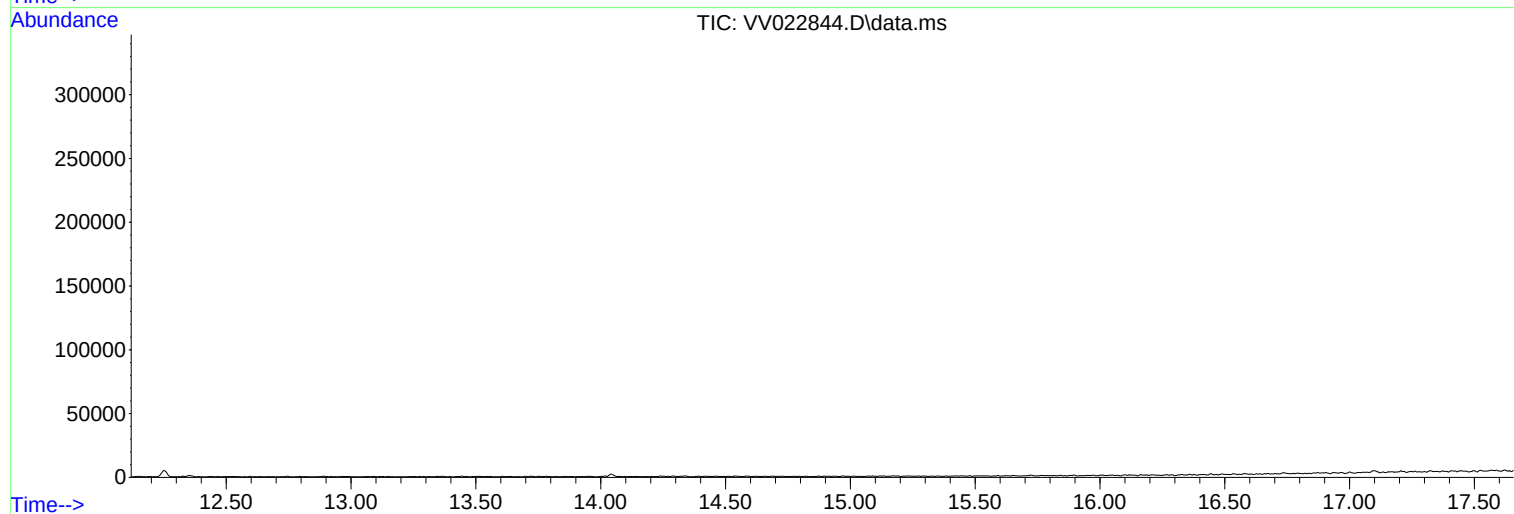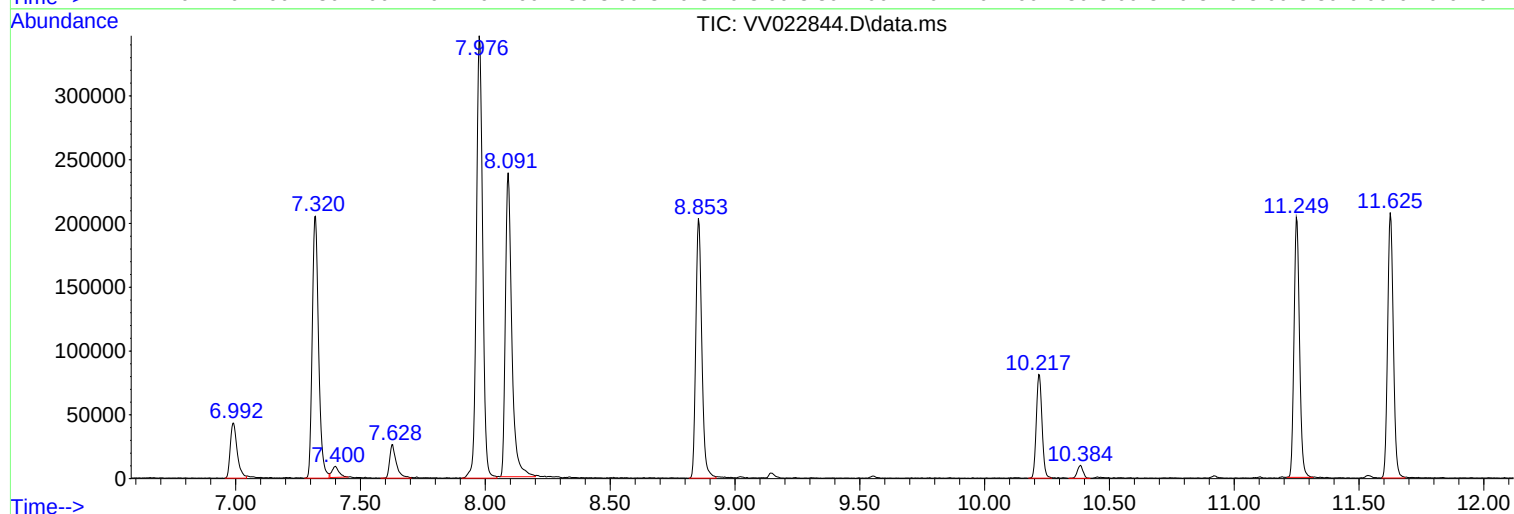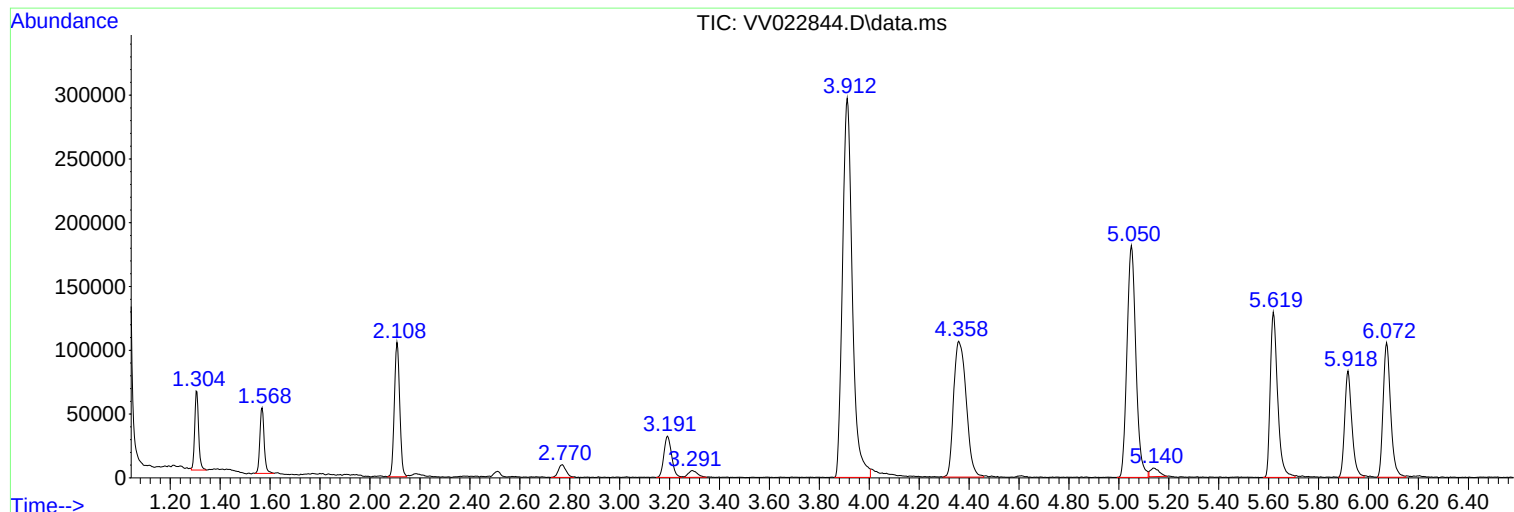

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022844.D
Acq On : 15 Oct 2021 18:17
Operator : SY/MD
Sample : M4223-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022844.D
Acq On : 15 Oct 2021 18:17
Operator : SY/MD
Sample : M4223-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
