

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022845.D
 Acq On : 15 Oct 2021 18:41
 Operator : SY/MD
 Sample : M4223-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG96

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	59793	63555	16.79%	2.007%
2	1.568	157	164	174	rVB	56242	61119	16.15%	1.930%
3	2.108	322	332	345	rBV	86290	123190	32.54%	3.891%
4	3.892	877	887	921	rBV	38305	134167	35.44%	4.238%
5	4.352	1014	1030	1054	rBV2	68349	172589	45.59%	5.451%
6	5.050	1231	1247	1268	rBV3	151836	378544	100.00%	11.956%
7	5.619	1413	1424	1448	rBV	111117	227248	60.03%	7.178%
8	6.072	1552	1565	1596	rVB2	89205	184272	48.68%	5.820%
9	6.992	1839	1851	1871	rBV	37499	72508	19.15%	2.290%
10	7.317	1941	1952	1969	rBV	179996	316678	83.66%	10.002%
11	7.397	1970	1977	1990	rVB	8266	15880	4.20%	0.502%
12	7.629	2039	2049	2066	rBV2	23142	41443	10.95%	1.309%
13	7.940	2136	2146	2156	rBV2	4417	8192	2.16%	0.259%
14	8.092	2182	2193	2224	rBV	201431	356225	94.10%	11.251%
15	8.854	2419	2430	2453	rBV	180093	295349	78.02%	9.329%
16	9.143	2512	2520	2530	rBV4	3124	4937	1.30%	0.156%
17	10.217	2844	2854	2867	rBV2	68662	108896	28.77%	3.440%
18	10.381	2897	2905	2917	rVB3	8475	13566	3.58%	0.428%
19	11.252	3164	3176	3194	rBV	183487	283926	75.00%	8.968%
20	11.625	3281	3292	3314	rBV	190519	298416	78.83%	9.426%
21	12.252	3477	3487	3496	rVB	3327	5339	1.41%	0.169%




Sum of corrected areas: 3166039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022845.D
Acq On : 15 Oct 2021 18:41
Operator : SY/MD
Sample : M4223-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

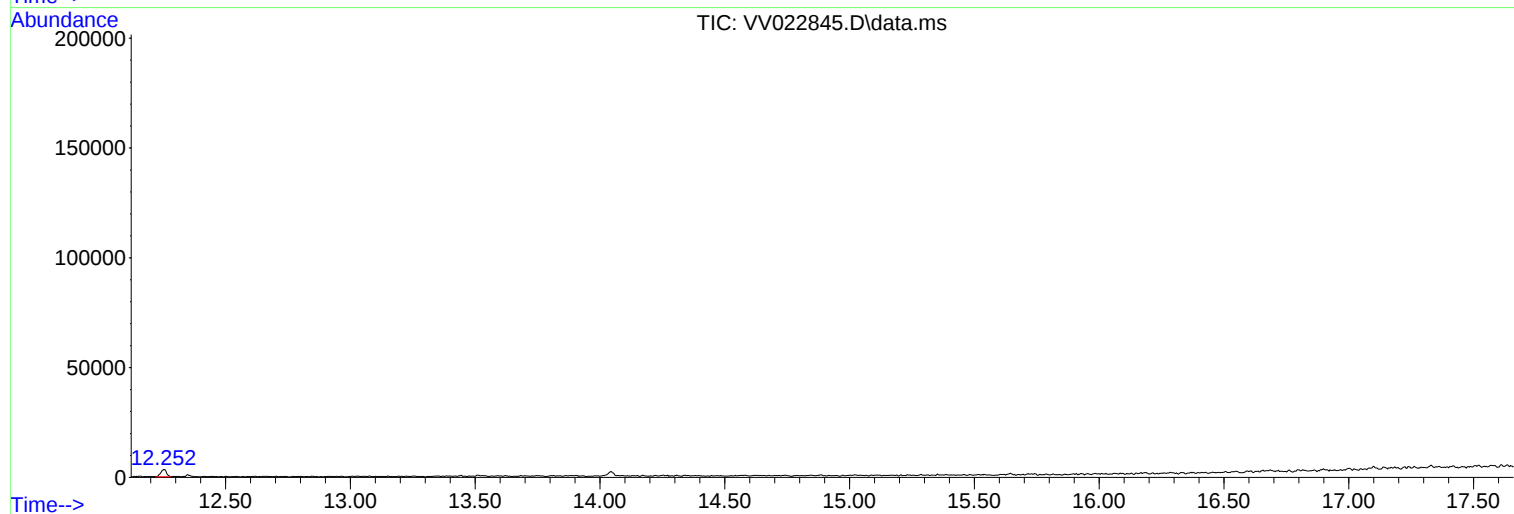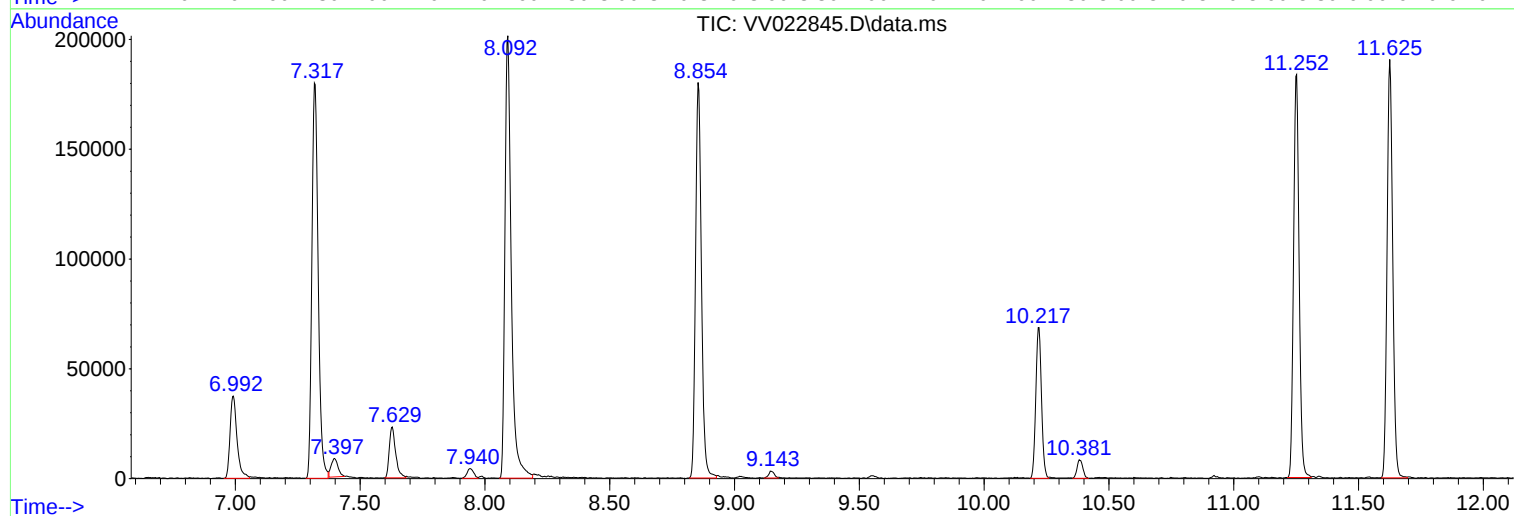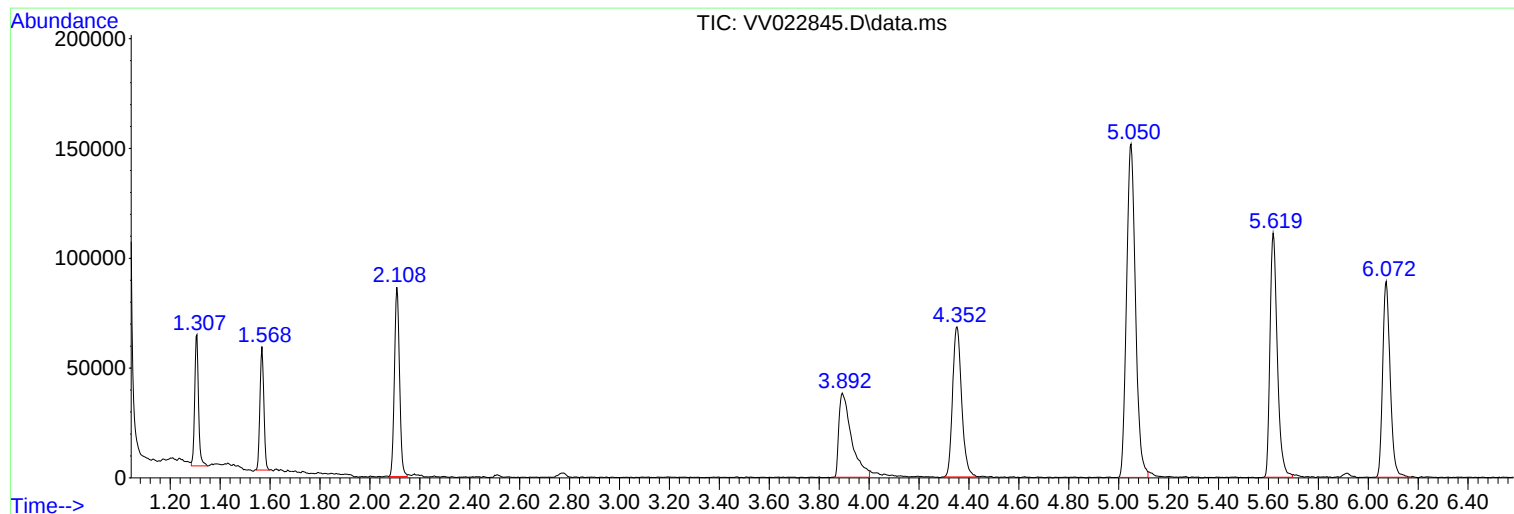

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022845.D
Acq On : 15 Oct 2021 18:41
Operator : SY/MD
Sample : M4223-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022845.D
Acq On : 15 Oct 2021 18:41
Operator : SY/MD
Sample : M4223-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
