

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022846.D
 Acq On : 15 Oct 2021 19:05
 Operator : SY/MD
 Sample : M4223-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG97

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	57290	59891	13.14%	1.593%
2	1.568	156	164	172	rBV	54617	59533	13.06%	1.583%
3	2.108	322	332	349	rBV	99487	145354	31.90%	3.866%
4	2.767	524	537	554	rBV2	29034	63195	13.87%	1.681%
5	3.892	877	887	920	rBV	51523	175662	38.55%	4.672%
6	4.352	1012	1030	1060	rBV2	82375	210921	46.29%	5.610%
7	5.050	1229	1247	1271	rBV3	181181	455685	100.00%	12.120%
8	5.619	1412	1424	1446	rBV	123740	255780	56.13%	6.803%
9	6.072	1550	1565	1591	rBV	107550	226117	49.62%	6.014%
10	6.992	1840	1851	1870	rBV2	44794	83795	18.39%	2.229%
11	7.320	1941	1953	1969	rBV	211196	369734	81.14%	9.834%
12	7.397	1969	1977	1992	rVB	11670	23346	5.12%	0.621%
13	7.625	2039	2048	2066	rBV	26467	48885	10.73%	1.300%
14	7.947	2136	2148	2155	rBV3	5886	10029	2.20%	0.267%
15	8.092	2182	2193	2229	rBV	241781	436692	95.83%	11.615%
16	8.854	2420	2430	2453	rBV	200733	328258	72.04%	8.731%
17	9.146	2513	2521	2534	rBV4	4747	8802	1.93%	0.234%
18	10.217	2842	2854	2867	rBV	82023	129767	28.48%	3.452%
19	10.384	2896	2906	2918	rBV2	9684	15977	3.51%	0.425%
20	11.249	3165	3175	3197	rVB	199040	308665	67.74%	8.210%
21	11.625	3281	3292	3309	rBV	213308	334373	73.38%	8.894%
22	12.249	3475	3486	3499	rBV3	5107	9244	2.03%	0.246%


Sum of corrected areas: 3759705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022846.D
Acq On : 15 Oct 2021 19:05
Operator : SY/MD
Sample : M4223-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

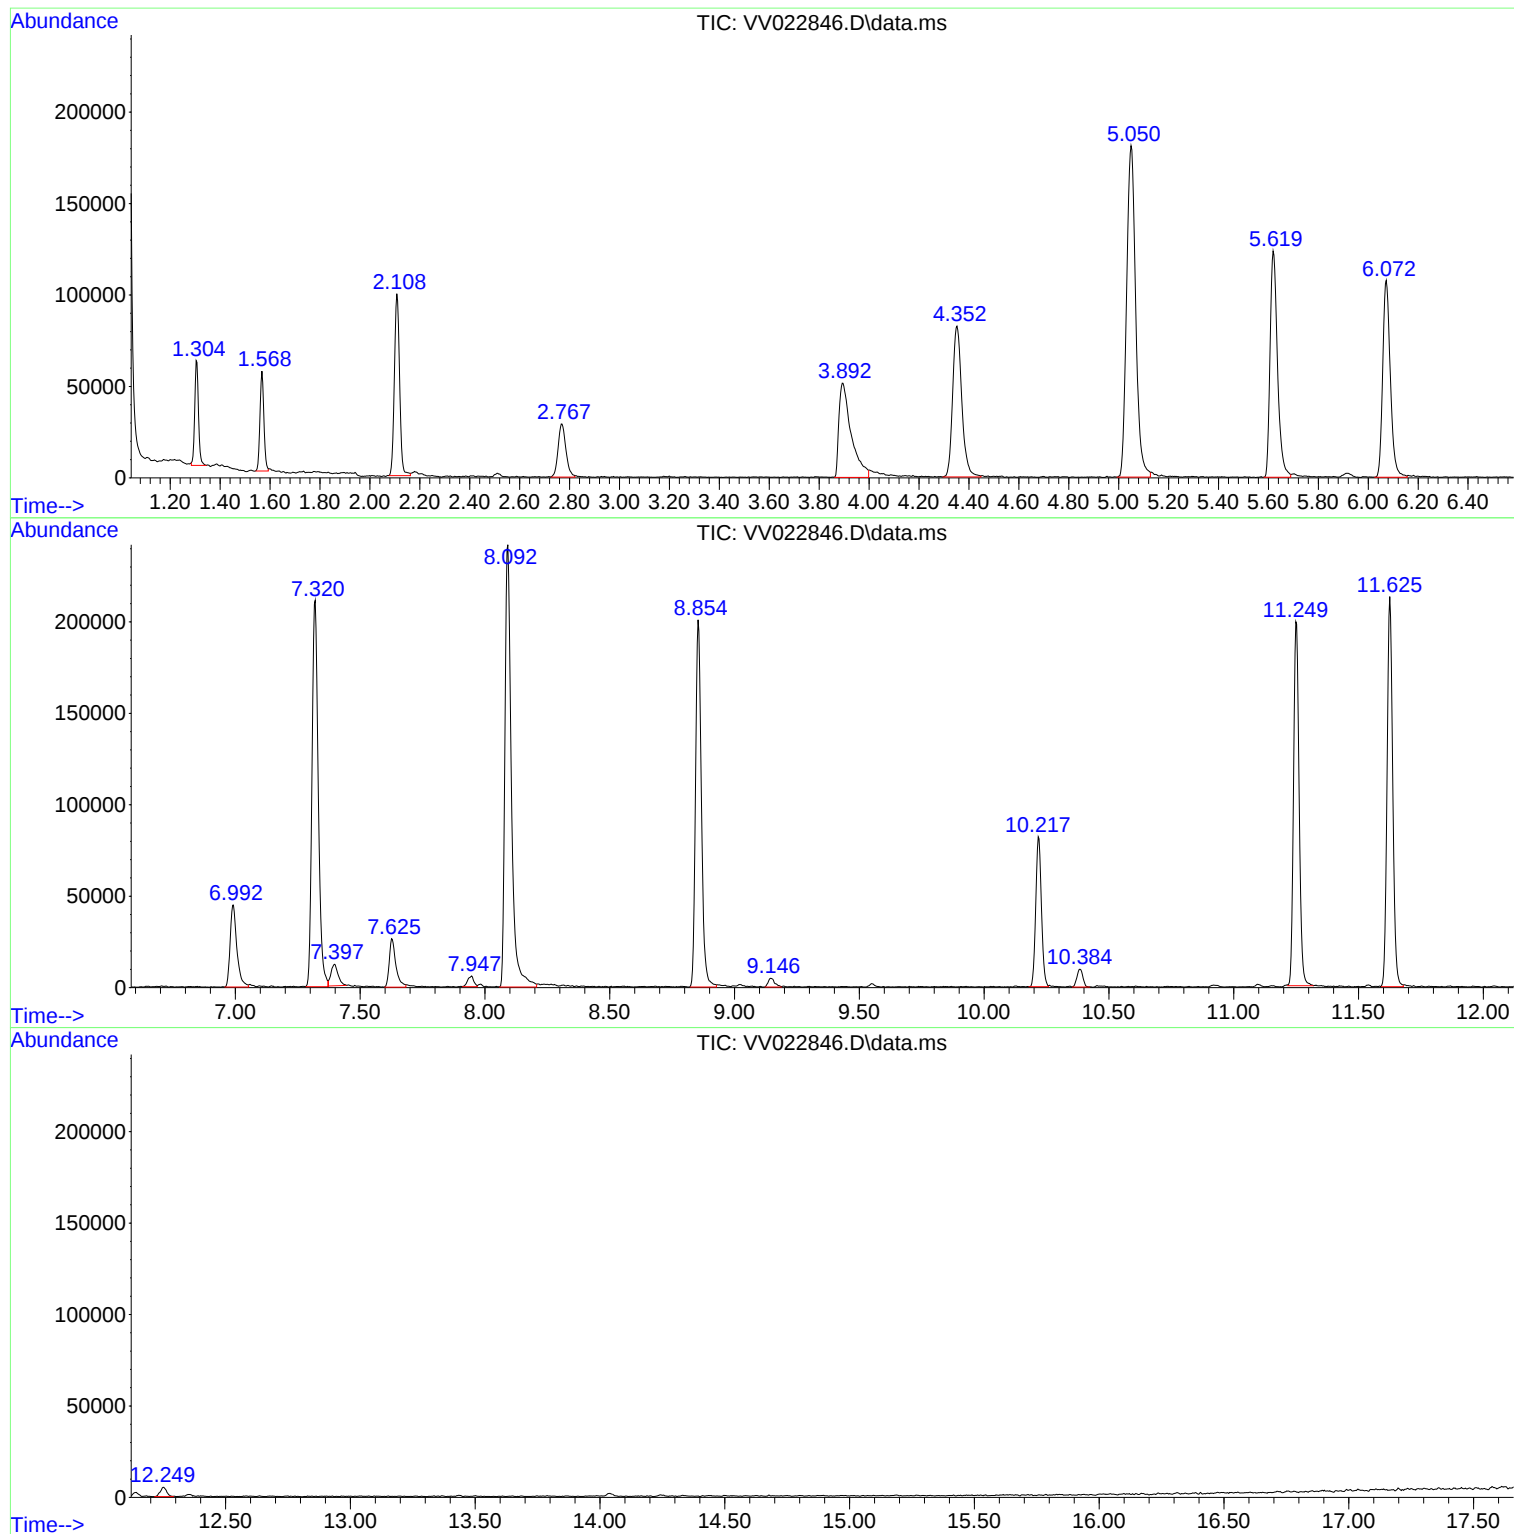

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022846.D
Acq On : 15 Oct 2021 19:05
Operator : SY/MD
Sample : M4223-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022846.D
Acq On : 15 Oct 2021 19:05
Operator : SY/MD
Sample : M4223-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
