

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022847.D
 Acq On : 15 Oct 2021 19:29
 Operator : SY/MD
 Sample : M4223-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG98

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	55979	58361	12.79%	1.389%
2	1.568	156	164	175	rBV	55584	63059	13.82%	1.501%
3	2.108	322	332	347	rBV	99599	146200	32.04%	3.479%
4	2.510	448	457	468	rVB8	3054	5827	1.28%	0.139%
5	2.767	526	537	551	rBV2	18514	38978	8.54%	0.928%
6	3.182	655	666	670	rBV6	3773	6056	1.33%	0.144%
7	3.908	878	892	926	rBV3	76235	272683	59.76%	6.489%
8	4.355	1014	1031	1056	rBV	82511	211974	46.46%	5.045%
9	5.050	1231	1247	1272	rBV3	181957	456269	100.00%	10.859%
10	5.619	1413	1424	1451	rBV	125117	256904	56.31%	6.114%
11	5.921	1505	1518	1538	rVB5	22622	50101	10.98%	1.192%
12	6.072	1551	1565	1585	rBV	107710	222654	48.80%	5.299%
13	6.992	1840	1851	1865	rBV2	43104	81294	17.82%	1.935%
14	7.320	1942	1953	1970	rBV	207904	364276	79.84%	8.669%
15	7.397	1970	1977	1991	rVB2	9555	18863	4.13%	0.449%
16	7.628	2036	2049	2068	rBV3	26459	49222	10.79%	1.171%
17	7.979	2134	2158	2178	rBV	186634	331228	72.59%	7.883%
18	8.091	2181	2193	2226	rBV	239031	433473	95.00%	10.316%
19	8.853	2419	2430	2453	rBV	199816	329891	72.30%	7.851%
20	9.146	2513	2521	2530	rBV4	4467	7372	1.62%	0.175%
21	10.217	2842	2854	2871	rBV	80844	129319	28.34%	3.078%
22	10.384	2896	2906	2916	rBV3	10031	16313	3.58%	0.388%
23	11.252	3165	3176	3196	rVV	197659	307813	67.46%	7.325%
24	11.625	3281	3292	3310	rBV	212529	335100	73.44%	7.975%
25	12.252	3477	3487	3501	rVB2	5242	8721	1.91%	0.208%


Sum of corrected areas: 4201951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022847.D
Acq On : 15 Oct 2021 19:29
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

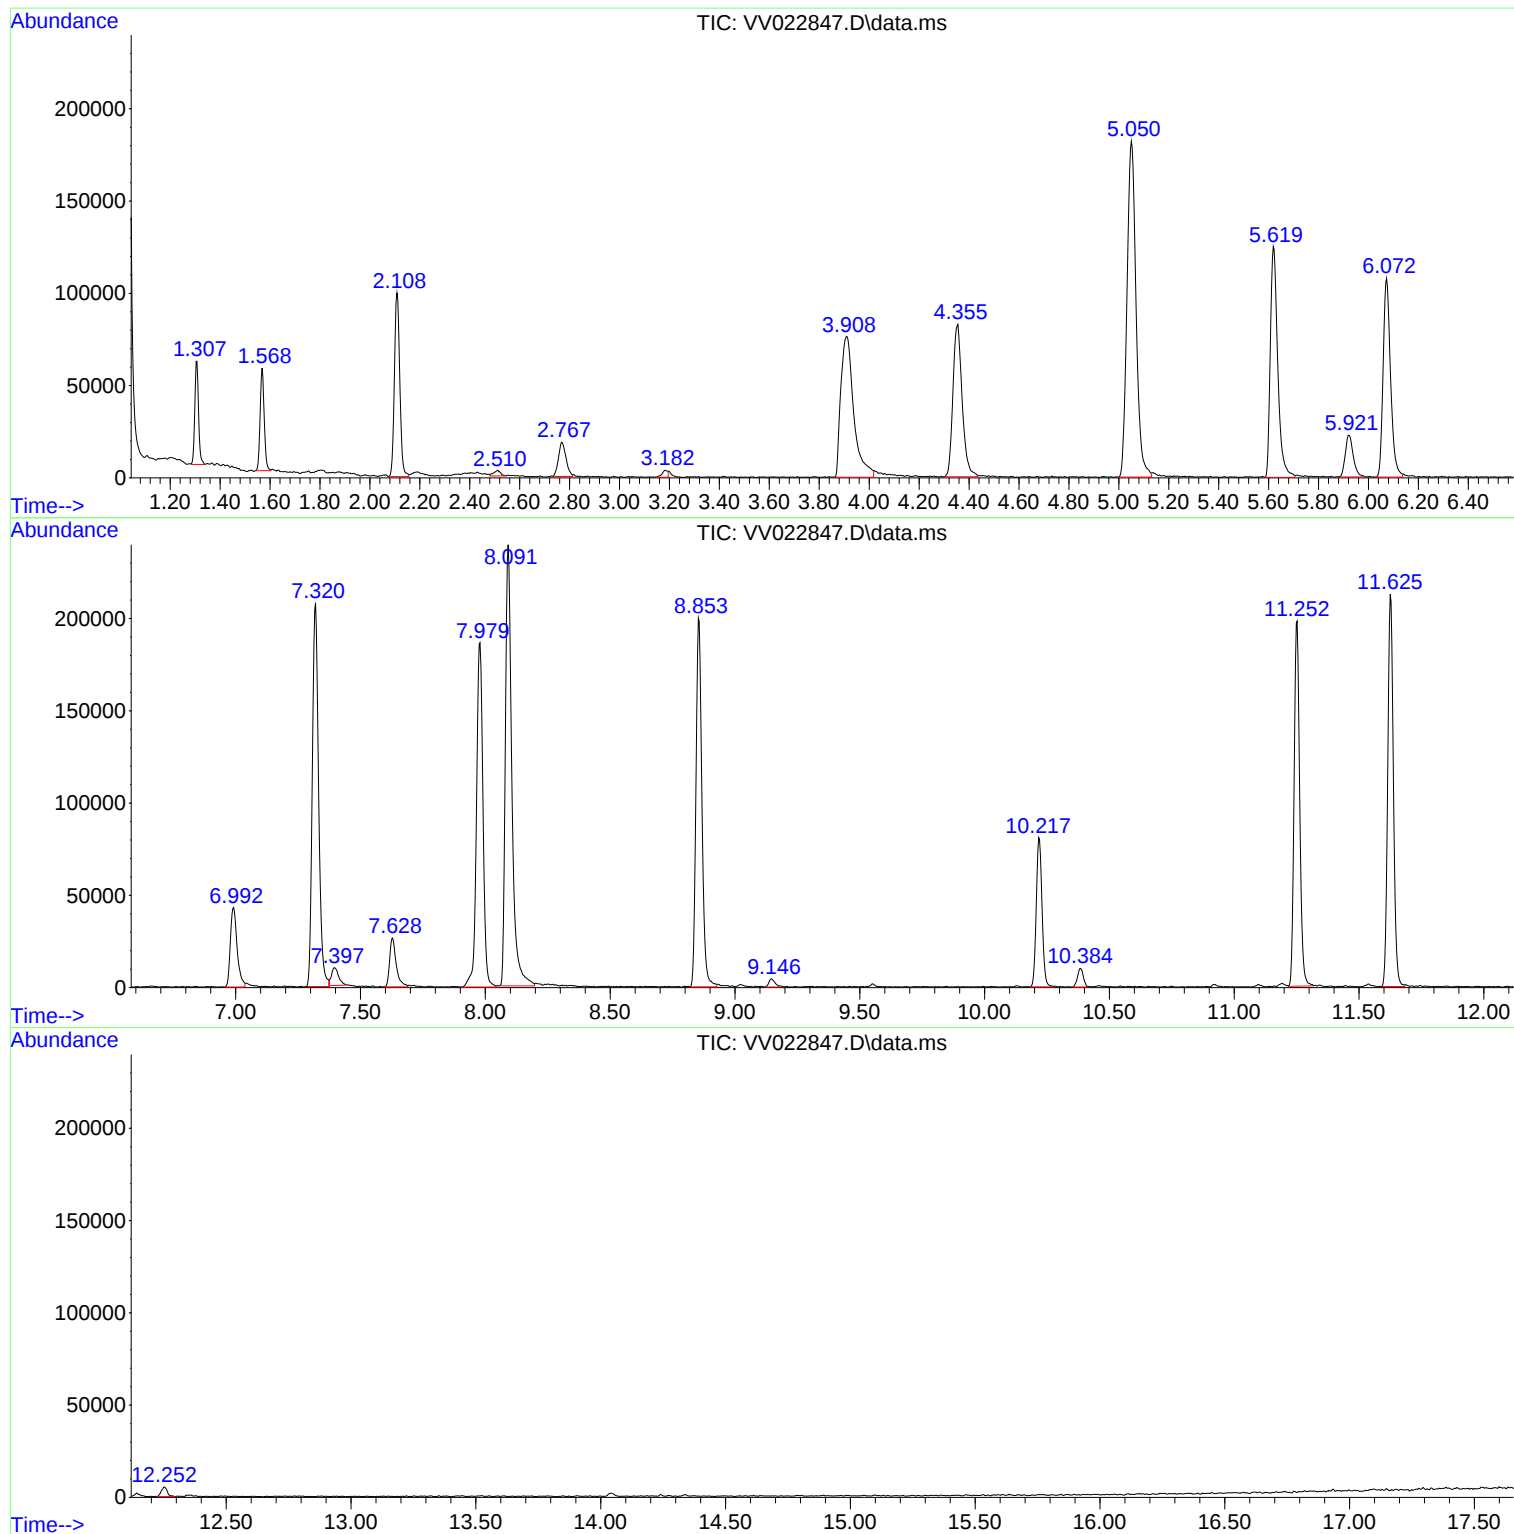

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022847.D
Acq On : 15 Oct 2021 19:29
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022847.D
Acq On : 15 Oct 2021 19:29
Operator : SY/MD
Sample : M4223-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
