

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022849.D
 Acq On : 15 Oct 2021 20:17
 Operator : SY/MD
 Sample : M4223-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	56780	61253	13.80%	1.684%
2	1.568	156	164	177	rVB	46769	55124	12.42%	1.515%
3	2.108	321	332	346	rBV	84559	121292	27.32%	3.334%
4	3.902	878	890	925	rBV2	40637	166510	37.51%	4.577%
5	4.355	1014	1031	1056	rBV2	87331	271726	61.20%	7.468%
6	5.050	1231	1247	1273	rBV3	175511	443962	100.00%	12.202%
7	5.619	1412	1424	1447	rBV	123682	253591	57.12%	6.970%
8	6.072	1552	1565	1590	rBV	104585	216334	48.73%	5.946%
9	6.992	1839	1851	1874	rBV	42841	80950	18.23%	2.225%
10	7.317	1941	1952	1968	rBV	199603	350334	78.91%	9.629%
11	7.397	1971	1977	1993	rVB2	7490	14331	3.23%	0.394%
12	7.629	2039	2049	2064	rBV	26466	46821	10.55%	1.287%
13	7.944	2138	2147	2151	rBV2	4547	7343	1.65%	0.202%
14	7.979	2151	2158	2173	rVB2	18520	31848	7.17%	0.875%
15	8.092	2181	2193	2228	rBV	229829	428912	96.61%	11.789%
16	8.854	2419	2430	2450	rBV	198417	325625	73.35%	8.950%
17	10.220	2843	2855	2872	rBV	78252	125127	28.18%	3.439%
18	10.384	2897	2906	2915	rBV3	7042	11532	2.60%	0.317%
19	11.249	3165	3175	3195	rBV	192681	299270	67.41%	8.225%
20	11.625	3280	3292	3312	rBV	205925	321033	72.31%	8.824%
21	12.252	3477	3487	3495	rVB4	3476	5431	1.22%	0.149%


Sum of corrected areas: 3638349

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022849.D
Acq On : 15 Oct 2021 20:17
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

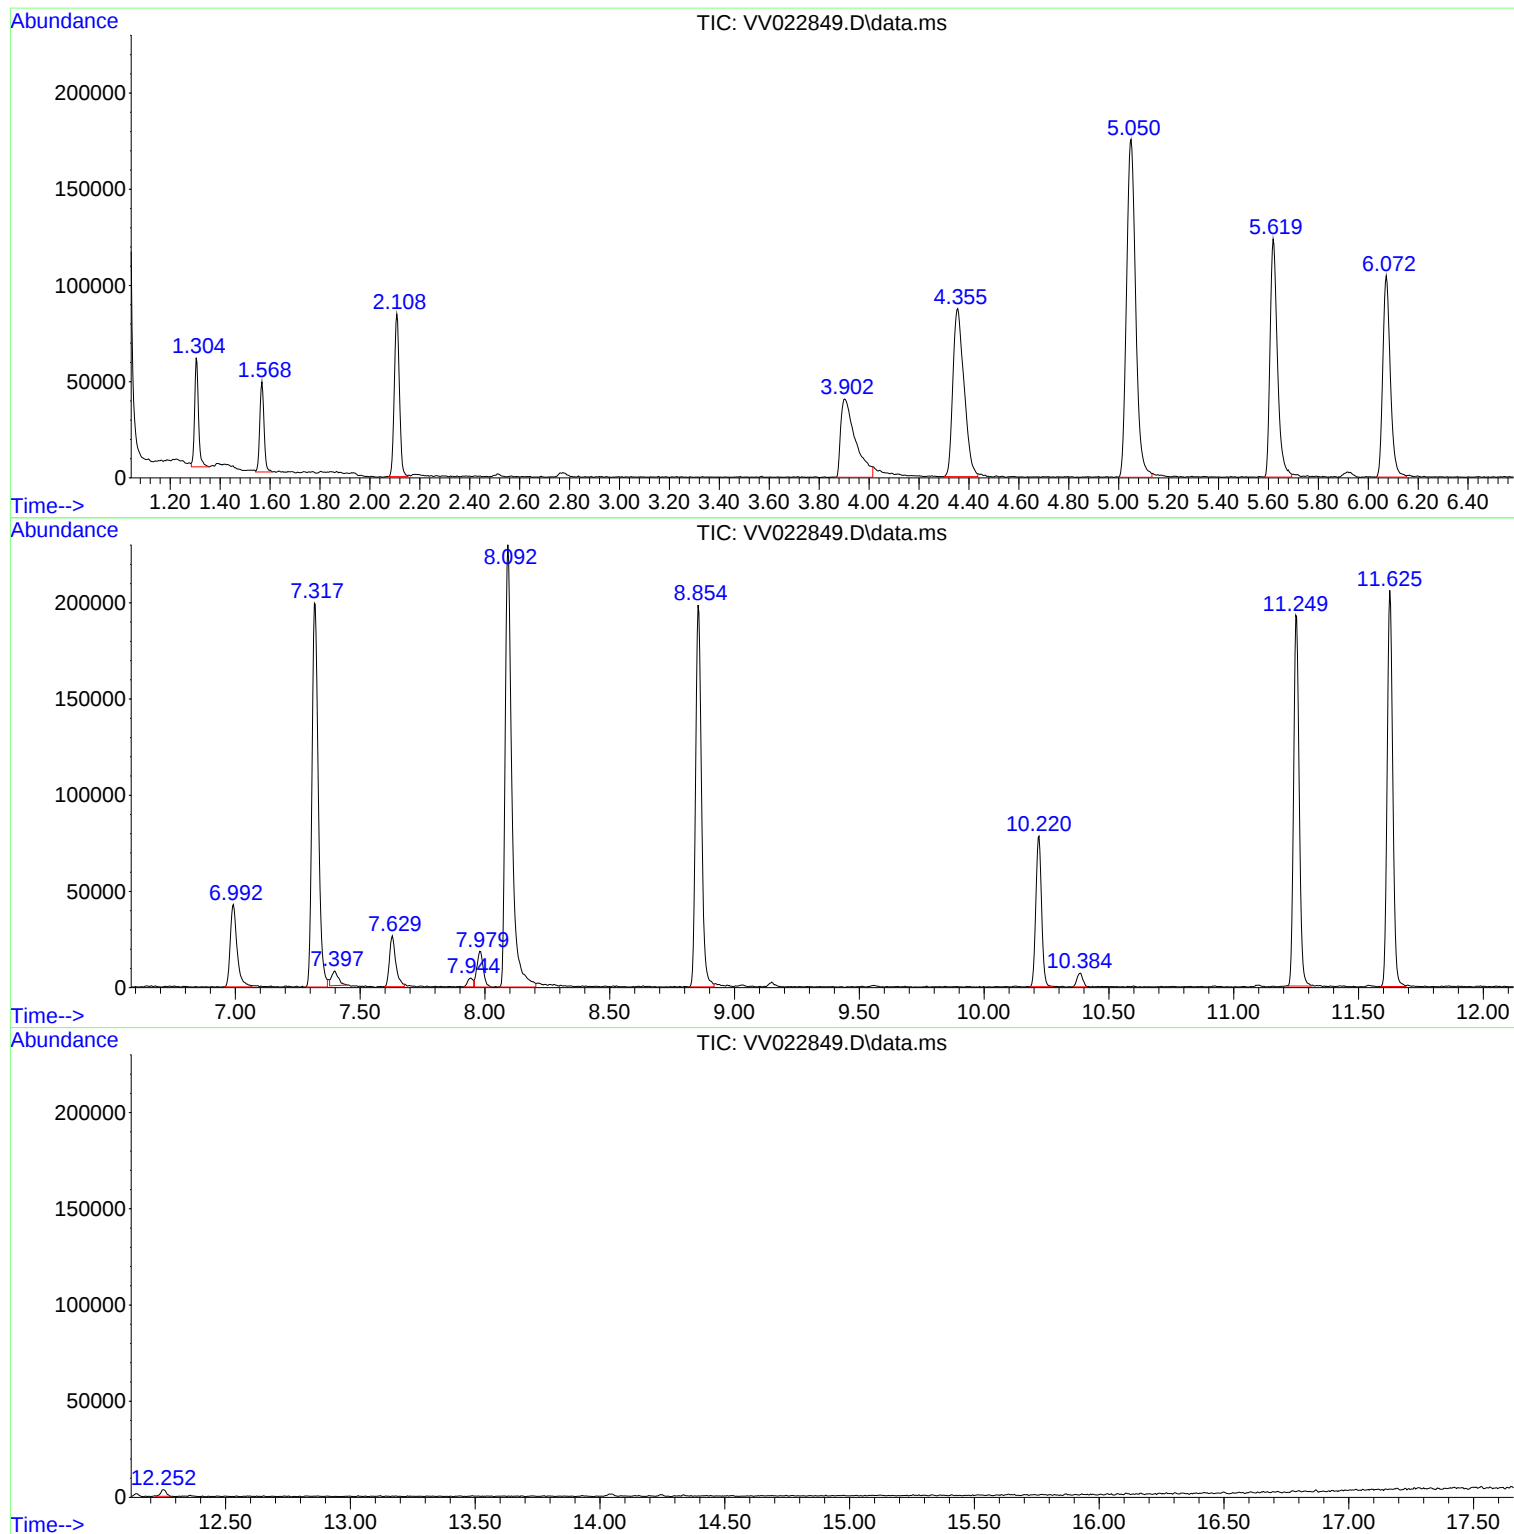

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022849.D
Acq On : 15 Oct 2021 20:17
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
Data File : VV022849.D
Acq On : 15 Oct 2021 20:17
Operator : SY/MD
Sample : M4223-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
