


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101521\
 Data File : VV022828.D
 Acq On : 15 Oct 2021 11:10
 Operator : SY/MD
 Sample : BFB216
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB216

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 19 04:07:06 2021

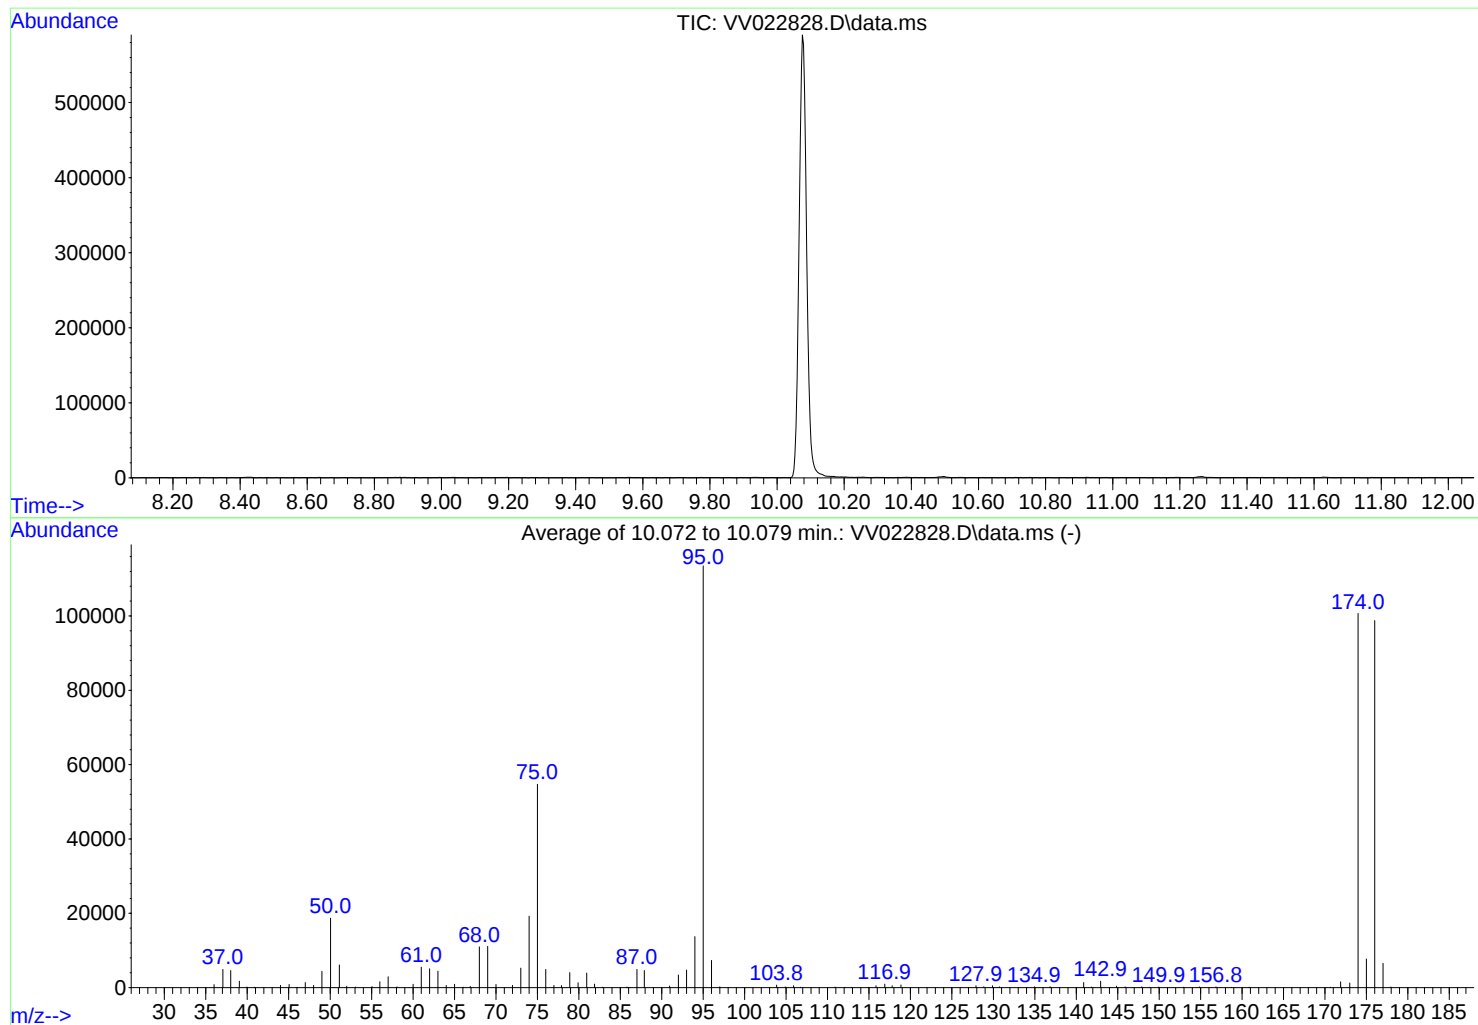

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	18669	PASS
75	95	30	80	48.2	54717	PASS
95	95	100	100	100.0	113496	PASS
96	95	5	9	6.5	7341	PASS
173	174	0.00	2	1.2	1258	PASS
174	95	50	120	88.7	100680	PASS
175	174	5	9	7.7	7709	PASS
176	174	95	105	98.1	98771	PASS
177	176	5	10	6.6	6543	PASS

m/z	Abundance
44.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	778.0
37.00	4854.0
38.00	4616.0
39.10	1665.0
40.00	148.0
40.90	103.0
44.00	789.0
45.00	825.0
45.90	137.0
47.00	1280.0
48.00	641.0
49.00	4218.0
50.10	18208.0
51.10	5856.0
52.00	344.0
53.00	173.0
55.00	301.0
56.00	1600.0
57.00	2865.0
58.10	202.0
60.00	898.0
61.00	5419.0
62.00	5092.0
63.00	4188.0
64.00	678.0
65.00	904.0
66.10	146.0
66.90	302.0
68.00	10759.0
69.00	10884.0
70.00	817.0
72.00	539.0
73.00	5073.0
74.00	18168.0
75.00	52328.0
76.00	4669.0
77.00	613.0
77.90	520.0
78.90	3831.0
79.90	1231.0
81.00	3711.0
81.90	928.0
82.80	112.0
85.80	198.0
87.00	4741.0
87.90	4531.0
91.00	431.0
92.00	3260.0
93.00	4609.0
94.00	13095.0
95.00	108832.0
96.00	7273.0
97.00	161.0
103.90	641.0
104.90	234.0
105.90	552.0
106.70	141.0
110.90	183.0
112.90	166.0
115.90	534.0
116.90	903.0
117.80	508.0
118.80	767.0
127.00	105.0
127.90	429.0
128.90	251.0
129.90	572.0
130.80	185.0
134.90	176.0
136.80	185.0
140.90	1299.0
141.90	204.0
143.00	1732.0
144.80	382.0
145.90	236.0
147.90	194.0
150.00	177.0
151.70	107.0
153.00	161.0
154.80	220.0
156.80	215.0
158.80	105.0
160.90	140.0
170.80	121.0
171.90	1537.0
173.00	1169.0
174.00	94072.0
175.00	7450.0
176.00	92184.0
177.00	6180.0
178.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	865.0
37.10	5138.0
38.00	4858.0
39.00	1828.0
39.90	154.0
40.90	134.0
44.00	871.0
45.10	869.0
46.10	145.0
47.00	1420.0
48.00	635.0
49.00	4538.0
50.10	19240.0
51.10	6351.0
52.00	406.0
53.10	208.0
55.10	311.0
56.00	1651.0
57.00	3050.0
58.00	239.0
60.00	953.0
61.00	5682.0
62.00	5215.0
63.00	4657.0
64.00	645.0
65.00	935.0
66.10	143.0
66.90	379.0
68.00	11282.0
69.00	11483.0
70.00	872.0
72.00	601.0
73.00	5468.0
74.00	20064.0
75.00	56776.0
76.00	5112.0
77.00	612.0
77.90	570.0
78.90	4209.0
79.90	1394.0
80.90	4010.0
81.90	983.0
82.90	124.0
85.80	177.0
86.00	159.0
87.00	5139.0
87.90	4670.0
90.90	451.0
92.00	3499.0
93.00	4814.0
94.00	14270.0
95.00	117392.0
96.00	7612.0
97.00	214.0
103.80	723.0
104.90	221.0
105.90	547.0
106.80	151.0
110.90	194.0
112.10	112.0
112.80	133.0
114.90	109.0
115.90	529.0
116.90	990.0
117.80	510.0
118.80	748.0
127.90	559.0
128.90	255.0
129.90	528.0
130.70	215.0
135.00	198.0
136.80	264.0
140.90	1420.0
141.80	200.0
142.90	1775.0
144.10	111.0
144.90	404.0
145.90	246.0
147.90	239.0
148.80	112.0
150.00	167.0
153.00	160.0
154.90	227.0
156.90	230.0
160.80	156.0
170.60	133.0
171.90	1603.0
173.00	1320.0
174.00	103848.0
175.00	7982.0
176.00	102312.0
177.00	6739.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

178.00

196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	836.0
37.00	4740.0
38.00	4370.0
39.00	1744.0
39.90	177.0
40.90	106.0
44.00	766.0
45.10	915.0
46.10	175.0
47.00	1391.0
48.00	592.0
49.00	4366.0
50.00	18560.0
51.10	6148.0
52.00	444.0
53.10	183.0
55.10	281.0
56.00	1488.0
57.00	2861.0
58.00	200.0
60.00	918.0
61.00	5374.0
62.00	4968.0
63.00	4437.0
64.00	547.0
65.00	839.0
66.00	129.0
66.90	381.0
68.00	10848.0
69.00	10963.0
70.00	888.0
72.00	632.0
73.00	5234.0
74.00	19568.0
75.00	55048.0
76.00	5004.0
77.00	548.0
77.90	536.0
78.90	4119.0
79.90	1372.0
80.90	4024.0
81.90	897.0
82.90	125.0
85.70	124.0
86.20	166.0
87.00	4881.0
87.90	4607.0
90.90	437.0
92.00	3436.0
93.00	4806.0
94.00	13827.0
95.00	114264.0
96.00	7138.0
97.00	256.0
103.80	681.0
104.90	178.0
105.90	487.0
106.80	135.0
110.90	158.0
112.10	131.0
114.90	145.0
115.80	440.0
116.90	918.0
117.80	493.0
118.90	686.0
127.90	594.0
128.80	222.0
129.90	445.0
130.70	213.0
134.90	230.0
136.90	314.0
140.90	1370.0
141.80	182.0
142.90	1608.0
144.10	135.0
144.90	399.0
145.90	215.0
146.80	129.0
147.90	270.0
148.80	127.0
149.90	124.0
152.90	145.0
154.90	228.0
156.90	271.0
158.70	110.0
159.20	119.0
160.80	160.0
170.60	152.0
171.90	1506.0
173.00	1286.0
174.00	104120.0
175.00	7694.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

176.00101816.0

177.006710.0

177.90200.0

Instrument :
MSVOA_V

ClientSampleId :
BFB216