

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101618\
 Data File : VV008299.D
 Acq On : 16 Oct 2018 15:25
 Operator : SY/MD
 Sample : J5406-11
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5

Quant Time: Oct 19 11:40:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 17 02:28:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	98254	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88412	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	34254	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29879	5.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.60%
7) Chloroethane-d5	1.59	69	22908	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.60%
11) 1,1-Dichloroethene-d2	2.13	63	43672	4.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.00%
20) 2-Butanone-d5	3.97	46	94732	50.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.74%
24) Chloroform-d	4.41	84	58546	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.09	65	30523	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.10	84	129109	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
36) 1,2-Dichloropropane-d6	6.12	67	43560	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.36	98	111288	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.67	79	14703	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.14	63	52639	42.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24400	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	33404	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	8011	7.950 ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101618\
Data File : VV008299.D
Acq On : 16 Oct 2018 15:25
Operator : SY/MD
Sample : J5406-11
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK5

Quant Time: Oct 19 11:40:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 17 02:28:08 2018
Response via : Initial Calibration

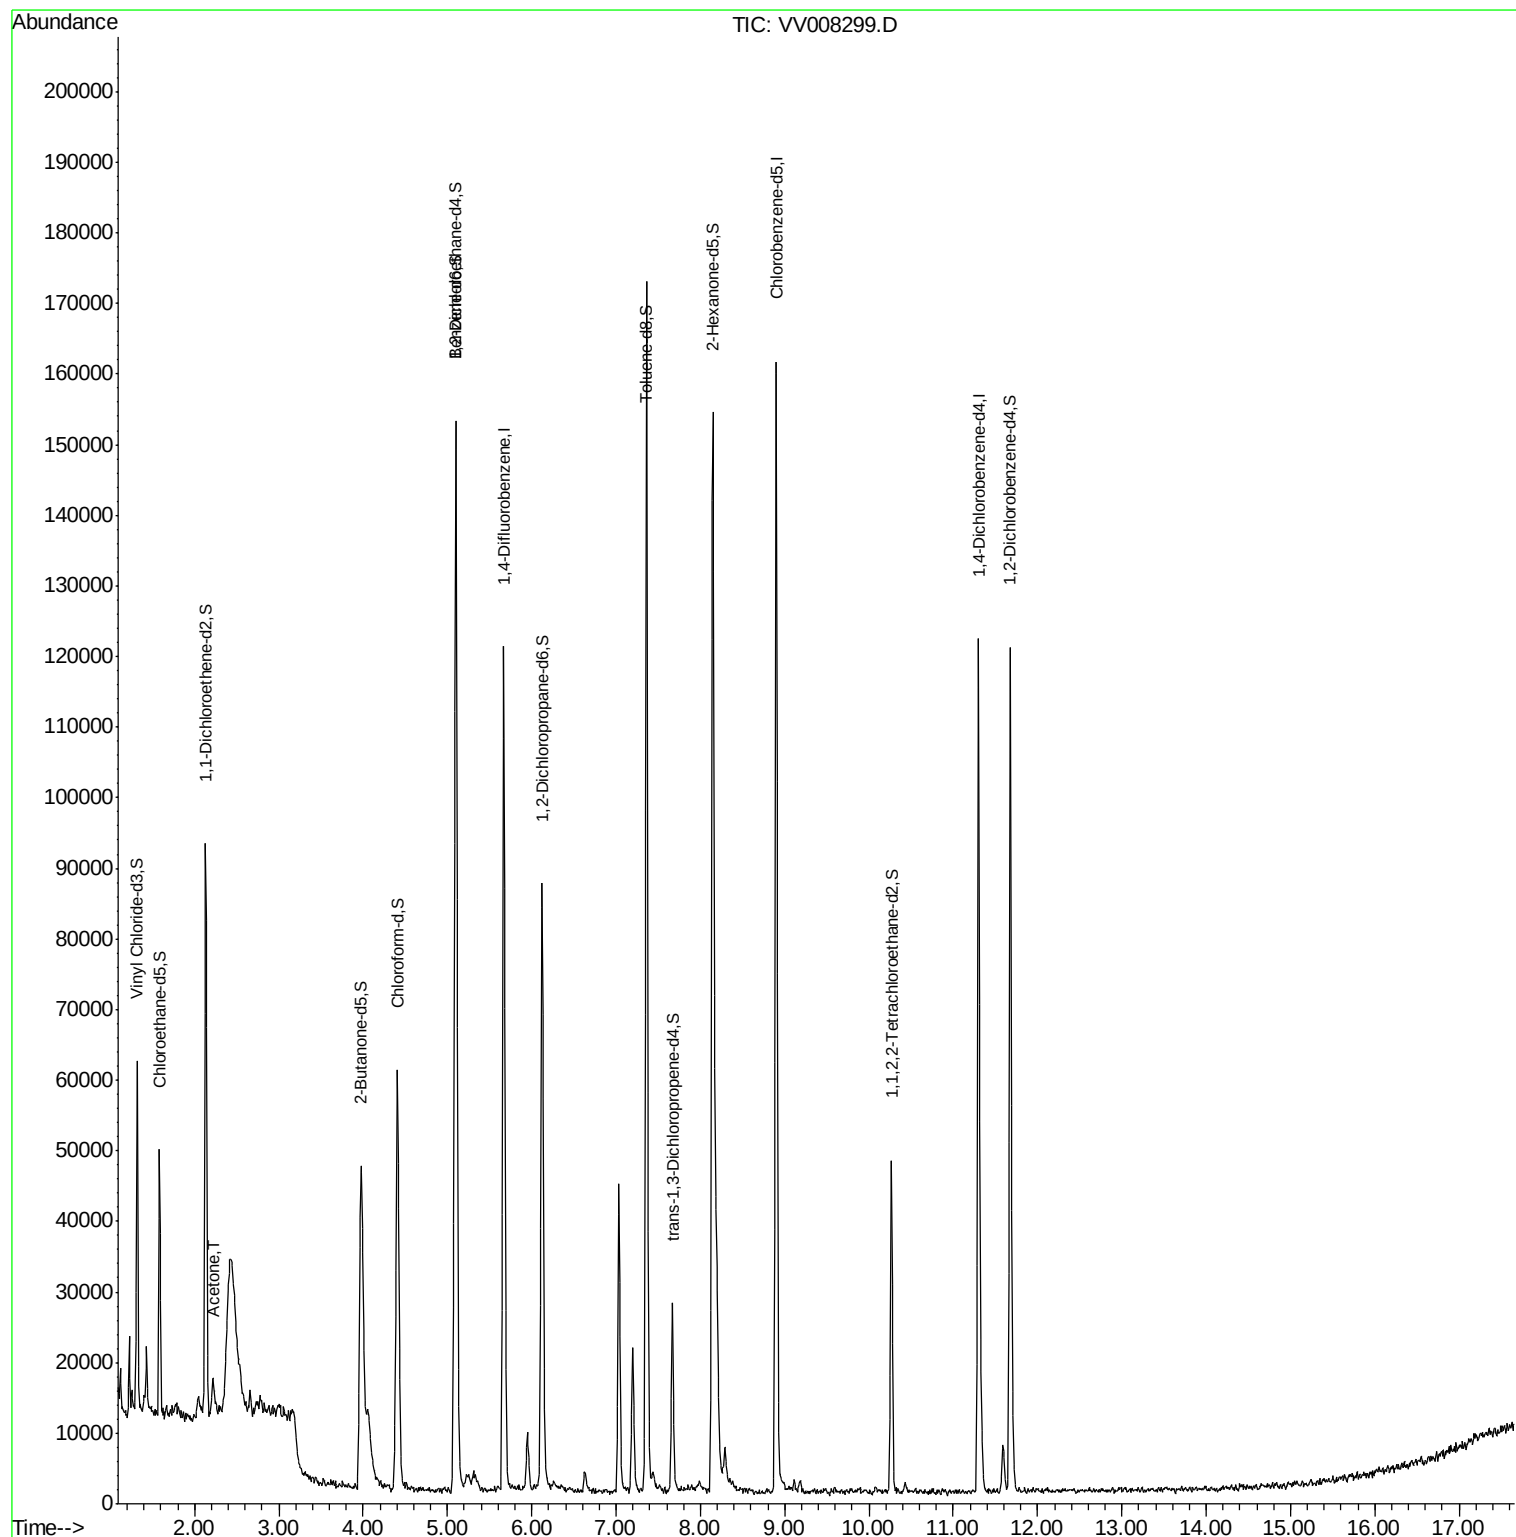

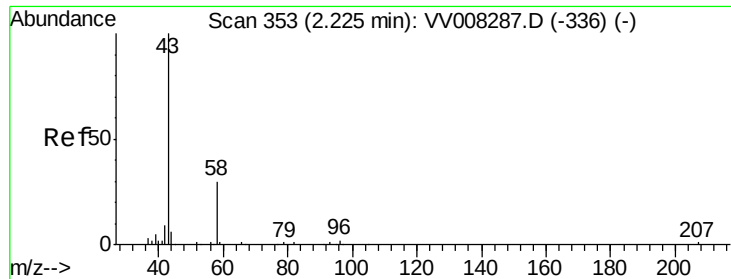

#13

Acetone

Concen: 7.950 ug/L

RT: 2.22 min Scan# 352

Delta R.T. -0.00 min

Lab File: VV008299.D

Acq: 16 Oct 2018 15:25

Instrument :
MSVOA_V
ClientSampleId :
C0AK5

Tot Ion: 43 Resp: 8011

Ion Ratio Lower Upper

43 100

58 41.4 0.0 62.0

