

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101618\
 Data File : VV008300.D
 Acq On : 16 Oct 2018 15:54
 Operator : SY/MD
 Sample : J5406-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Quant Time: Oct 19 11:40:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 17 02:28:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	84344	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	73775	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	28219	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22694	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.59	69	18333	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.13	63	32897	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	3.98	46	76841	48.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.12%
24) Chloroform-d	4.41	84	46521	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.09	65	24789	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
32) Benzene-d6	5.10	84	101444	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.12	67	34841	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	90546	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.67	79	11158	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
46) 2-Hexanone-d5	8.14	63	42857	41.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.64%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	19227	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	26420	4.93	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.60%


Target Compounds					Ovalue
17) Methyl tert-butyl Ether	2.82	73	16427	1.427 ug/L	99
34) Trichloroethene	5.96	95	2841	0.412 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101618\
Data File : VV008300.D
Acq On : 16 Oct 2018 15:54
Operator : SY/MD
Sample : J5406-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Time: Oct 19 11:40:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 17 02:28:08 2018
Response via : Initial Calibration




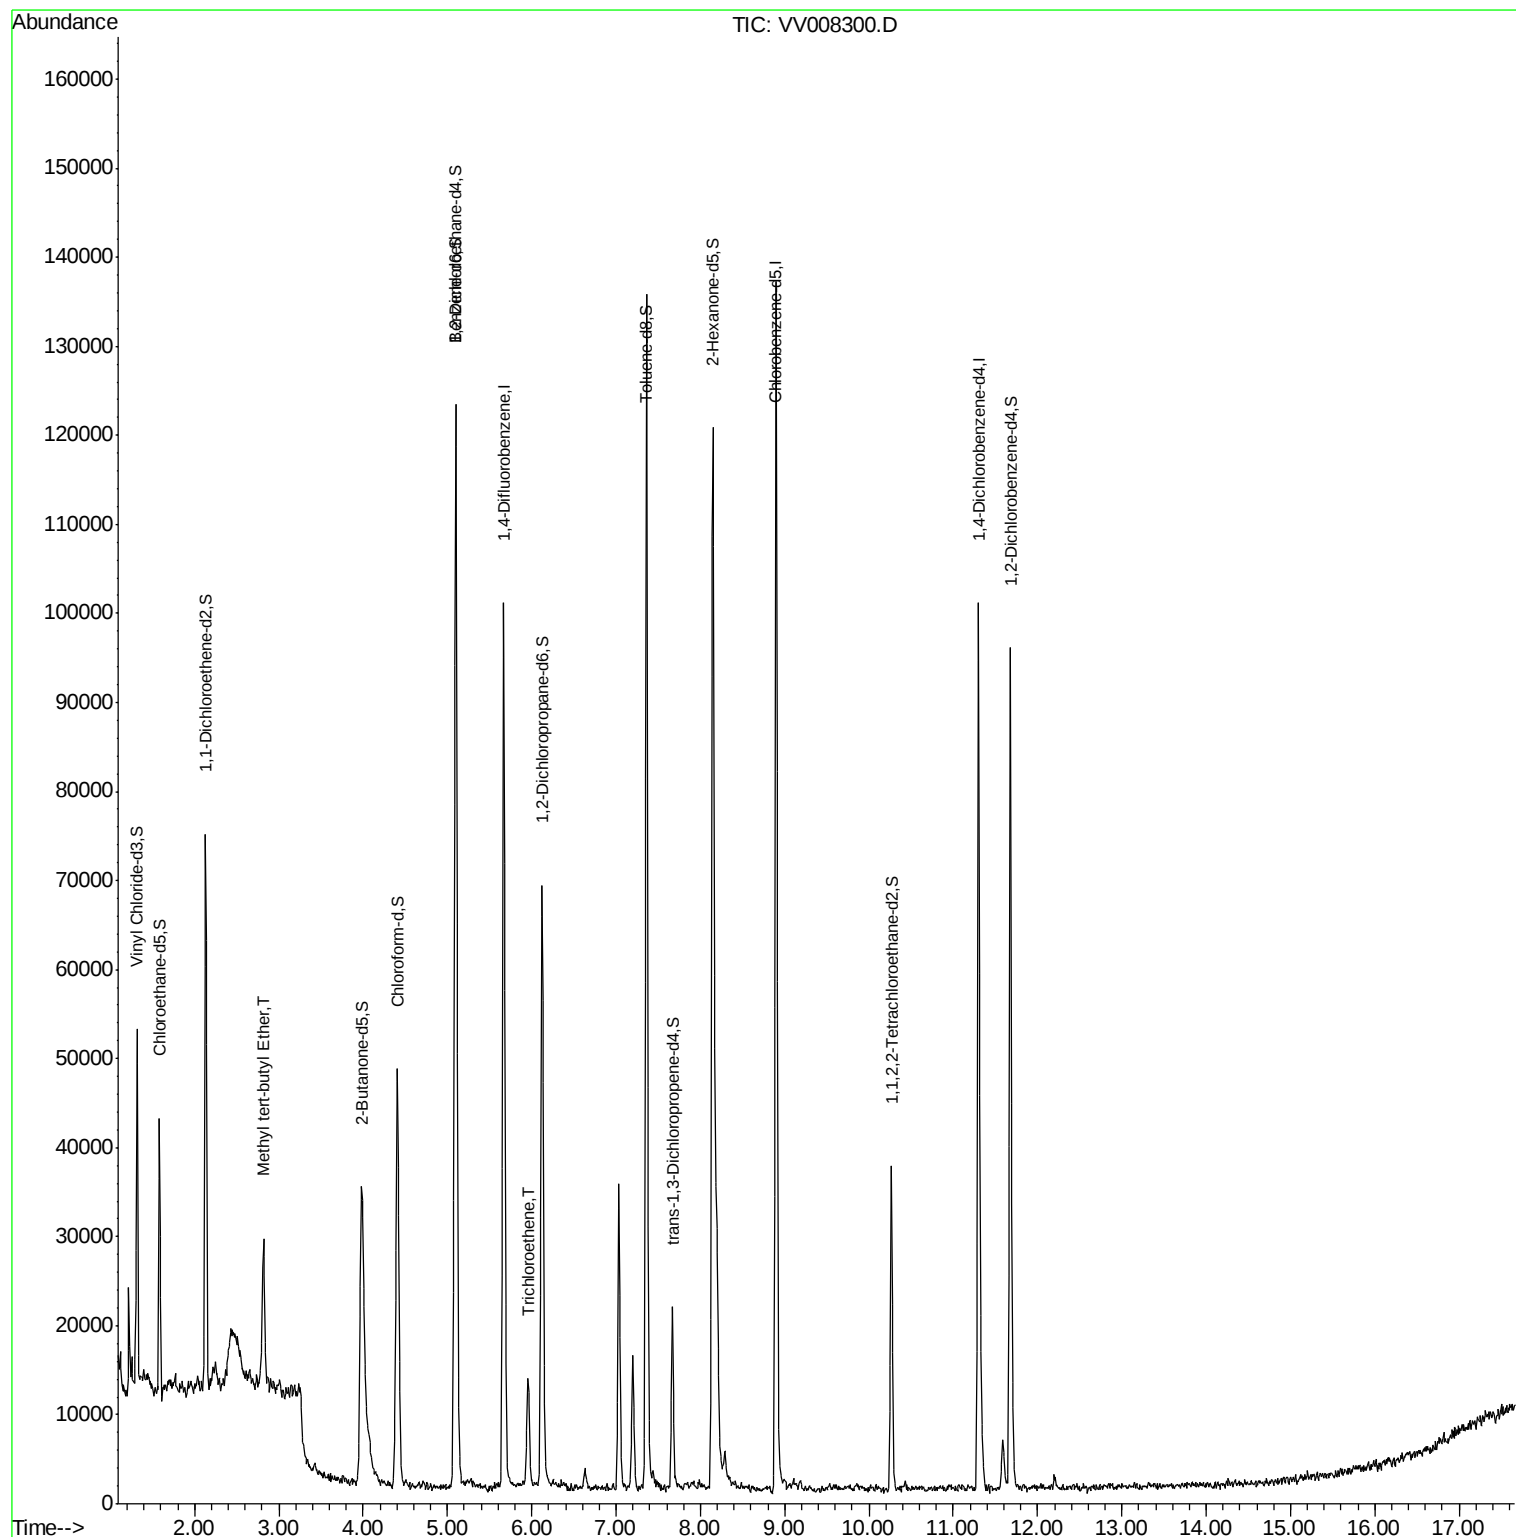


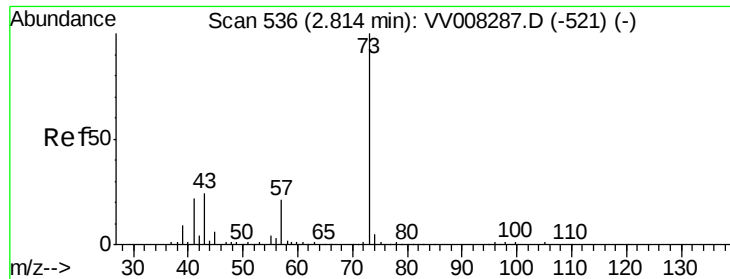

#17
Methvl tert-butvl Ether
Concen: 1.427 ug/L
RT: 2.82 min Scan# 537
Delta R.T. 0.00 min
Lab File: VV008300.D
Acq: 16 Oct 2018 15:54

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Tot Ion: 73 Resp: 16427
Ion Ratio Lower Upper
73 100
43 23.8 19.0 28.6
57 21.5 18.2 27.2

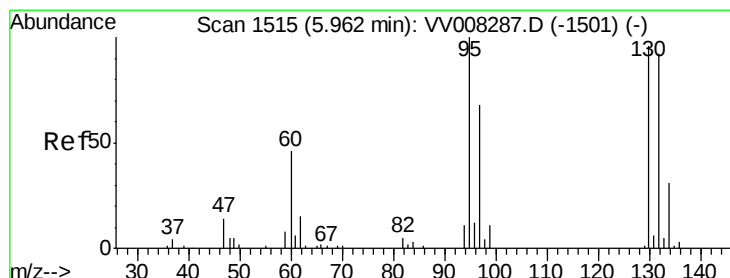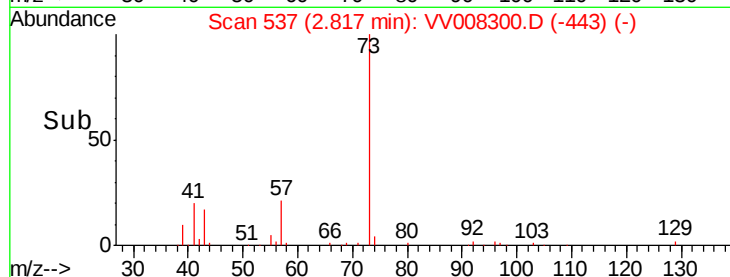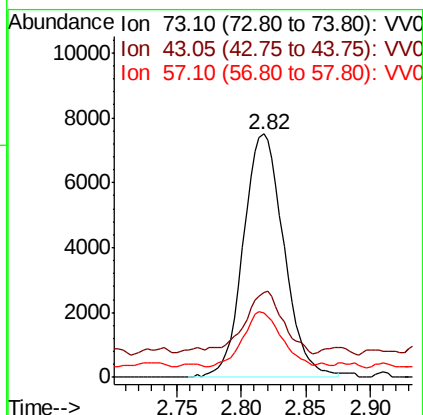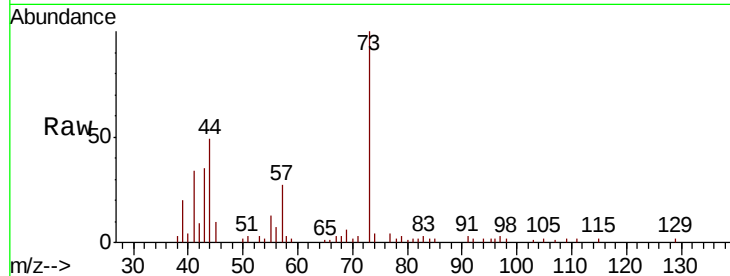

#34
Trichloroethene
Concen: 0.412 ug/L
RT: 5.96 min Scan# 1516
Delta R.T. 0.00 min
Lab File: VV008300.D
Acq: 16 Oct 2018 15:54

Tgt Ion: 95 Resp: 2841
Ion Ratio Lower Upper
95 100
97 70.9 44.4 82.4
132 89.7 60.4 112.2
130 94.7 65.5 121.7

