

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101618\
 Data File : VV008302.D
 Acq On : 16 Oct 2018 17:19
 Operator : SY/MD
 Sample : J5406-13
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK7

Quant Time: Oct 19 11:41:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 17 02:28:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	82680	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	73548	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	28524	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22813	4.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.60%
7) Chloroethane-d5	1.58	69	18011	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.13	63	32449	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.98	46	76825	49.02	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.04%
24) Chloroform-d	4.41	84	46574	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.09	65	25220	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.10	84	102971	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.12	67	35263	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.36	98	90648	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
43) trans-1,3-Dichloropropene-	7.67	79	11379	3.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.20%
46) 2-Hexanone-d5	8.14	63	43848	42.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.82%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	20005	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	26826	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
17) Methyl tert-butyl Ether	2.82	73	17160	1.521 ug/L	98
34) Trichloroethene	5.96	95	4382	0.638 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101618\
Data File : VV008302.D
Acq On : 16 Oct 2018 17:19
Operator : SY/MD
Sample : J5406-13
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Quant Time: Oct 19 11:41:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 17 02:28:08 2018
Response via : Initial Calibration

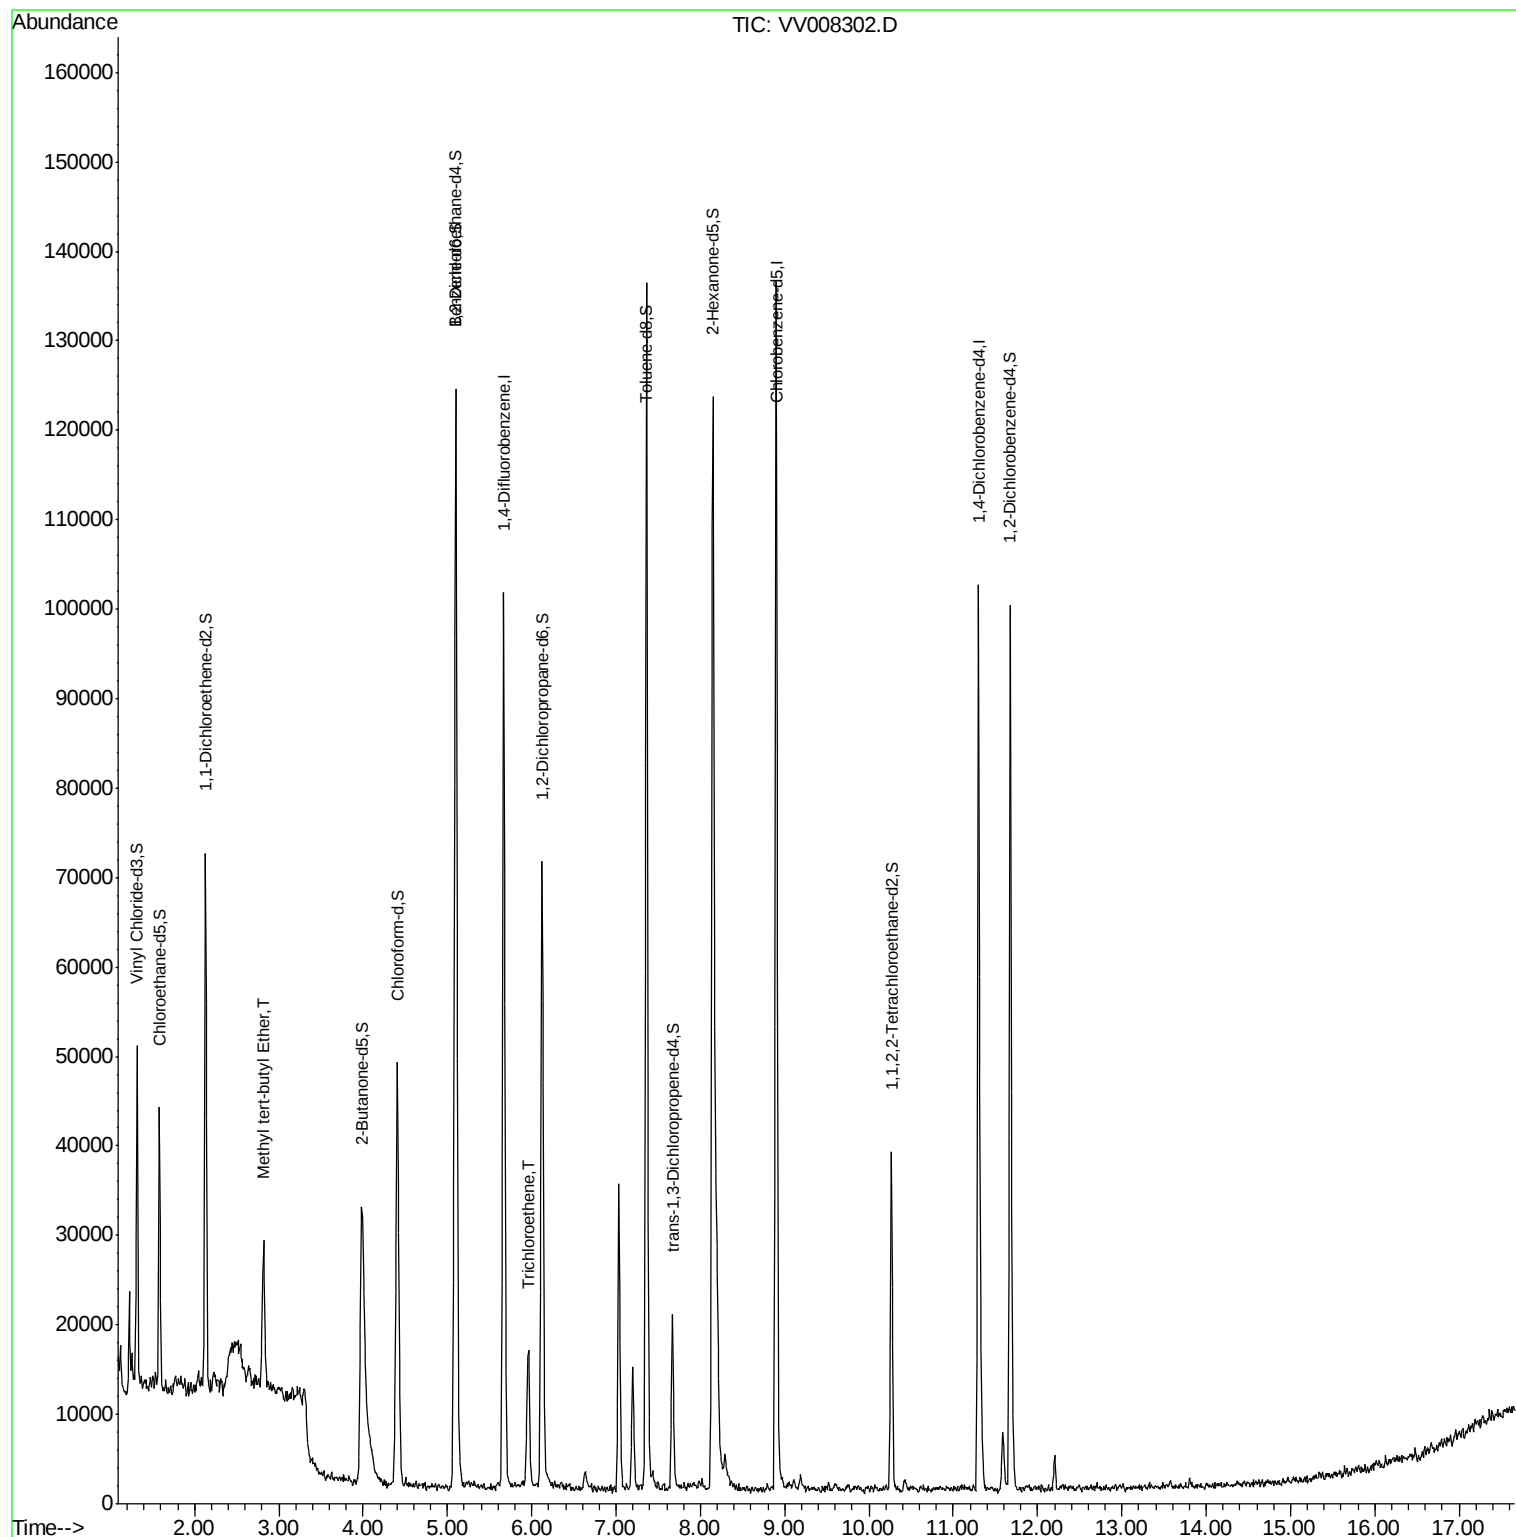


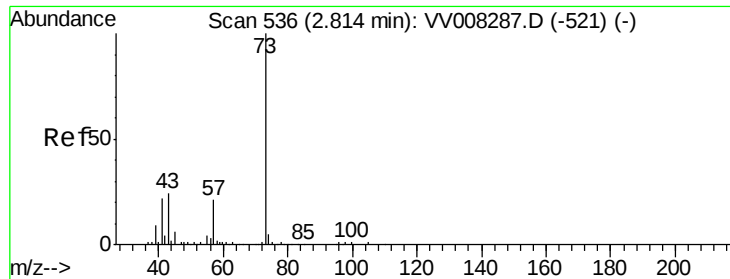




#17
Methvl tert-butvl Ether
Concen: 1.521 ug/L
RT: 2.82 min Scan# 537
Delta R.T. 0.00 min
Lab File: VV008302.D
Acq: 16 Oct 2018 17:19

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Tot Ion: 73 Resp: 17160
Ion Ratio Lower Upper
73 100
43 24.8 19.0 28.6
57 24.0 18.2 27.2

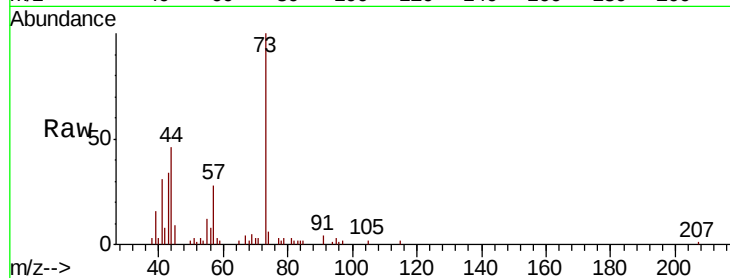


Abundance Ion 73.10 (72.80 to 73.80): VV0
Ion 43.05 (42.75 to 43.75): VV0
Ion 57.10 (56.80 to 57.80): VV0

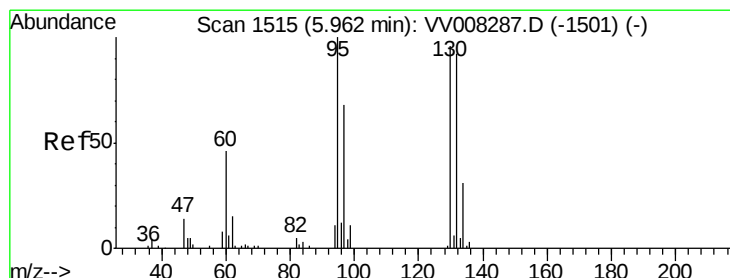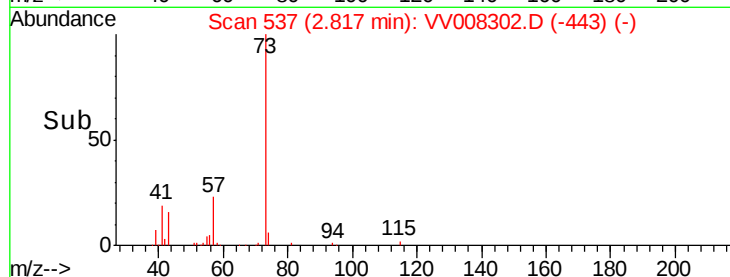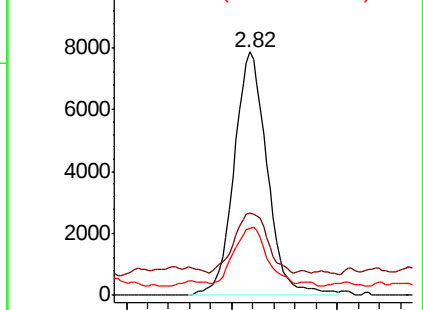

#34
Trichloroethene
Concen: 0.638 ug/L
RT: 5.96 min Scan# 1516
Delta R.T. 0.00 min
Lab File: VV008302.D
Acq: 16 Oct 2018 17:19

Tgt Ion: 95 Resp: 4382
Ion Ratio Lower Upper
95 100
97 62.1 44.4 82.4
132 82.3 60.4 112.2
130 93.1 65.5 121.7

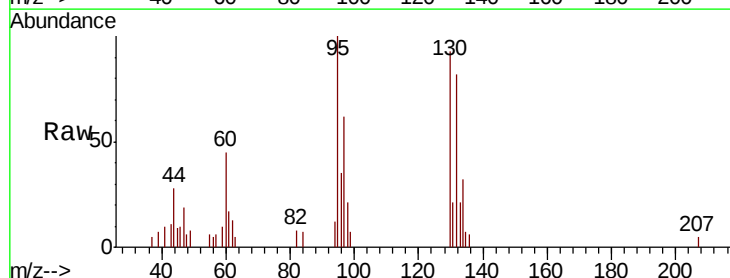

Abundance Ion 95.00 (94.70 to 95.70): VV0
Ion 96.95 (96.65 to 97.65): VV0
Ion 131.95 (131.65 to 132.65): VV0
Ion 129.95 (129.65 to 130.65): VV0

