

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101618\
 Data File : VV008307.D
 Acq On : 16 Oct 2018 19:41
 Operator : SY/MD
 Sample : J5406-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Quant Time: Oct 19 11:47:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 17 02:28:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	84582	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	75865	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	30219	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23957	5.01	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.20%
7) Chloroethane-d5	1.59	69	15948	4.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.60%
11) 1,1-Dichloroethene-d2	2.14	63	35596	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.96	46	78188	48.77	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.54%
24) Chloroform-d	4.41	84	47436	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	5.09	65	24793	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.10	84	102483	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.13	67	35466	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	89799	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.67	79	12177	4.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.00%
46) 2-Hexanone-d5	8.14	63	44293	41.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.06%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	19171	3.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	26870	4.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	3659	4.218 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101618\
Data File : VV008307.D
Acq On : 16 Oct 2018 19:41
Operator : SY/MD
Sample : J5406-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Time: Oct 19 11:47:49 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 17 02:28:08 2018
Response via : Initial Calibration

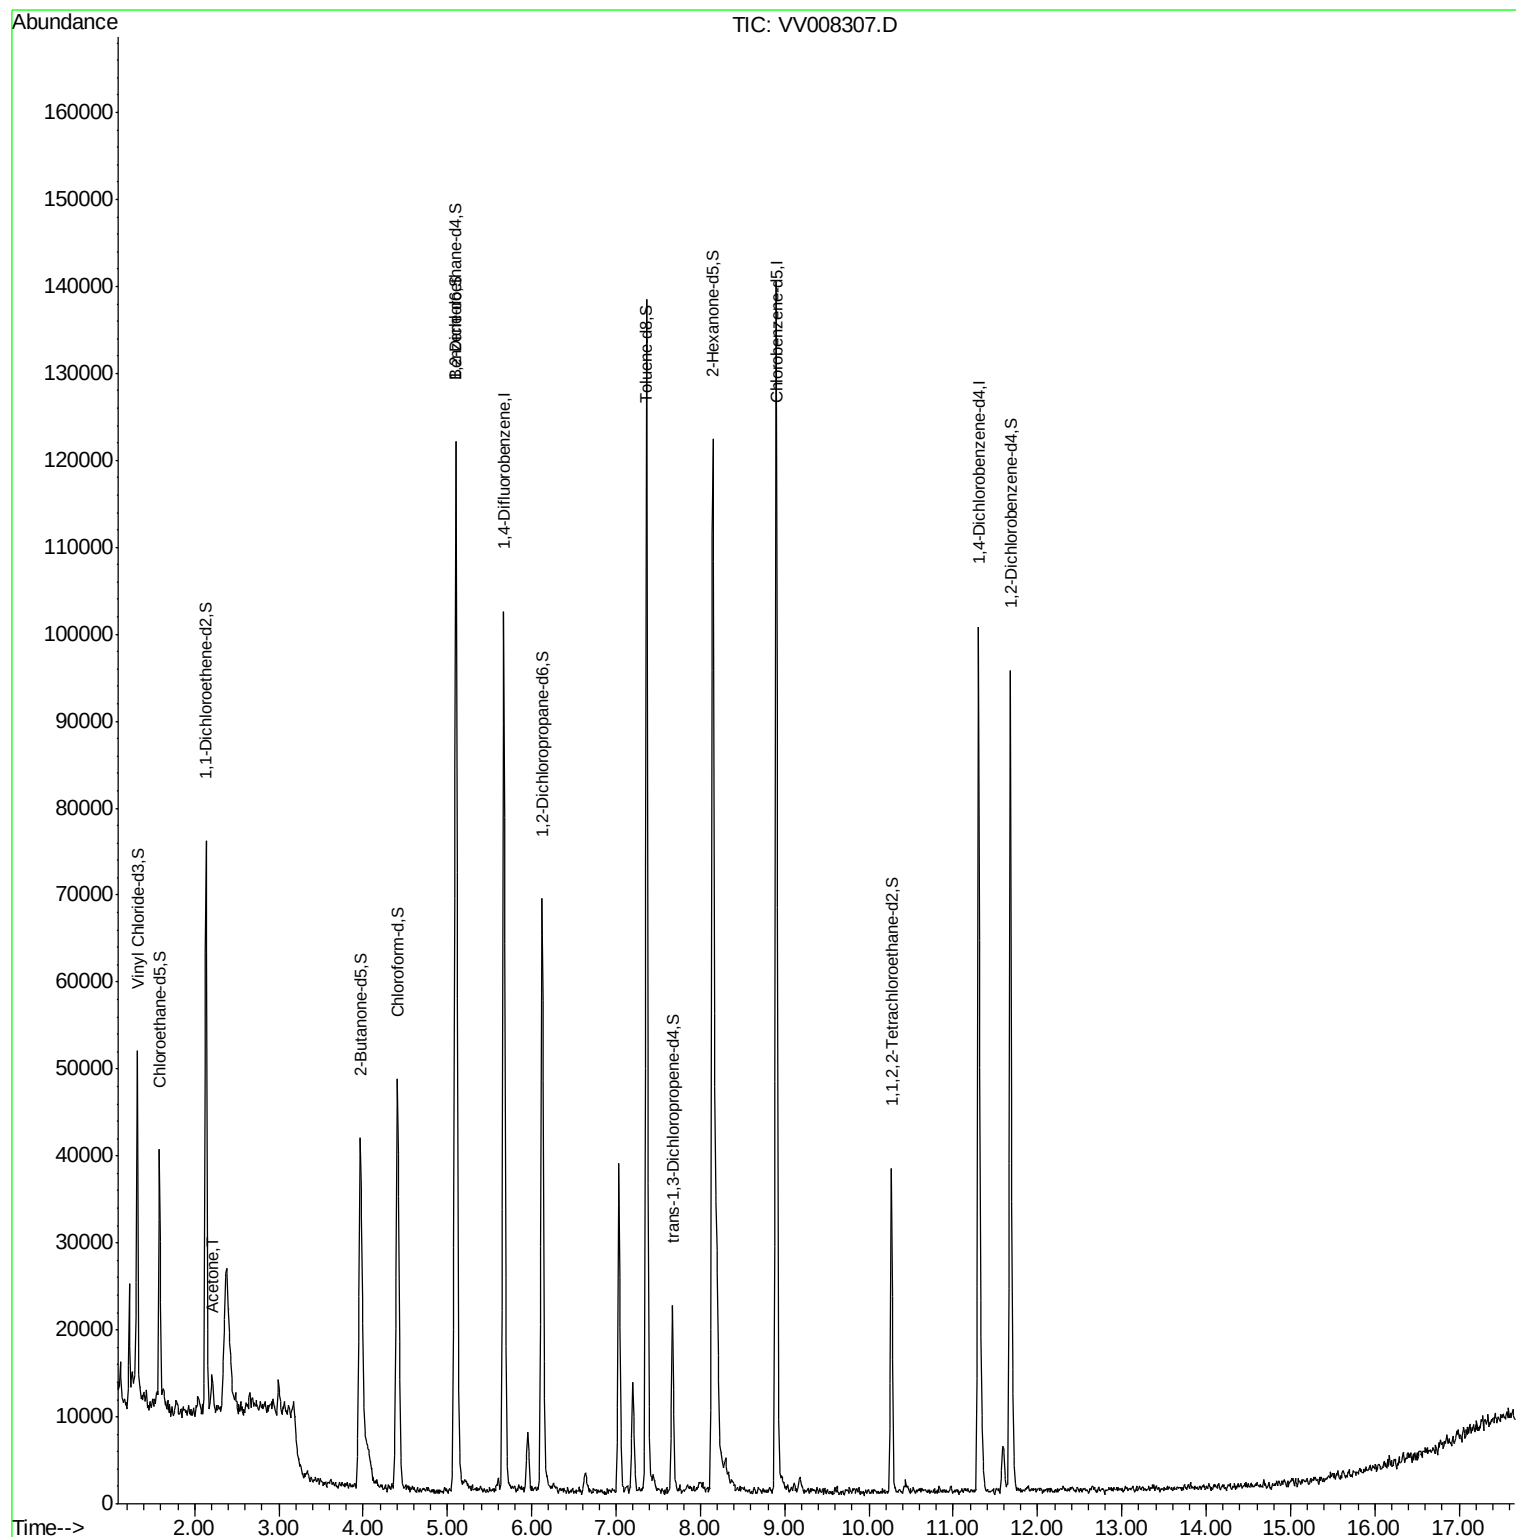

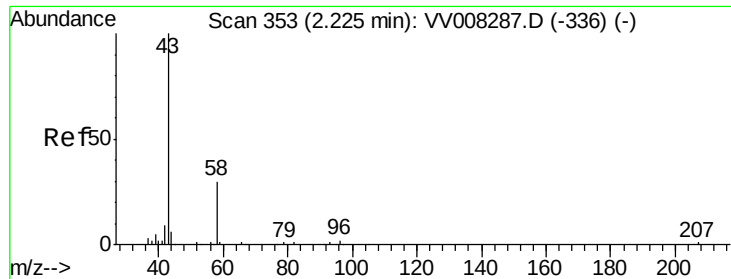

#13

Acetone

Concen: 4.218 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.02 min

Lab File: VV008307.D

Acq: 16 Oct 2018 19:41

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Tot Ion: 43 Resp: 3659

Ion Ratio Lower Upper

43 100

58 34.2 0.0 62.0

