


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101618\
Data File : VV008286.D
Acq On : 16 Oct 2018 09:10
Operator : SY/MD
Sample : BFB87
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB87

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 19 11:58:02 2018

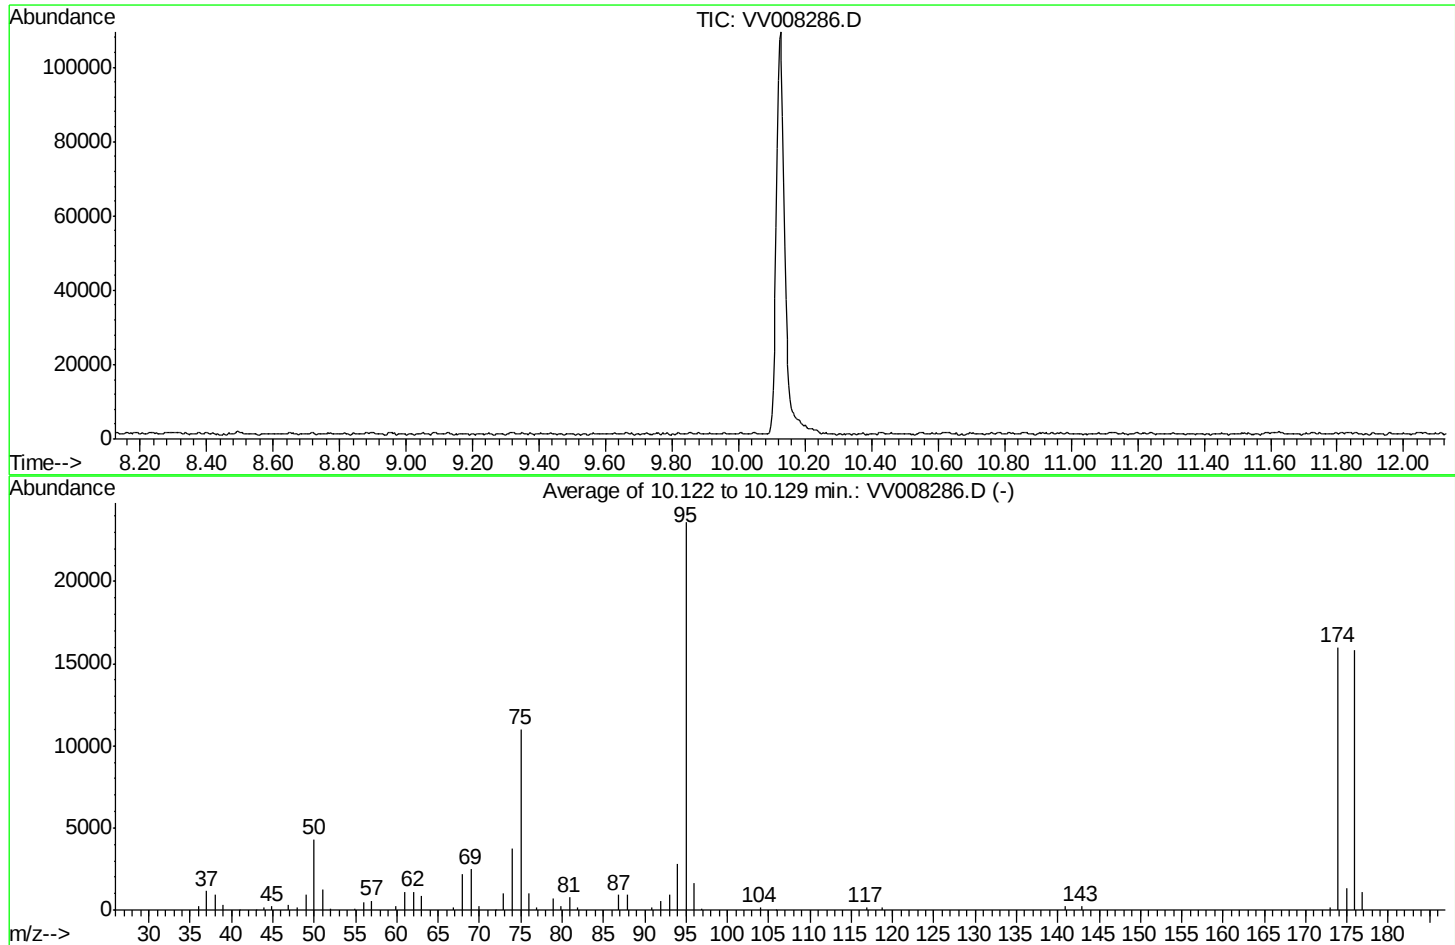

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4267	PASS
75	95	30	80	46.5	10983	PASS
95	95	100	100	100.0	23597	PASS
96	95	5	9	6.9	1625	PASS
173	174	0.00	2	1.2	191	PASS
174	95	50	120	67.6	15952	PASS
175	174	5	9	8.3	1320	PASS
176	174	95	101	99.2	15822	PASS
177	176	5	9	7.0	1106	PASS

Scan 2796 (10.080 min): VV008286.D
BFB87

m/z	Abundance
39.00	107.0
39.90	112.0
41.00	215.0
42.90	159.0
43.90	406.0
55.00	159.0
57.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	240.0
36.90	1151.0
38.00	947.0
39.00	467.0
40.90	254.0
43.00	190.0
44.00	593.0
44.90	224.0
46.90	271.0
48.00	135.0
49.00	970.0
50.00	4375.0
51.00	1275.0
54.90	233.0
56.00	473.0
57.00	699.0
59.90	275.0
61.00	1058.0
62.00	1204.0
63.00	790.0
66.80	117.0
68.00	2293.0
69.00	2535.0
70.00	267.0
71.90	118.0
73.00	1061.0
74.00	3885.0
75.00	11119.0
76.00	1088.0
77.00	152.0
78.90	708.0
79.90	212.0
80.90	720.0
81.90	134.0
86.90	836.0
87.90	906.0
90.90	128.0
91.90	582.0
92.90	918.0
94.00	2963.0
95.00	24088.0
96.00	1691.0
96.90	122.0
103.90	131.0
105.90	122.0
116.80	192.0
118.80	171.0
140.90	216.0
142.90	200.0
173.00	196.0
173.90	15663.0
174.90	1286.0
175.90	15840.0
176.90	1091.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	265.0
36.90	1176.0
38.00	955.0
39.00	455.0
39.90	121.0
41.00	221.0
43.00	191.0
44.00	552.0
44.90	213.0
46.90	290.0
48.00	140.0
49.00	995.0
50.00	4391.0
51.00	1276.0
52.00	114.0
54.90	234.0
56.00	475.0
57.00	729.0
59.90	251.0
61.00	1084.0
62.00	1125.0
63.00	867.0
66.80	138.0
68.00	2232.0
69.00	2562.0
70.00	255.0
72.90	1027.0
74.00	3846.0
75.00	11243.0
76.00	1085.0
76.80	157.0
78.90	758.0
79.90	205.0
80.90	755.0
81.90	144.0
86.90	968.0
87.90	962.0
90.90	121.0
91.90	595.0
93.00	970.0
94.00	2854.0
95.00	24288.0
96.00	1704.0
96.90	102.0
103.90	136.0
116.80	159.0
118.80	155.0
140.90	208.0
142.80	210.0
173.00	191.0
173.90	16448.0
174.90	1363.0
175.90	16381.0
176.90	1144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.00	256.0
37.00	1098.0
38.00	883.0
38.90	437.0
39.90	126.0
41.00	220.0
43.00	187.0
44.00	508.0
44.90	184.0
46.90	303.0
48.00	139.0
49.00	925.0
50.00	4037.0
51.00	1213.0
52.00	125.0
54.90	219.0
56.00	449.0
57.00	670.0
59.90	193.0
61.00	1054.0
62.00	960.0
63.00	823.0
66.80	130.0
68.00	2009.0
69.00	2351.0
70.00	238.0
72.90	915.0
74.00	3397.0
75.00	10587.0
76.00	983.0
76.80	140.0
78.90	715.0
79.90	192.0
80.90	766.0
81.80	149.0
86.90	987.0
87.90	888.0
90.90	132.0
91.90	551.0
93.00	921.0
94.00	2531.0
95.00	22416.0
96.00	1481.0
104.00	118.0
116.90	115.0
118.80	124.0
140.80	186.0
142.80	215.0
173.00	187.0
173.90	15746.0
174.90	1313.0
175.90	15245.0
176.90	1083.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87