

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018939.D
 Acq On : 16 Oct 2020 16:02
 Operator : SY/MD
 Sample : L4426-07
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG411

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	166361	170035	15.88%	2.029%
2	1.576	144	151	167	rVB	145830	160730	15.01%	1.918%
3	2.119	310	320	351	rVB	287471	453081	42.32%	5.407%
4	2.524	440	446	447	rBV3	1080	1140	0.11%	0.014%
5	2.585	462	465	467	rBV2	453	283	0.03%	0.003%
6	2.884	555	558	561	rBV	401	314	0.03%	0.004%
7	2.952	577	579	582	rBV	356	211	0.02%	0.003%
8	3.151	638	641	643	rBV	281	181	0.02%	0.002%
9	3.299	684	687	693	rVB2	296	269	0.03%	0.003%
10	3.380	701	712	713	rBV	392	519	0.05%	0.006%
11	3.466	735	739	740	rBV	343	225	0.02%	0.003%
12	3.540	758	762	763	rBV	245	176	0.02%	0.002%
13	3.621	784	787	790	rBV	391	259	0.02%	0.003%
14	3.682	805	806	807	rBV	211	55	0.01%	0.001%
15	3.746	821	826	827	rBV2	326	259	0.02%	0.003%
16	3.849	856	858	862	rBV	160	121	0.01%	0.001%
17	3.904	865	875	904	rBV2	73985	208201	19.45%	2.485%
18	4.370	1005	1020	1055	rBV	166678	417868	39.03%	4.987%
19	4.576	1082	1084	1088	rVB2	418	191	0.02%	0.002%
20	4.608	1092	1094	1096	rVB2	303	111	0.01%	0.001%
21	4.650	1105	1107	1112	rVB3	400	209	0.02%	0.002%
22	4.691	1117	1120	1128	rBV4	729	880	0.08%	0.011%
23	4.730	1128	1132	1136	rVB3	372	273	0.03%	0.003%
24	4.756	1136	1140	1142	rBV2	275	198	0.02%	0.002%
25	4.778	1145	1147	1150	rVB2	361	137	0.01%	0.002%
26	4.801	1150	1154	1156	rBV	326	299	0.03%	0.004%
27	4.859	1168	1172	1174	rBV2	239	144	0.01%	0.002%
28	4.878	1174	1178	1179	rBV2	271	170	0.02%	0.002%
29	4.936	1194	1196	1199	rVB3	353	201	0.02%	0.002%
30	4.955	1199	1202	1206	rBV2	405	402	0.04%	0.005%
31	5.068	1220	1237	1277	rBV2	410777	1070695	100.00%	12.777%
32	5.412	1341	1344	1346	rBV	482	362	0.03%	0.004%
33	5.460	1357	1359	1364	rVB2	478	292	0.03%	0.003%
34	5.527	1379	1380	1382	rVB2	311	76	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018939.D
 Acq On : 16 Oct 2020 16:02
 Operator : SY/MD
 Sample : L4426-07
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG411

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	5.544	1382	1385	1387	rBV	406	272	0.03%	0.003%
36	5.569	1391	1393	1396	rVV	227	109	0.01%	0.001%
37	5.637	1402	1414	1445	rBV	361694	720533	67.30%	8.598%
38	5.923	1491	1503	1527	rBV2	43082	92713	8.66%	1.106%
39	6.090	1541	1555	1583	rBV	237384	486226	45.41%	5.802%
40	6.453	1664	1668	1670	rBV	361	308	0.03%	0.004%
41	6.486	1675	1678	1680	rBV	244	155	0.01%	0.002%
42	6.540	1691	1695	1697	rBV	227	224	0.02%	0.003%
43	6.608	1713	1716	1720	rBV2	302	234	0.02%	0.003%
44	6.682	1737	1739	1741	rVB2	514	190	0.02%	0.002%
45	6.752	1758	1761	1763	rBV2	203	141	0.01%	0.002%
46	6.791	1770	1773	1777	rBV2	338	303	0.03%	0.004%
47	6.900	1804	1807	1809	rBV	311	235	0.02%	0.003%
48	7.006	1828	1840	1865	rBV	128522	236020	22.04%	2.816%
49	7.334	1930	1942	1962	rBV	475188	821473	76.72%	9.803%
50	7.640	2026	2037	2063	rBV	92696	164858	15.40%	1.967%
51	7.897	2113	2117	2118	rBV	549	341	0.03%	0.004%
52	8.000	2144	2149	2157	rVB6	1516	1864	0.17%	0.022%
53	8.106	2170	2182	2222	rBV2	208776	460115	42.97%	5.491%
54	8.601	2334	2336	2341	rBV3	299	201	0.02%	0.002%
55	8.672	2356	2358	2362	rBV2	467	375	0.04%	0.004%
56	8.704	2366	2368	2370	rVB	264	72	0.01%	0.001%
57	8.768	2385	2388	2391	rBV	266	92	0.01%	0.001%
58	8.791	2391	2395	2396	rBV	231	188	0.02%	0.002%
59	8.871	2407	2420	2443	rBV	563794	909768	84.97%	10.856%
60	9.045	2470	2474	2478	rBV4	856	853	0.08%	0.010%
61	9.225	2528	2530	2532	rVB	249	97	0.01%	0.001%
62	9.373	2574	2576	2578	rBV	248	146	0.01%	0.002%
63	9.534	2621	2626	2630	rBV2	660	564	0.05%	0.007%
64	9.614	2650	2651	2652	rBV	151	41	0.00%	0.000%
65	9.630	2652	2656	2660	rVB2	299	282	0.03%	0.003%
66	9.746	2688	2692	2695	rBV2	368	323	0.03%	0.004%
67	9.765	2695	2698	2705	rVV2	434	494	0.05%	0.006%
68	9.810	2710	2712	2713	rBV	255	100	0.01%	0.001%
69	9.868	2729	2730	2733	rBV	230	130	0.01%	0.002%
70	9.913	2739	2744	2748	rBV2	410	419	0.04%	0.005%
71	9.939	2749	2752	2754	rVV	259	128	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSV0A V\DATA\VV101620\
Data File : VV018939.D
Acq On : 16 Oct 2020 16:02
Operator : SY/MD
Sample : L4426-07
Misc : 5.0ml/MSV0A V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG411

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.235	2832	2844	2866	rVB	228137	360232	33.64%	4.299%
73	10.402	2886	2896	2905	rBV2	3847	6397	0.60%	0.076%
74	10.601	2955	2958	2959	rBV2	213	116	0.01%	0.001%
75	10.929	3056	3060	3061	rBV	416	255	0.02%	0.003%
76	11.209	3145	3147	3151	rBV	354	303	0.03%	0.004%
77	11.270	3154	3166	3187	rBV	553348	854387	79.80%	10.196%
78	11.646	3271	3283	3305	rBV	481508	768866	71.81%	9.175%
79	12.055	3406	3410	3411	rBV	365	253	0.02%	0.003%


Sum of corrected areas: 8379963

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101620\
Data File : VV018939.D
Acq On : 16 Oct 2020 16:02
Operator : SY/MD
Sample : L4426-07
Misc : 5.0ml/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG411

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

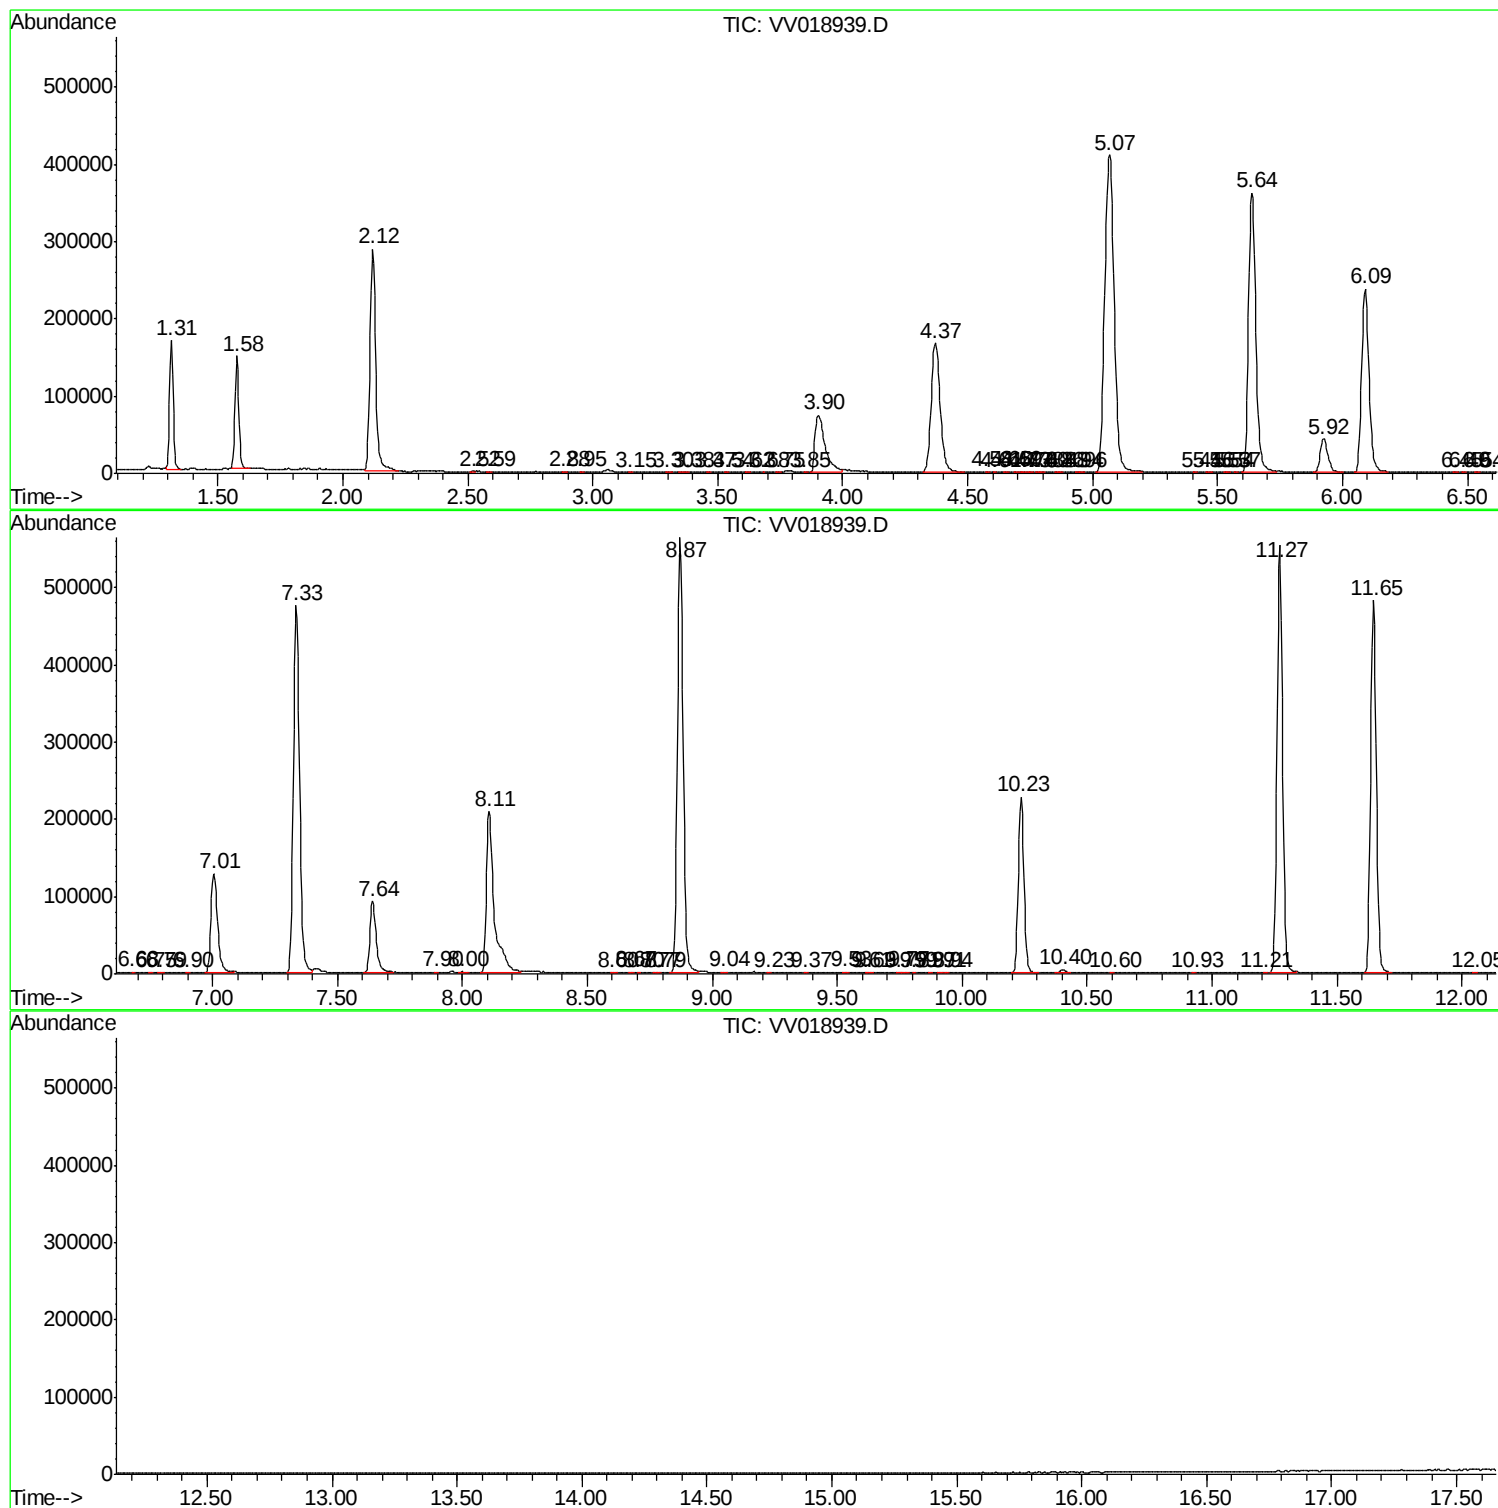

Data Path : Z:\VOASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018939.D
Acq On : 16 Oct 2020 16:02
Operator : SY/MD
Sample : L4426-07
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG411

Quant Method : Z:\VOASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018939.D
Acq On : 16 Oct 2020 16:02
Operator : SY/MD
Sample : L4426-07
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG411

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc