

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018944.D
 Acq On : 16 Oct 2020 18:01
 Operator : SY/MD
 Sample : L4426-03 200X
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	183377	182914	5.97%	1.463%
2	1.576	144	151	171	rVB	162250	183158	5.98%	1.465%
3	2.123	311	321	344	rVB	307751	477155	15.57%	3.817%
4	2.489	432	435	438	rVB2	651	406	0.01%	0.003%
5	2.528	438	447	453	rBV4	2820	4365	0.14%	0.035%
6	2.785	523	527	532	rBV4	452	434	0.01%	0.003%
7	2.910	560	566	568	rBV3	442	483	0.02%	0.004%
8	3.782	836	837	839	rBV	185	90	0.00%	0.001%
9	3.836	851	854	856	rBV2	660	367	0.01%	0.003%
10	3.904	865	875	921	rBV	105063	300044	9.79%	2.400%
11	4.376	1008	1022	1052	rVB	210102	519206	16.94%	4.153%
12	4.798	1151	1153	1155	rBV	387	223	0.01%	0.002%
13	4.926	1190	1193	1196	rBV3	403	264	0.01%	0.002%
14	4.971	1205	1207	1210	rVB2	473	247	0.01%	0.002%
15	4.994	1210	1214	1220	rVB2	386	431	0.01%	0.003%
16	5.071	1220	1238	1266	rBV2	505602	1307064	42.64%	10.455%
17	5.367	1328	1330	1333	rVB2	471	164	0.01%	0.001%
18	5.483	1364	1366	1371	rBV3	390	394	0.01%	0.003%
19	5.579	1394	1396	1397	rBV	301	112	0.00%	0.001%
20	5.640	1401	1415	1447	rBV	372987	750597	24.49%	6.004%
21	5.929	1493	1505	1525	rBV3	46647	100986	3.29%	0.808%
22	6.093	1542	1556	1582	rBV	299454	598981	19.54%	4.791%
23	6.309	1620	1623	1626	rBV2	756	633	0.02%	0.005%
24	6.380	1643	1645	1650	rBV3	272	187	0.01%	0.001%
25	6.418	1656	1657	1659	rBV2	168	58	0.00%	0.000%
26	6.550	1694	1698	1699	rBV2	279	169	0.01%	0.001%
27	6.601	1712	1714	1716	rBV3	264	182	0.01%	0.001%
28	6.759	1759	1763	1765	rBV	506	362	0.01%	0.003%
29	6.814	1776	1780	1784	rBV2	400	284	0.01%	0.002%
30	6.859	1793	1794	1796	rBV	254	110	0.00%	0.001%
31	6.907	1807	1809	1813	rVB2	271	146	0.00%	0.001%
32	6.929	1813	1816	1818	rBV2	288	212	0.01%	0.002%
33	6.968	1825	1828	1829	rBV2	250	113	0.00%	0.001%
34	7.007	1829	1840	1866	rBV	149002	276075	9.01%	2.208%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018944.D
 Acq On : 16 Oct 2020 18:01
 Operator : SY/MD
 Sample : L4426-03 200X
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	7.248	1913	1915	1920	rVB3	618	406	0.01%	0.003%
36	7.290	1926	1928	1931	rBV3	527	292	0.01%	0.002%
37	7.338	1931	1943	1972	rBV	535087	928365	30.29%	7.426%
38	7.643	2025	2038	2062	rBV	106262	189611	6.19%	1.517%
39	7.843	2097	2100	2102	rBV	332	179	0.01%	0.001%
40	7.881	2108	2112	2115	rBV2	482	282	0.01%	0.002%
41	7.997	2134	2148	2173	rBV	1834508	3065186	100.00%	24.519%
42	8.106	2173	2182	2224	rVB2	287774	579784	18.92%	4.638%
43	8.576	2325	2328	2331	rBV3	420	341	0.01%	0.003%
44	8.659	2350	2354	2356	rBV2	324	276	0.01%	0.002%
45	8.724	2371	2374	2375	rBV	246	153	0.00%	0.001%
46	8.740	2378	2379	2382	rBV	196	139	0.00%	0.001%
47	8.830	2403	2407	2409	rBV	379	278	0.01%	0.002%
48	8.871	2409	2420	2442	rBV	550596	881437	28.76%	7.051%
49	9.100	2489	2491	2494	rBV2	367	190	0.01%	0.002%
50	9.158	2505	2509	2512	rBV3	267	267	0.01%	0.002%
51	9.196	2520	2521	2522	rBV3	118	39	0.00%	0.000%
52	9.273	2542	2545	2553	rVB	473	547	0.02%	0.004%
53	9.309	2553	2556	2558	rBV	237	161	0.01%	0.001%
54	9.402	2582	2585	2587	rBV2	311	211	0.01%	0.002%
55	9.460	2601	2603	2604	rBV	335	153	0.00%	0.001%
56	9.502	2612	2616	2618	rBV	190	160	0.01%	0.001%
57	9.633	2654	2657	2659	rBV2	256	130	0.00%	0.001%
58	9.704	2674	2679	2681	rBV3	421	365	0.01%	0.003%
59	9.727	2684	2686	2688	rBV2	399	176	0.01%	0.001%
60	9.781	2700	2703	2705	rBV	325	193	0.01%	0.002%
61	9.830	2714	2718	2721	rVB2	186	145	0.00%	0.001%
62	9.846	2721	2723	2724	rBV2	181	77	0.00%	0.001%
63	9.907	2739	2742	2744	rBV	295	214	0.01%	0.002%
64	10.016	2773	2776	2777	rBV2	136	87	0.00%	0.001%
65	10.029	2778	2780	2783	rBV2	279	213	0.01%	0.002%
66	10.090	2797	2799	2800	rBV	141	73	0.00%	0.001%
67	10.238	2833	2845	2862	rBV	300102	462081	15.08%	3.696%
68	10.347	2876	2879	2882	rBV2	517	261	0.01%	0.002%
69	10.556	2941	2944	2946	rBV2	277	181	0.01%	0.001%
70	10.666	2973	2978	2982	rBV2	246	310	0.01%	0.002%
71	10.785	3012	3015	3022	rBV	388	331	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
Data File : VV018944.D
Acq On : 16 Oct 2020 18:01
Operator : SY/MD
Sample : L4426-03 200X
Misc : 5.0ml/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	11.106	3112	3115	3117	rVB	444	217	0.01%	0.002%
73	11.270	3155	3166	3190	rBV	526134	810924	26.46%	6.487%
74	11.563	3255	3257	3259	rBV	361	194	0.01%	0.002%
75	11.646	3271	3283	3308	rBV	562134	866825	28.28%	6.934%
76	11.942	3371	3375	3383	rVB3	556	583	0.02%	0.005%
77	11.977	3384	3386	3389	rBV2	287	195	0.01%	0.002%
78	12.206	3455	3457	3460	rBV	185	134	0.00%	0.001%
79	12.482	3537	3543	3550	rBV4	404	521	0.02%	0.004%
80	12.614	3582	3584	3588	rBV2	252	182	0.01%	0.001%
81	12.678	3601	3604	3605	rBV	382	219	0.01%	0.002%
82	12.871	3661	3664	3667	rBV2	339	247	0.01%	0.002%
83	12.981	3695	3698	3703	rBV3	420	384	0.01%	0.003%
84	13.125	3740	3743	3744	rBV	334	174	0.01%	0.001%
85	13.662	3906	3910	3913	rBV	438	394	0.01%	0.003%
86	13.788	3946	3949	3952	rVB	565	349	0.01%	0.003%


Sum of corrected areas: 12501452

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101620\
Data File : VV018944.D
Acq On : 16 Oct 2020 18:01
Operator : SY/MD
Sample : L4426-03 200X
Misc : 5.0ml/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

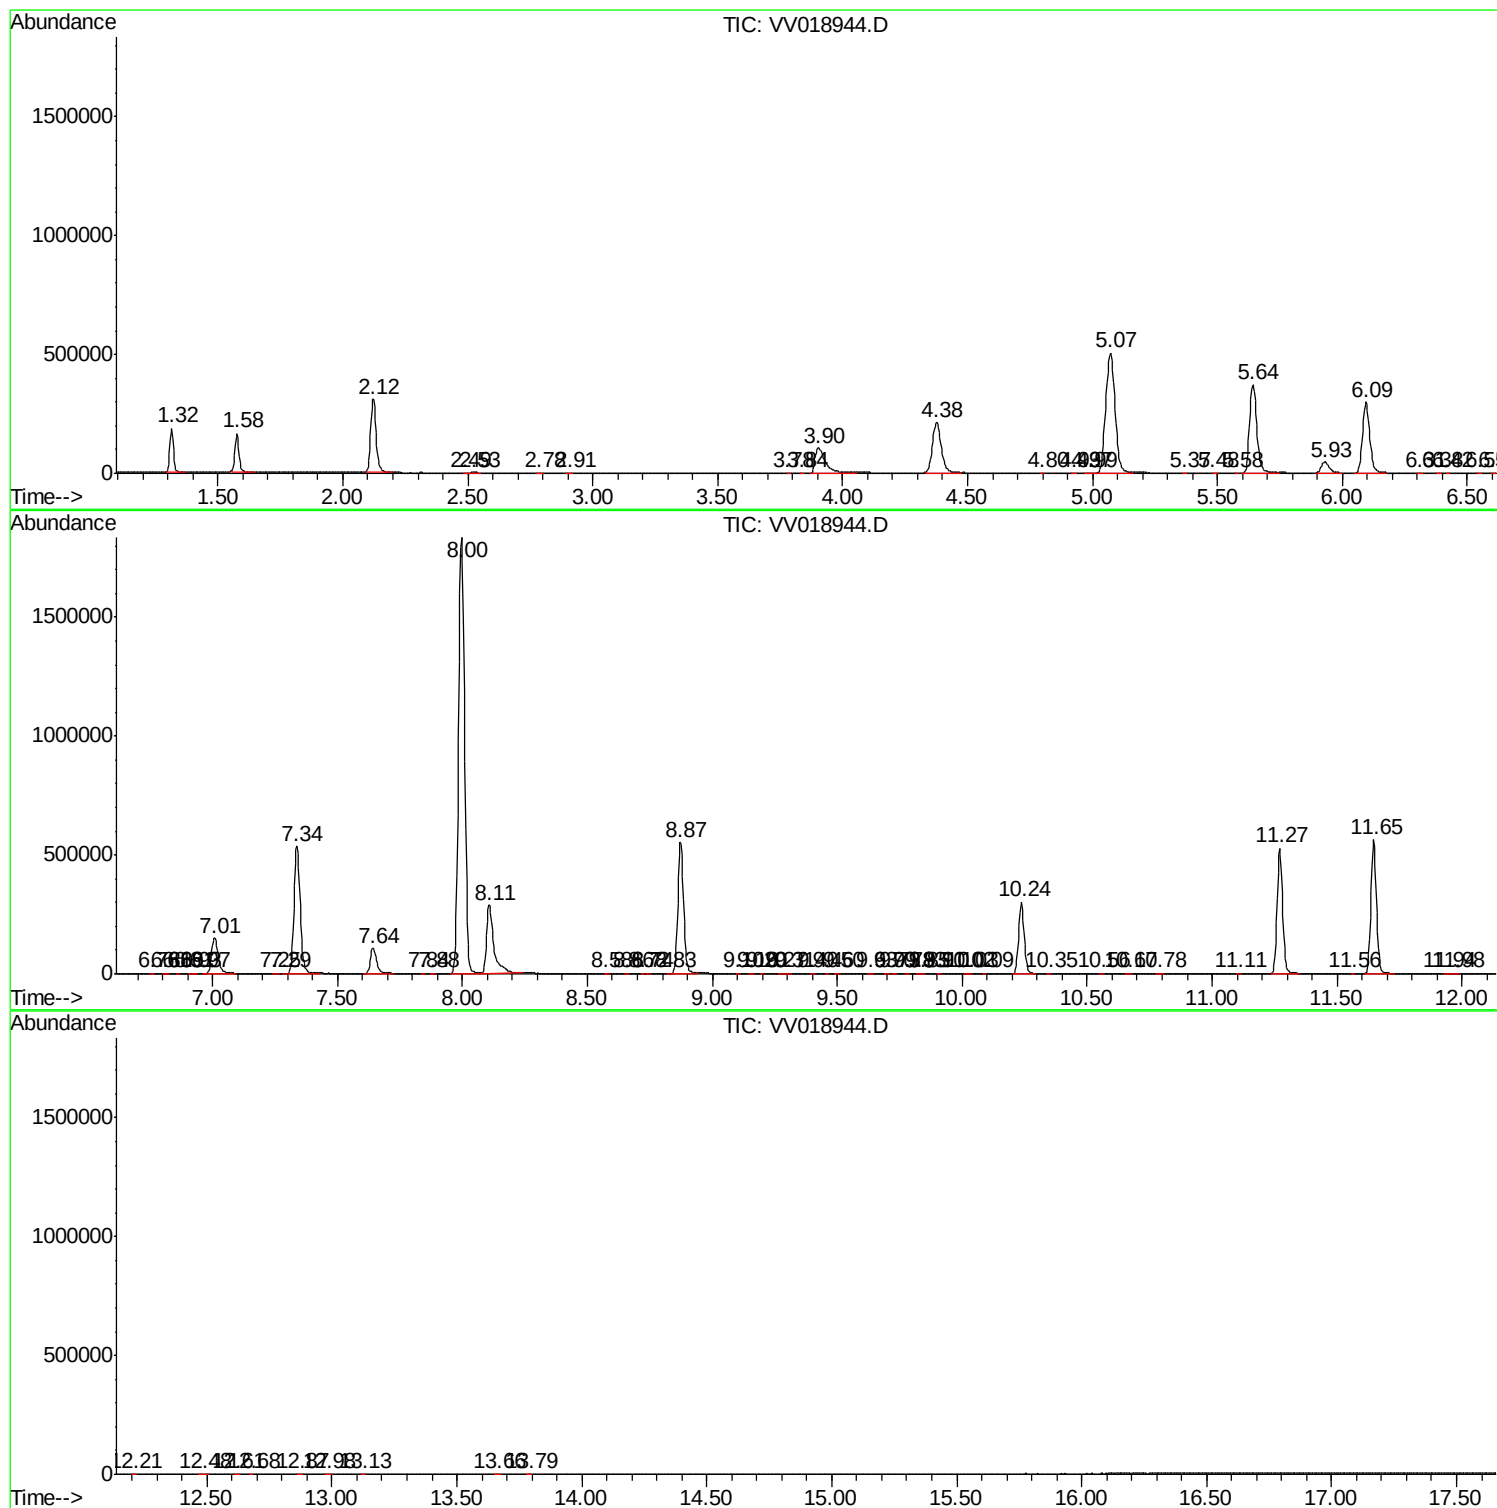

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018944.D
Acq On : 16 Oct 2020 18:01
Operator : SY/MD
Sample : L4426-03 200X
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3Z4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018944.D
Acq On : 16 Oct 2020 18:01
Operator : SY/MD
Sample : L4426-03 200X
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3Z4

Quant Method : Z:\VOASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc