

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018951.D
 Acq On : 16 Oct 2020 20:48
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	179783	180568	13.42%	1.838%
2	1.576	144	151	164	rBV	161457	177417	13.18%	1.806%
3	2.119	311	320	350	rVB	317777	494755	36.76%	5.037%
4	2.528	440	447	456	rVB4	1878	2846	0.21%	0.029%
5	2.984	584	589	590	rBV2	412	297	0.02%	0.003%
6	3.032	598	604	607	rBV2	647	500	0.04%	0.005%
7	3.061	609	613	616	rVB4	634	495	0.04%	0.005%
8	3.084	616	620	625	rBV3	531	565	0.04%	0.006%
9	3.312	690	691	693	rBV2	234	73	0.01%	0.001%
10	3.354	701	704	705	rBV	210	129	0.01%	0.001%
11	3.405	718	720	723	rVB2	396	216	0.02%	0.002%
12	3.547	762	764	765	rBV	329	145	0.01%	0.001%
13	3.759	828	830	833	rBV2	280	177	0.01%	0.002%
14	3.862	859	862	865	rBV2	498	345	0.03%	0.004%
15	3.907	865	876	911	rBV	100358	292310	21.72%	2.976%
16	4.376	1007	1022	1056	rVB	209075	516023	38.34%	5.253%
17	4.830	1161	1163	1165	rBV	404	223	0.02%	0.002%
18	4.955	1198	1202	1205	rBV2	566	467	0.03%	0.005%
19	5.071	1221	1238	1267	rBV2	524144	1345883	100.00%	13.701%
20	5.640	1403	1415	1441	rBV	395249	791261	58.79%	8.055%
21	5.926	1493	1504	1521	rBV	50053	102426	7.61%	1.043%
22	6.093	1542	1556	1583	rBV	304719	618875	45.98%	6.300%
23	6.380	1642	1645	1648	rBV2	509	439	0.03%	0.004%
24	6.421	1655	1658	1661	rBV2	452	258	0.02%	0.003%
25	6.749	1758	1760	1762	rBV2	295	121	0.01%	0.001%
26	6.859	1791	1794	1796	rBV	332	191	0.01%	0.002%
27	6.894	1802	1805	1807	rBV	489	340	0.03%	0.003%
28	6.929	1812	1816	1819	rBV	403	378	0.03%	0.004%
29	7.007	1829	1840	1866	rBV	156224	286343	21.28%	2.915%
30	7.338	1931	1943	1968	rBV	587749	1021485	75.90%	10.399%
31	7.589	2019	2021	2023	rBV3	287	137	0.01%	0.001%
32	7.643	2028	2038	2060	rVV	111299	194718	14.47%	1.982%
33	8.000	2141	2149	2158	rVV6	4481	7240	0.54%	0.074%
34	8.036	2158	2160	2162	rVB	300	84	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018951.D
 Acq On : 16 Oct 2020 20:48
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	8.106	2172	2182	2225	rBV2	279613	598362	44.46%	6.091%
36	8.566	2320	2325	2328	rBV	424	467	0.03%	0.005%
37	8.672	2356	2358	2360	rBV2	458	284	0.02%	0.003%
38	8.752	2378	2383	2387	rBV4	511	559	0.04%	0.006%
39	8.871	2409	2420	2447	rBV	603382	972124	72.23%	9.896%
40	9.074	2481	2483	2488	rVB3	772	486	0.04%	0.005%
41	9.100	2488	2491	2492	rBV2	639	306	0.02%	0.003%
42	9.161	2508	2510	2515	rVB3	493	304	0.02%	0.003%
43	9.254	2535	2539	2540	rBV	357	192	0.01%	0.002%
44	9.293	2546	2551	2553	rBV2	450	376	0.03%	0.004%
45	9.344	2564	2567	2570	rBV2	244	178	0.01%	0.002%
46	9.402	2582	2585	2588	rVB2	384	280	0.02%	0.003%
47	9.534	2624	2626	2629	rBV2	444	202	0.02%	0.002%
48	9.627	2653	2655	2657	rBV	390	163	0.01%	0.002%
49	9.672	2665	2669	2672	rBV2	346	252	0.02%	0.003%
50	9.801	2706	2709	2716	rBV	423	427	0.03%	0.004%
51	9.833	2717	2719	2721	rBV2	283	116	0.01%	0.001%
52	9.878	2732	2733	2736	rVB	317	93	0.01%	0.001%
53	9.916	2743	2745	2747	rBV	228	92	0.01%	0.001%
54	9.929	2747	2749	2754	rVB2	471	276	0.02%	0.003%
55	10.000	2767	2771	2772	rBV2	231	153	0.01%	0.002%
56	10.061	2785	2790	2792	rBV2	286	246	0.02%	0.003%
57	10.238	2833	2845	2867	rVB	282992	449794	33.42%	4.579%
58	10.373	2886	2887	2889	rBV	176	60	0.00%	0.001%
59	10.399	2892	2895	2897	rBV	207	131	0.01%	0.001%
60	10.437	2905	2907	2910	rBV	288	116	0.01%	0.001%
61	10.585	2949	2953	2958	rVB2	505	487	0.04%	0.005%
62	10.608	2958	2960	2962	rBV2	506	289	0.02%	0.003%
63	10.746	2999	3003	3006	rBV2	469	426	0.03%	0.004%
64	10.765	3006	3009	3013	rVV2	375	272	0.02%	0.003%
65	10.791	3014	3017	3020	rVV2	313	214	0.02%	0.002%
66	10.842	3029	3033	3034	rBV2	466	360	0.03%	0.004%
67	10.894	3047	3049	3054	rVB	476	280	0.02%	0.003%
68	11.019	3084	3088	3092	rBV3	291	280	0.02%	0.003%
69	11.039	3092	3094	3097	rBV	174	101	0.01%	0.001%
70	11.096	3110	3112	3116	rVB	210	109	0.01%	0.001%
71	11.132	3116	3123	3124	rBV2	404	444	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101620\
 Data File : VV018951.D
 Acq On : 16 Oct 2020 20:48
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0ml/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	11.232	3148	3154	3155	rBV	286	294	0.02%	0.003%
73	11.270	3155	3166	3189	rVV	563163	860630	63.95%	8.761%
74	11.408	3207	3209	3210	rBV	319	132	0.01%	0.001%
75	11.524	3243	3245	3247	rBV2	448	240	0.02%	0.002%
76	11.646	3271	3283	3302	rBV	574632	891668	66.25%	9.077%
77	11.839	3341	3343	3346	rBV	211	119	0.01%	0.001%
78	12.125	3428	3432	3434	rBV	375	278	0.02%	0.003%
79	12.193	3450	3453	3457	rBV3	312	283	0.02%	0.003%
80	12.315	3489	3491	3494	rBV2	330	273	0.02%	0.003%
81	12.476	3536	3541	3544	rBV2	385	391	0.03%	0.004%
82	12.820	3641	3648	3649	rBV3	469	509	0.04%	0.005%
83	12.984	3697	3699	3700	rBV	203	87	0.01%	0.001%
84	13.582	3880	3885	3889	rBV2	479	522	0.04%	0.005%
85	13.739	3931	3934	3936	rBV3	663	396	0.03%	0.004%
86	13.948	3996	3999	4000	rBV	330	186	0.01%	0.002%


Sum of corrected areas: 9823039

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A V\DATA\VV101620\
Data File : VV018951.D
Acq On : 16 Oct 2020 20:48
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0ml/MSV0A V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

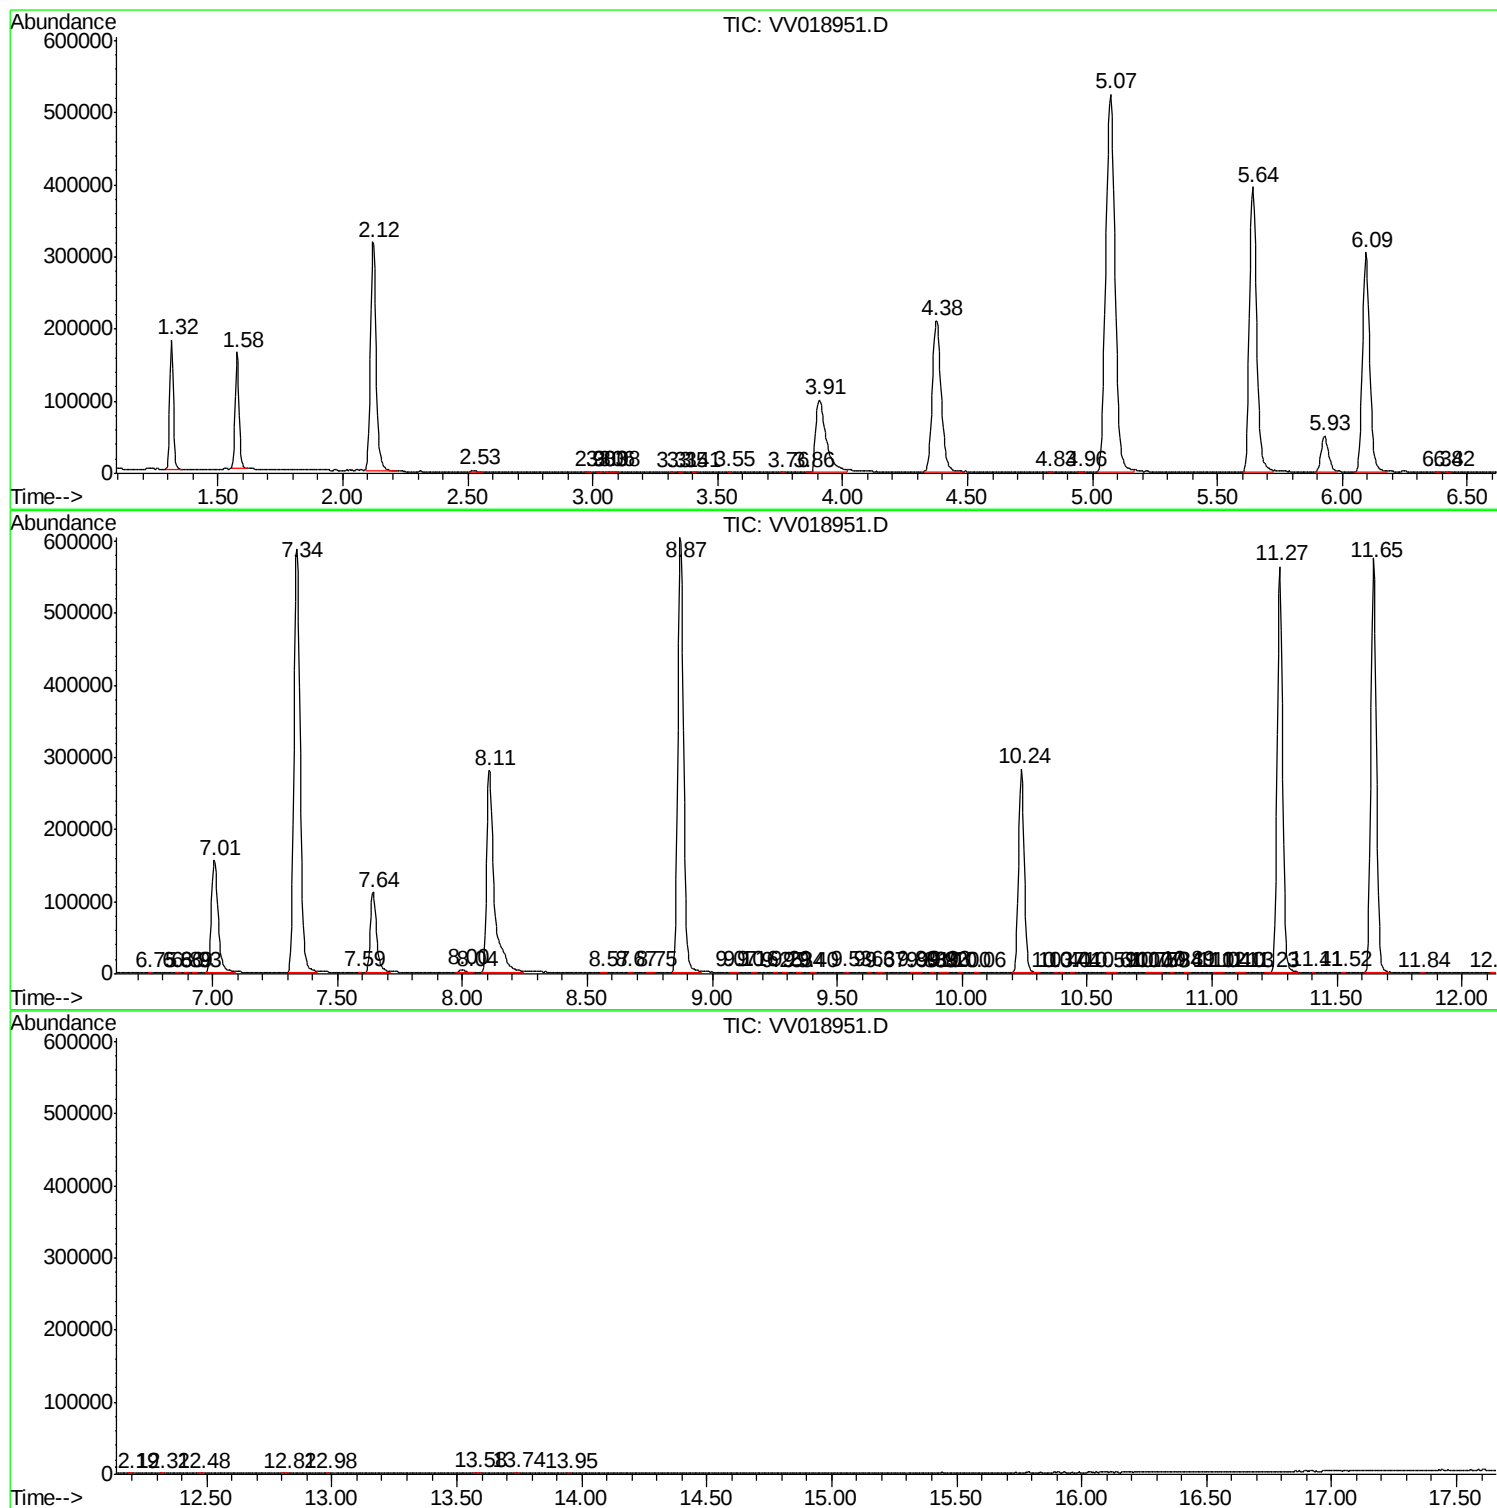

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018951.D
Acq On : 16 Oct 2020 20:48
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101620\
Data File : VV018951.D
Acq On : 16 Oct 2020 20:48
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0ml/MSV0A_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc