


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV01620\
 Data File : VV018934.D
 Acq On : 16 Oct 2020 13:08
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 19 10:44:54 2020

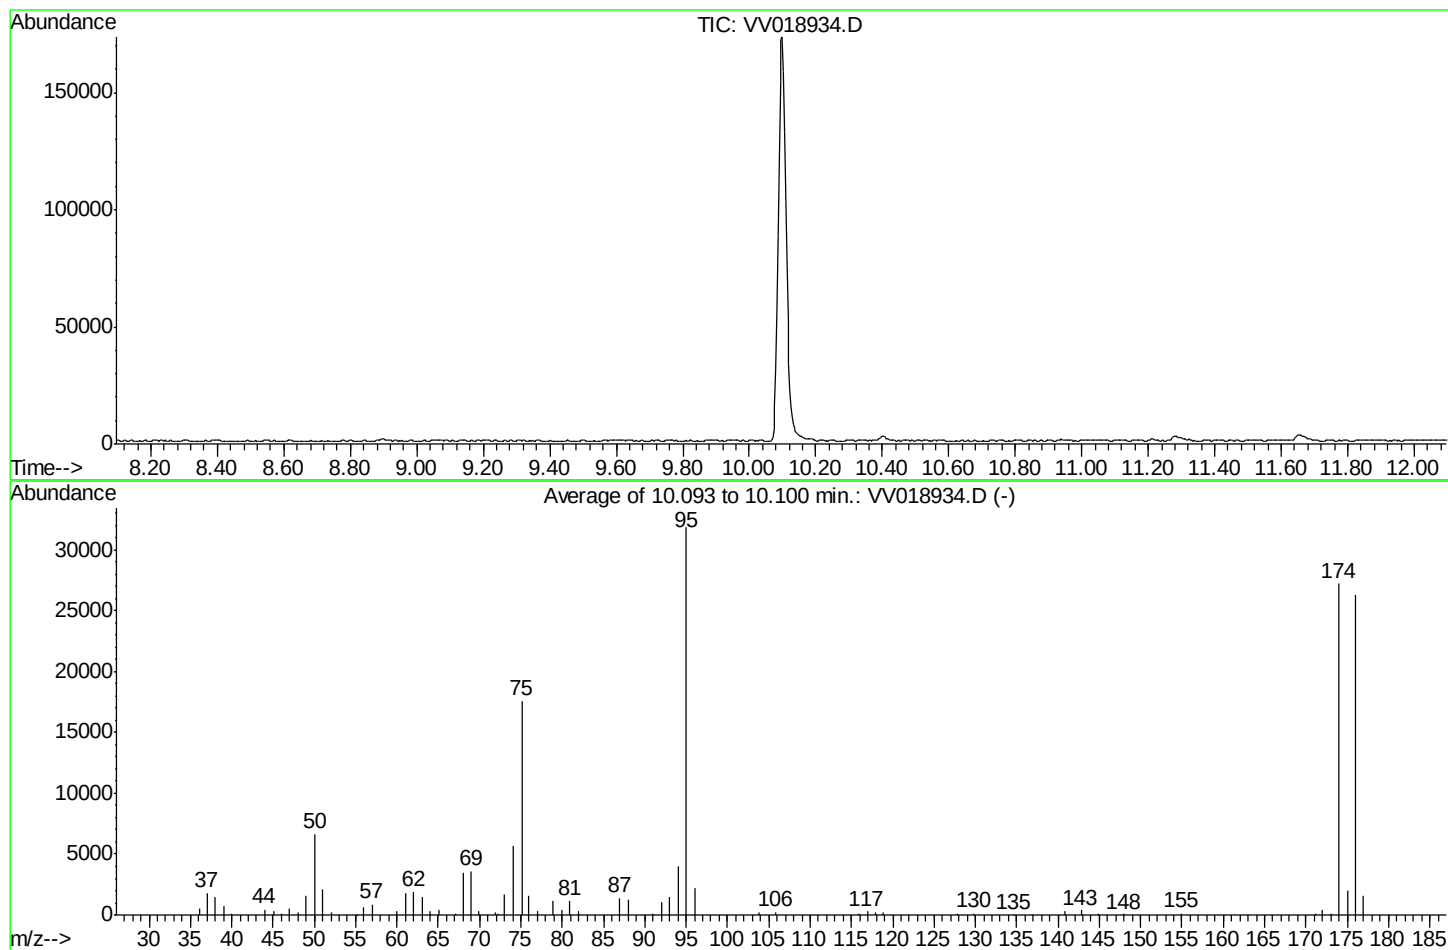

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	6679	PASS
75	95	30	80	55.2	17584	PASS
95	95	100	100	100.0	31858	PASS
96	95	5	9	6.8	2167	PASS
173	174	0.00	2	0.6	157	PASS
174	95	50	120	85.5	27224	PASS
175	174	5	9	7.5	2053	PASS
176	174	95	101	96.6	26290	PASS
177	176	5	9	6.1	1591	PASS

m/z	Abundance
36.10	466.0
37.00	1736.0
38.00	1305.0
39.00	773.0
40.00	356.0
44.00	1372.0
45.00	341.0
46.00	117.0
47.00	402.0
48.00	199.0
49.00	1436.0
50.10	6448.0
51.00	1939.0
52.00	152.0
55.20	111.0
56.00	606.0
57.00	787.0
59.90	331.0
61.00	1700.0
62.00	1832.0
63.00	1319.0
63.90	283.0
65.10	366.0
68.00	3299.0
69.00	3239.0
70.00	271.0
71.80	163.0
72.20	114.0
73.00	1609.0
74.00	5423.0
75.10	16576.0
76.00	1493.0
77.00	334.0
78.90	1069.0
79.90	394.0
81.00	1166.0
82.00	320.0
87.00	1337.0
88.00	1150.0
91.00	106.0
92.00	932.0
93.00	1246.0
94.00	3610.0
95.00	29816.0
96.00	1916.0
103.80	209.0
105.90	249.0
115.90	140.0
116.90	274.0
117.80	140.0
119.00	237.0
127.80	112.0
129.90	136.0
140.90	310.0
142.80	406.0
144.80	145.0
155.00	105.0
171.90	416.0
174.00	24968.0
175.00	1899.0
176.00	23568.0
177.00	1444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.10	546.0
37.00	1876.0
38.00	1548.0
39.00	811.0
40.00	343.0
44.00	1380.0
45.00	380.0
46.00	120.0
47.00	491.0
48.00	252.0
49.00	1653.0
50.10	6884.0
51.00	2225.0
52.00	170.0
56.00	618.0
57.00	855.0
59.90	362.0
61.00	1801.0
62.00	2012.0
63.10	1497.0
64.00	288.0
65.10	410.0
67.10	127.0
68.00	3576.0
69.00	3733.0
70.00	326.0
71.80	178.0
72.20	144.0
73.00	1716.0
74.00	5858.0
75.10	18264.0
76.00	1702.0
77.00	326.0
78.90	1154.0
79.90	390.0
80.90	1216.0
82.00	367.0
87.00	1453.0
88.00	1277.0
91.00	107.0
92.00	1053.0
93.00	1479.0
94.00	4129.0
95.10	32992.0
96.00	2238.0
103.80	194.0
105.90	247.0
115.90	163.0
116.90	291.0
117.90	171.0
118.90	237.0
127.80	107.0
129.90	142.0
140.90	355.0
142.80	394.0
144.80	165.0
148.00	112.0
155.00	120.0
171.10	125.0
171.90	414.0
174.00	28224.0
175.00	2122.0
176.00	27232.0
177.00	1636.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	544.0
37.00	1830.0
38.00	1666.0
39.00	755.0
40.00	309.0
44.00	1377.0
45.10	361.0
46.00	118.0
47.00	573.0
48.00	258.0
49.00	1652.0
50.10	6705.0
51.00	2232.0
52.00	174.0
56.00	591.0
57.00	894.0
59.90	348.0
61.00	1749.0
62.00	1953.0
63.10	1489.0
64.00	285.0
65.10	376.0
67.10	151.0
68.00	3547.0
69.00	3766.0
69.90	333.0
71.90	211.0
73.00	1700.0
74.00	5732.0
75.10	17912.0
76.00	1676.0
77.00	268.0
78.90	1182.0
79.90	368.0
80.90	1163.0
81.90	381.0
87.00	1383.0
88.00	1317.0
92.00	1093.0
93.00	1592.0
94.00	4316.0
95.10	32768.0
96.00	2349.0
103.90	166.0
105.80	191.0
116.00	172.0
116.90	290.0
118.00	211.0
118.80	241.0
127.80	102.0
129.90	141.0
134.70	119.0
136.80	110.0
140.90	385.0
142.90	418.0
144.80	152.0
148.00	116.0
155.00	136.0
171.20	116.0
171.90	383.0
173.00	472.0
174.00	28480.0
175.00	2140.0
176.00	28072.0
177.00	1694.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

Scan 2790 (10.061 min): VV018934.D
BFB76

m/z	Abundance
39.90	255.0
44.00	937.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76