

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101623\
 Data File : VV032433.D
 Acq On : 16 Oct 2023 10:31
 Operator : SY/MD
 Sample : VV1016WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 17 04:47:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 16 02:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	7877	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	7425	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3908	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6378	0.494	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	98.000%		
4) 1,2-Dichloroethane-d4	4.946	65	3956	0.484	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
7) 1,2-Dichloropropane-d6	5.995	67	5075	0.498	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	100.000%		
8) Toluene-d8	7.253	98	12027	0.497	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3367	0.480	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	96.000%		
Target Compounds						
6) Trichloroethene	5.852	95	153	0.019	ug/L	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101623\
Data File : VV032433.D
Acq On : 16 Oct 2023 10:31
Operator : SY/MD
Sample : VV1016WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 17 04:47:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 16 02:50:34 2023
Response via : Initial Calibration

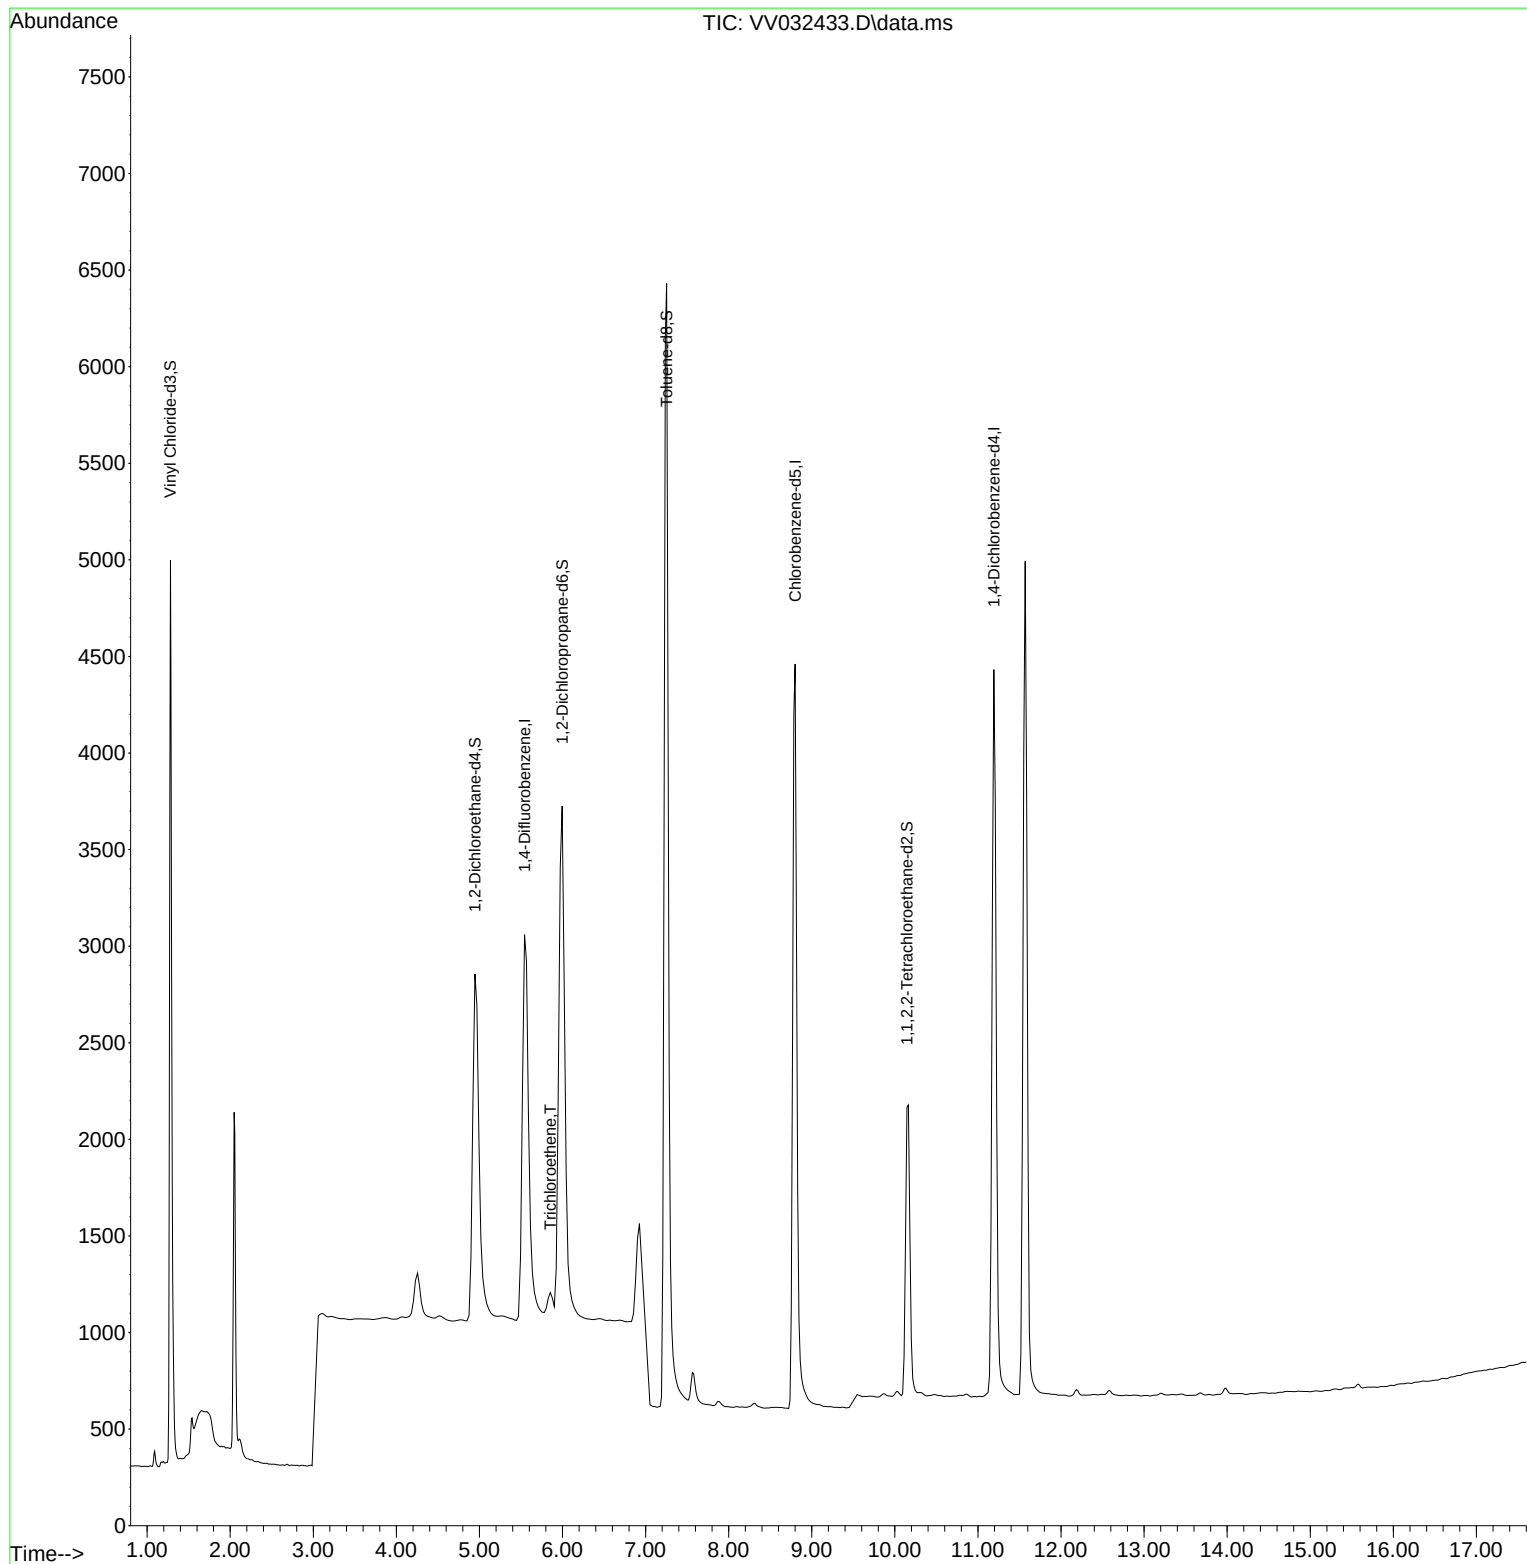

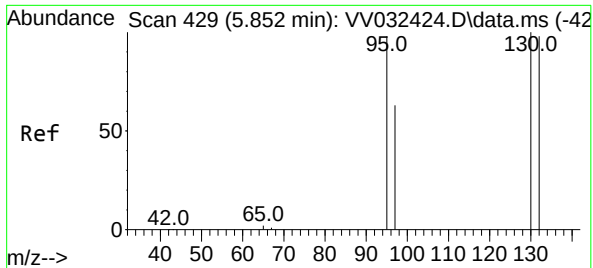

#6
 Trichloroethene
 Concen: 0.019 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV032433.D
 Acq: 16 Oct 2023 10:31

Instrument :
 MSVOA_V
 ClientSampleId :

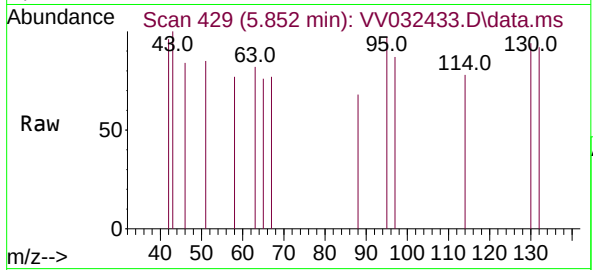

Tgt Ion: 95	Resp: 153
Ion Ratio	Lower Upper
95	100
97	89.8 47.3 87.9#
132	94.9 69.2 128.6
130	96.9 70.9 131.7

