


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101719\
 Data File : VV013173.D
 Acq On : 17 Oct 2019 15:43
 Operator : SY/MD
 Sample : BFB43
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB43

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 18 03:32:46 2019

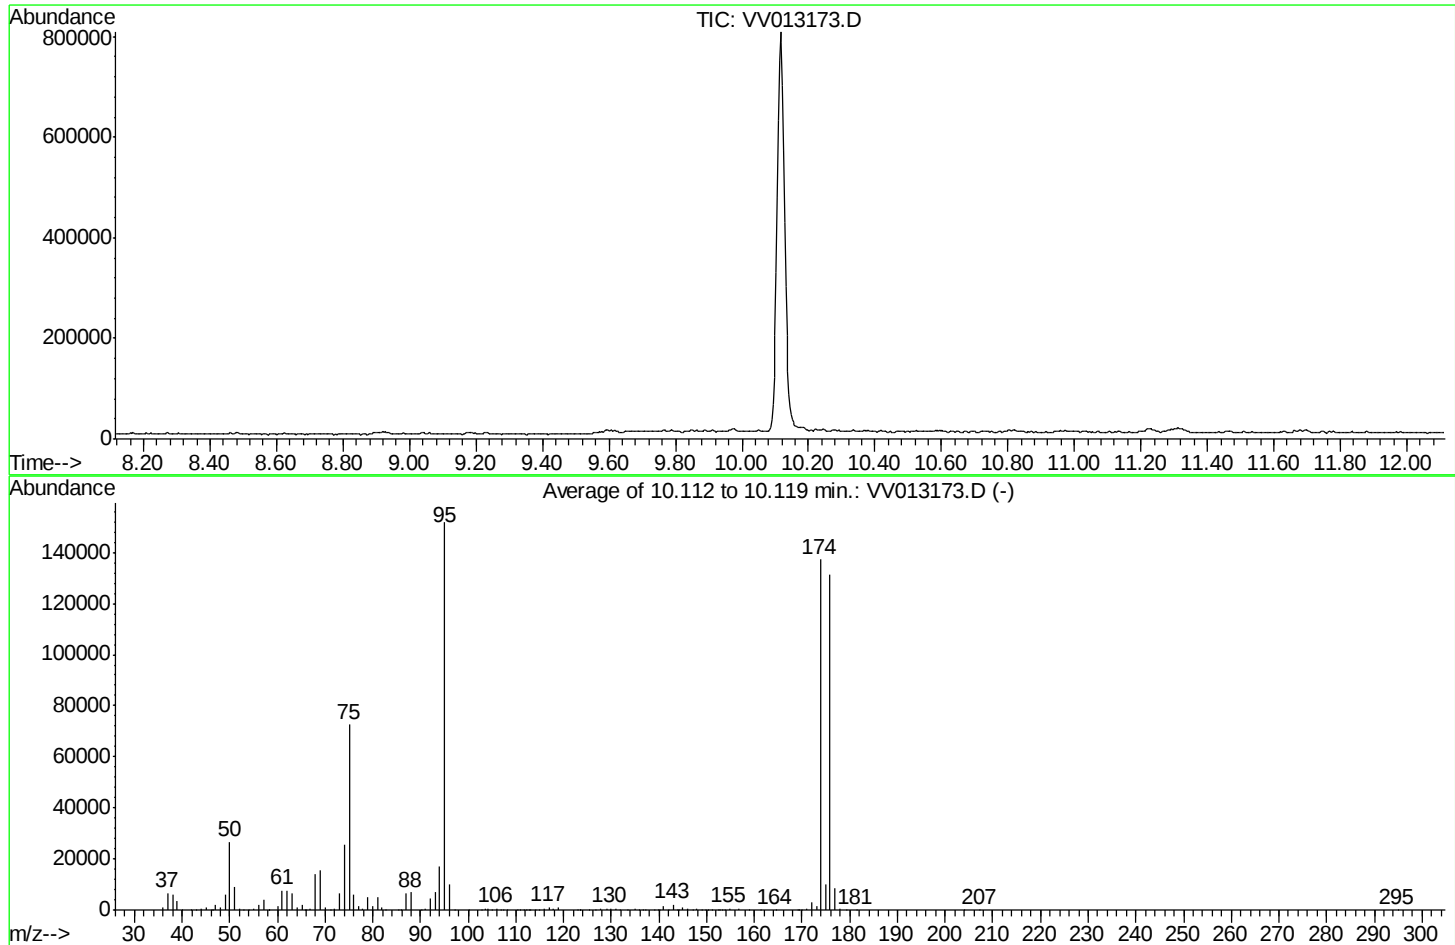

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	26807	PASS
75	95	30	80	47.8	72508	PASS
95	95	100	100	100.0	151808	PASS
96	95	5	9	6.5	9792	PASS
173	174	0.00	2	1.3	1728	PASS
174	95	50	120	90.4	137280	PASS
175	174	5	9	7.3	10028	PASS
176	174	95	101	95.8	131544	PASS
177	176	5	9	6.5	8591	PASS

m/z	Abundance
36.00	5365.0
37.00	7191.0
38.00	7482.0
39.00	3455.0
40.00	2088.0
41.80	153.0
42.10	147.0
43.00	317.0
44.00	2490.0
45.00	1238.0
46.10	470.0
47.00	2017.0
47.90	1021.0
49.00	6157.0
50.00	25936.0
51.00	9047.0
51.90	446.0
52.90	276.0
54.00	218.0
55.00	380.0
56.10	1866.0
57.00	3474.0
58.10	210.0
60.00	1508.0
61.00	7623.0
62.00	6943.0
63.00	6403.0
64.00	1292.0
65.10	2021.0
66.10	406.0
66.90	437.0
68.00	13807.0
69.00	15084.0
70.00	1354.0
71.10	271.0
71.90	754.0
73.00	6580.0
74.00	25456.0
75.00	70616.0
76.00	6165.0
77.00	1480.0
77.80	581.0
78.90	4702.0
80.00	1277.0
80.90	4662.0
81.90	1075.0
82.60	159.0
85.20	193.0
85.80	252.0
87.00	5993.0
87.90	7426.0
90.00	139.0
90.80	553.0
92.00	4208.0
93.00	6704.0
94.00	16632.0
95.00	146752.0
96.00	9790.0
97.00	279.0
102.70	137.0
103.70	508.0
104.10	512.0
105.00	238.0
105.90	606.0
106.80	143.0
107.30	105.0
110.20	143.0
110.80	133.0
111.80	186.0
112.20	193.0
113.10	165.0
114.00	134.0
114.90	162.0
115.90	651.0
116.90	1064.0
117.80	508.0
118.80	1009.0
123.30	123.0
123.70	149.0
125.30	107.0
126.60	157.0
127.80	536.0
129.00	372.0
129.90	482.0
130.90	310.0
131.60	114.0
133.30	124.0
134.80	229.0
135.90	111.0
136.70	224.0
137.20	257.0
139.10	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

139.70	175.0
140.10	166.0
140.80	1497.0
141.90	205.0
142.90	1781.0
144.20	122.0
144.80	813.0
145.80	347.0
147.90	572.0
151.00	132.0
152.30	118.0
152.80	126.0
153.80	157.0
154.80	521.0
156.80	327.0
158.90	126.0
169.40	131.0
170.90	316.0
171.90	2682.0
173.10	1636.0
173.90	130048.0
174.90	9687.0
175.90	121864.0
176.90	8069.0
177.90	417.0
207.30	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	5038.0
37.00	7357.0
38.00	7960.0
39.00	3585.0
39.90	1788.0
41.80	200.0
43.00	289.0
44.00	2627.0
45.10	1371.0
46.30	521.0
47.00	2154.0
47.90	1238.0
49.00	6186.0
50.00	27624.0
51.00	9570.0
52.00	445.0
53.00	219.0
54.00	192.0
55.00	441.0
56.10	2035.0
57.00	3920.0
58.30	213.0
60.00	1580.0
61.00	7941.0
62.00	7628.0
63.00	6837.0
64.00	1349.0
65.10	2257.0
66.10	338.0
66.90	486.0
68.00	14849.0
69.00	16302.0
70.00	1358.0
71.10	214.0
72.00	861.0
73.00	6457.0
74.00	26360.0
75.00	74944.0
76.00	6485.0
77.10	1517.0
77.90	670.0
78.90	5275.0
80.00	1340.0
81.00	5111.0
81.90	1013.0
82.70	165.0
85.20	153.0
85.90	201.0
86.90	6641.0
87.90	7191.0
90.10	175.0
90.90	579.0
92.00	4515.0
93.00	7304.0
94.00	17608.0
95.00	157120.0
96.00	10402.0
97.10	267.0
100.10	105.0
102.70	167.0
103.70	522.0
104.10	536.0
105.00	188.0
105.90	653.0
106.80	174.0
108.30	139.0
110.20	118.0
110.90	175.0
111.70	220.0
112.30	130.0
113.00	103.0
114.90	213.0
115.90	576.0
116.90	1228.0
117.80	529.0
118.90	1201.0
123.50	135.0
126.60	143.0
127.70	473.0
129.00	399.0
129.80	583.0
130.90	421.0
131.70	107.0
133.30	144.0
134.90	329.0
135.80	156.0
136.70	214.0
137.20	221.0
139.10	115.0
139.70	208.0
140.90	1449.0
142.00	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

142.90	2022.0
143.70	136.0
144.90	825.0
145.90	306.0
147.00	120.0
147.90	534.0
148.90	106.0
149.70	128.0
150.30	112.0
152.60	158.0
153.30	158.0
153.90	143.0
154.80	566.0
156.80	333.0
158.90	152.0
161.20	105.0
169.10	104.0
171.00	354.0
171.90	3011.0
173.00	1767.0
173.90	141696.0
174.90	10303.0
175.90	135744.0
176.90	8902.0
177.90	335.0
181.30	103.0
207.30	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	4743.0
37.00	7277.0
38.00	7382.0
39.00	3402.0
39.90	1581.0
40.80	210.0
41.90	212.0
43.00	258.0
44.00	2597.0
45.00	1371.0
47.00	2068.0
47.90	1281.0
49.00	5856.0
50.00	27232.0
51.00	8808.0
52.00	439.0
53.00	229.0
53.90	156.0
55.00	451.0
56.10	1932.0
57.00	4089.0
58.30	199.0
60.00	1522.0
61.00	7252.0
62.00	7638.0
63.10	6520.0
64.00	1102.0
65.10	2131.0
65.80	303.0
66.90	513.0
68.00	14536.0
69.00	15743.0
70.00	1169.0
71.10	129.0
72.00	840.0
73.00	6083.0
74.00	24400.0
75.00	72424.0
76.00	6070.0
77.10	1338.0
77.90	731.0
78.90	5327.0
80.00	1301.0
81.00	5268.0
81.90	951.0
82.80	180.0
86.00	260.0
86.90	6941.0
87.90	6343.0
90.10	162.0
90.90	648.0
92.00	4430.0
93.00	7116.0
94.00	16784.0
95.00	151552.0
96.00	9848.0
97.10	246.0
100.10	142.0
102.80	175.0
103.70	489.0
104.10	435.0
105.00	142.0
105.90	649.0
106.80	256.0
108.20	161.0
110.10	104.0
110.90	156.0
111.70	192.0
112.80	107.0
113.90	103.0
114.80	292.0
115.80	497.0
116.90	1338.0
117.80	576.0
118.90	1241.0
122.90	112.0
123.50	130.0
126.60	109.0
127.60	365.0
128.00	299.0
129.00	310.0
129.80	549.0
130.90	414.0
133.30	113.0
134.90	339.0
135.80	137.0
136.70	153.0
137.10	132.0
139.80	205.0
141.00	1334.0
142.90	2237.0
143.70	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

144.90	798.0
146.00	330.0
147.00	150.0
147.90	434.0
149.00	182.0
149.70	124.0
150.20	105.0
152.60	185.0
153.30	164.0
153.90	138.0
154.80	528.0
156.80	351.0
158.80	175.0
161.10	169.0
164.50	101.0
169.10	133.0
170.00	115.0
171.00	374.0
171.90	2950.0
172.90	1783.0
173.90	140096.0
174.90	10094.0
175.90	137024.0
176.90	8803.0
177.90	267.0
179.20	108.0
181.30	152.0
204.00	104.0
207.30	120.0
294.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	4128.0
37.00	508.0
37.90	1738.0
39.30	220.0
39.90	1634.0
41.00	232.0
41.40	142.0
42.10	193.0
43.10	150.0
43.90	1980.0
45.00	301.0
46.20	154.0
47.00	188.0
48.70	152.0
50.10	123.0
51.20	208.0
52.20	104.0
53.40	103.0
63.10	108.0
68.20	137.0
68.90	107.0
70.00	117.0
72.10	132.0
73.30	117.0
75.20	153.0
75.80	123.0
87.00	111.0
91.20	135.0
96.10	221.0
99.00	128.0
99.80	141.0
100.50	124.0
104.40	115.0
108.50	124.0
121.80	118.0
126.30	111.0
128.10	103.0
147.60	122.0
153.70	125.0
177.60	125.0
220.80	120.0
254.50	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43