




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032444.D
 Acq On : 17 Oct 2023 14:40
 Operator : SY/MD
 Sample : 04903-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 18 06:02:40 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
 Supervised By :Semsettin Yesilyurt 10/20/2023

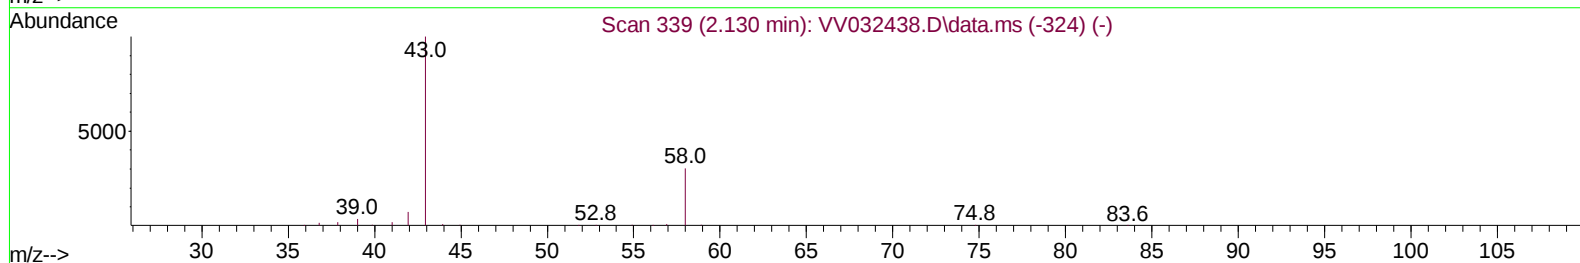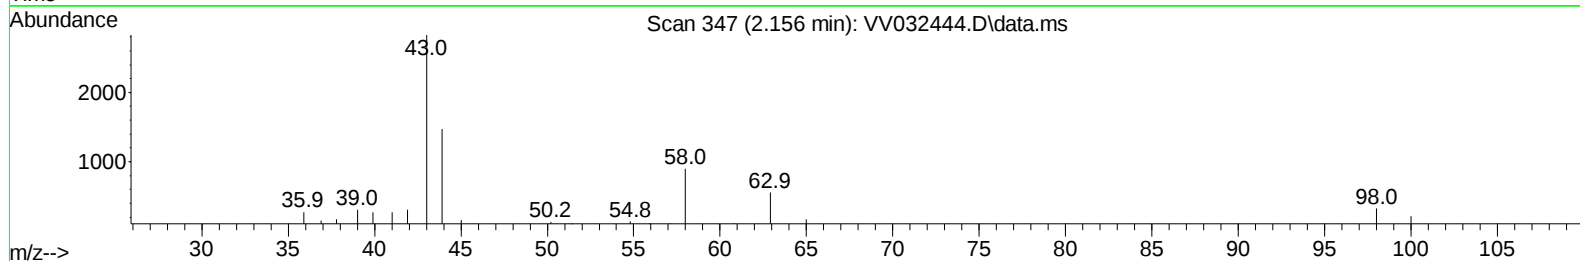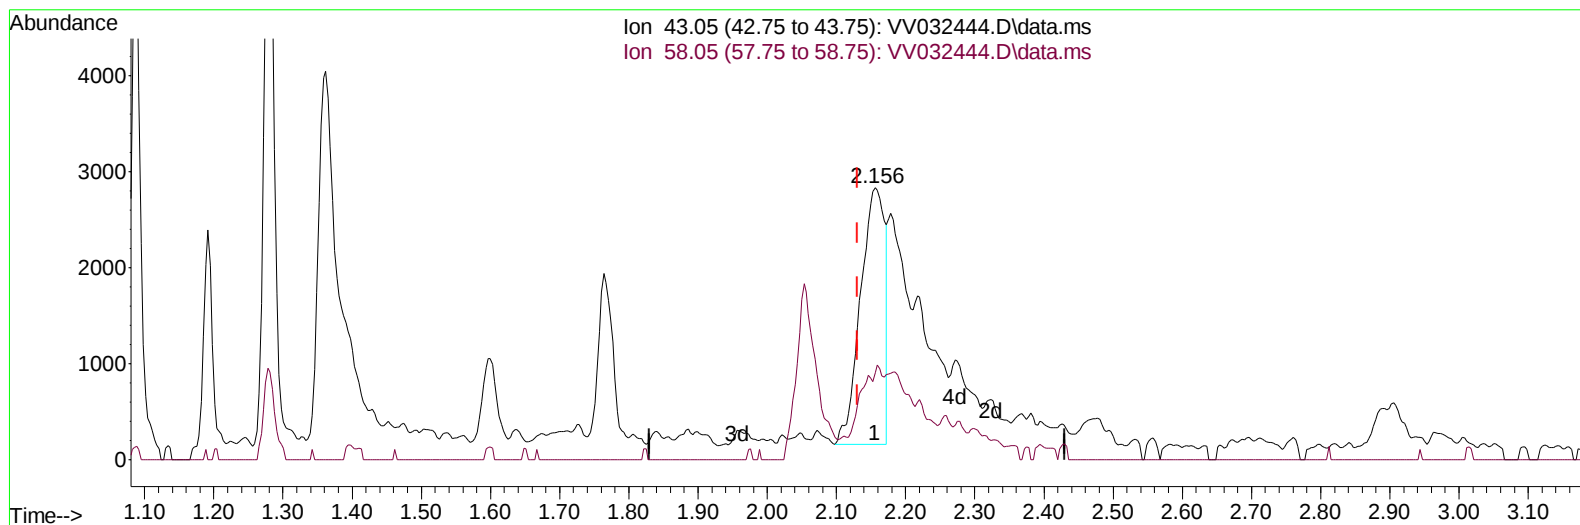

TIC: VV032444.D\data.ms

(13) Acetone (T)

2.156min (+ 0.026) 4.17 ug/L

response 6567

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	1.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032444.D
Acq On : 17 Oct 2023 14:40
Operator : SY/MD
Sample : 04903-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 18 06:02:40 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
Supervised By :Semsettin Yesilyurt 10/20/2023

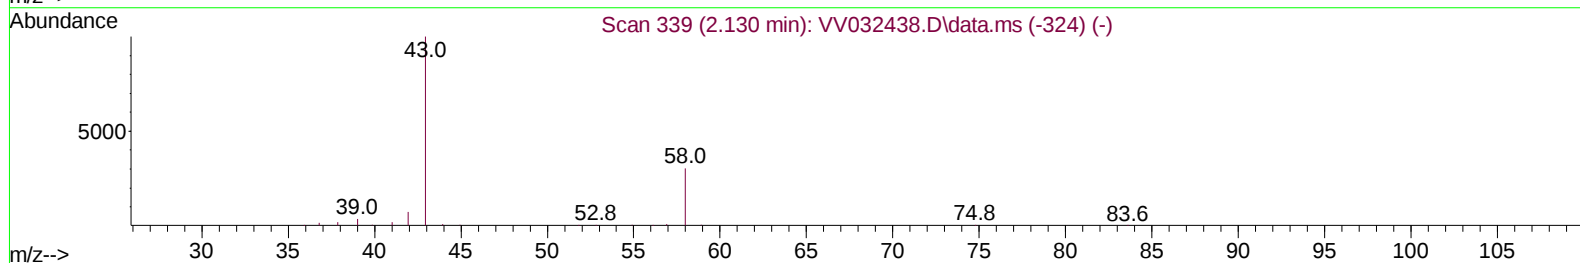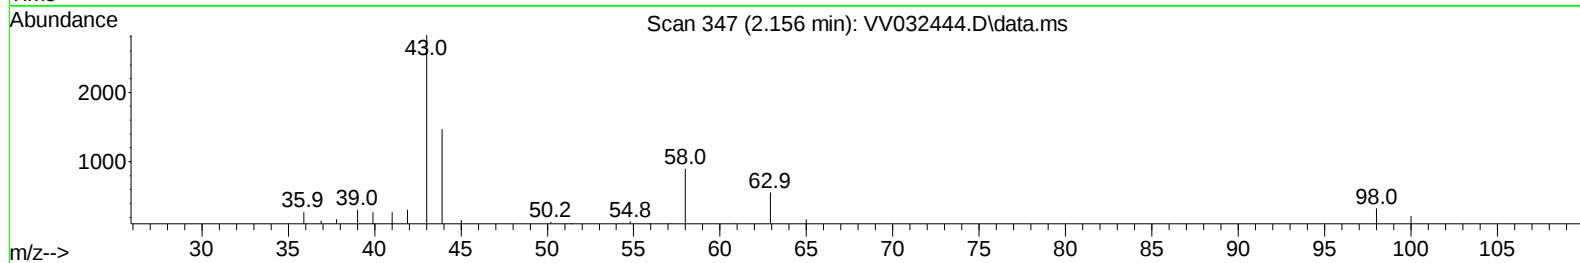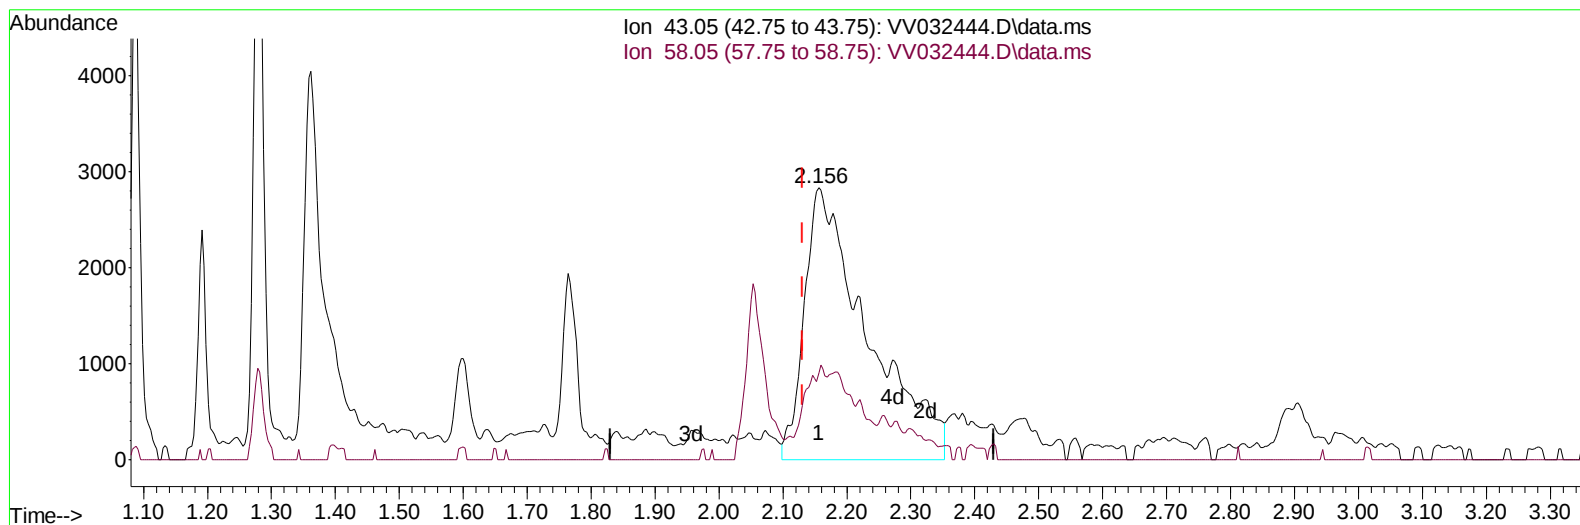

TIC: VV032444.D\data.ms

(13) Acetone (T)

2.156min (+ 0.026) 12.29 ug/L m

response 19350

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	0.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032444.D
 Acq On : 17 Oct 2023 14:40
 Operator : SY/MD
 Sample : 04903-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 18 06:02:40 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
 Supervised By :Semsettin Yesilyurt 10/20/2023

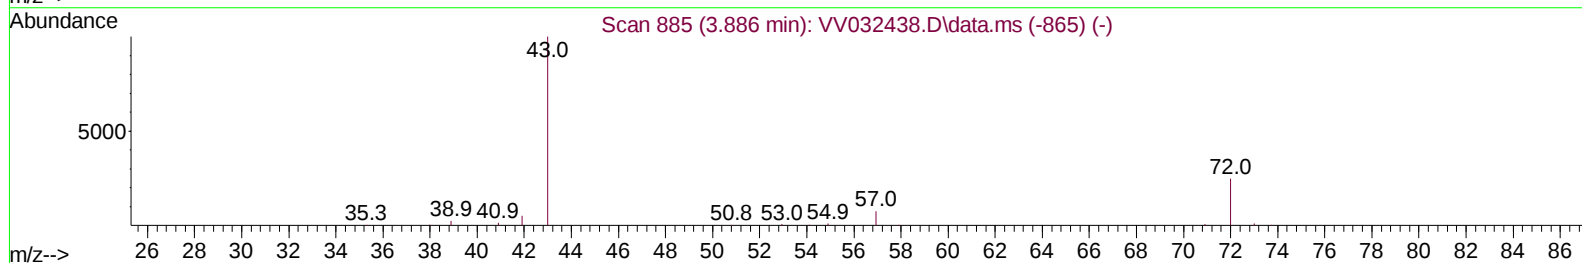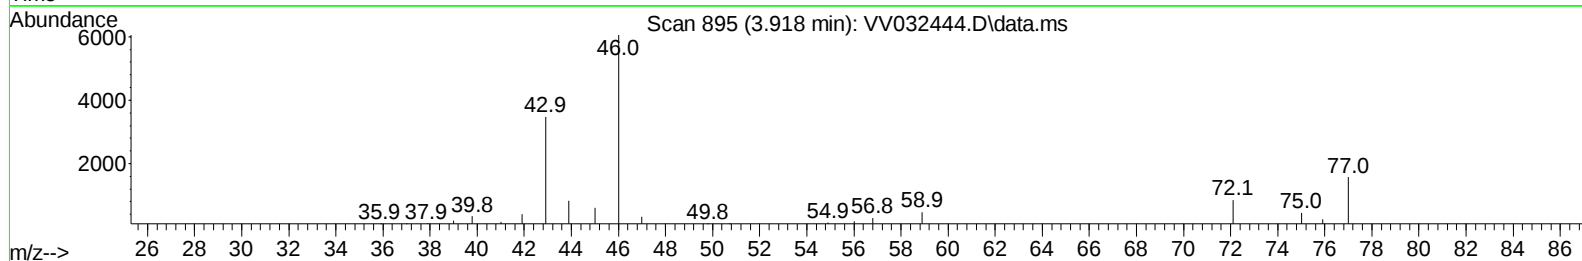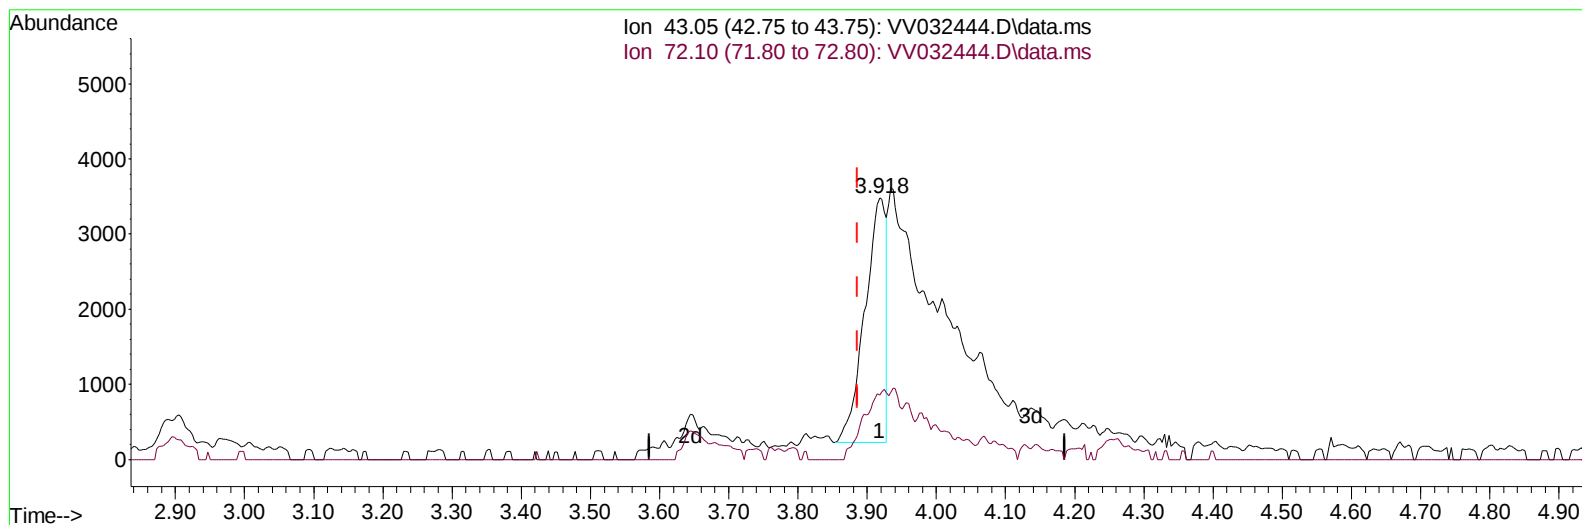

TIC: VV032444.D\data.ms

(21) 2-Butanone (T)

3.918min (+ 0.032) 2.80 ug/L

response 6895

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.20	32.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032444.D
Acq On : 17 Oct 2023 14:40
Operator : SY/MD
Sample : 04903-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 18 06:02:40 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
Supervised By :Semsettin Yesilyurt 10/20/2023

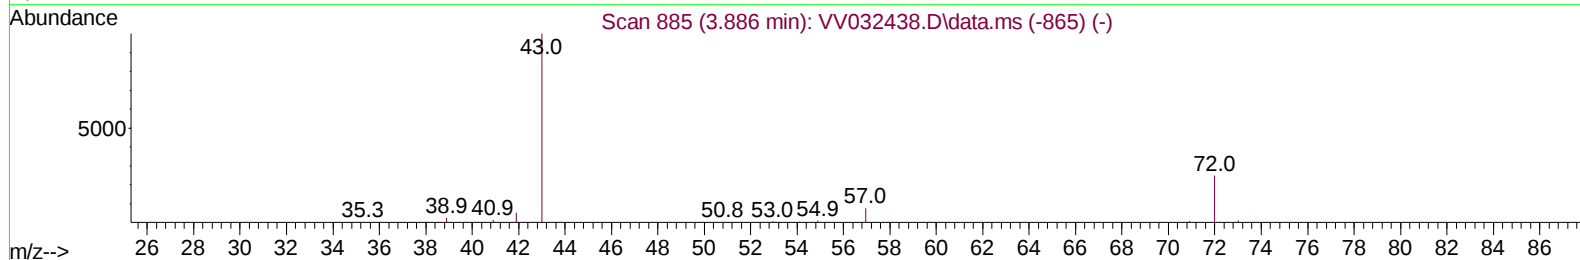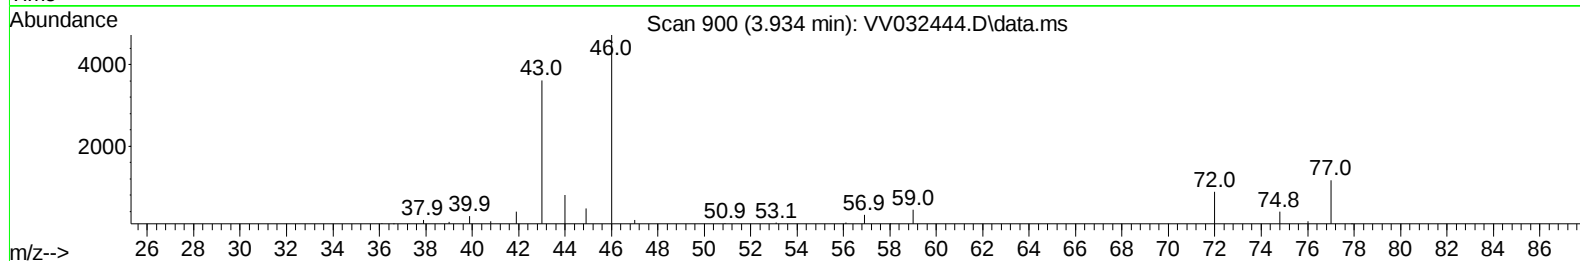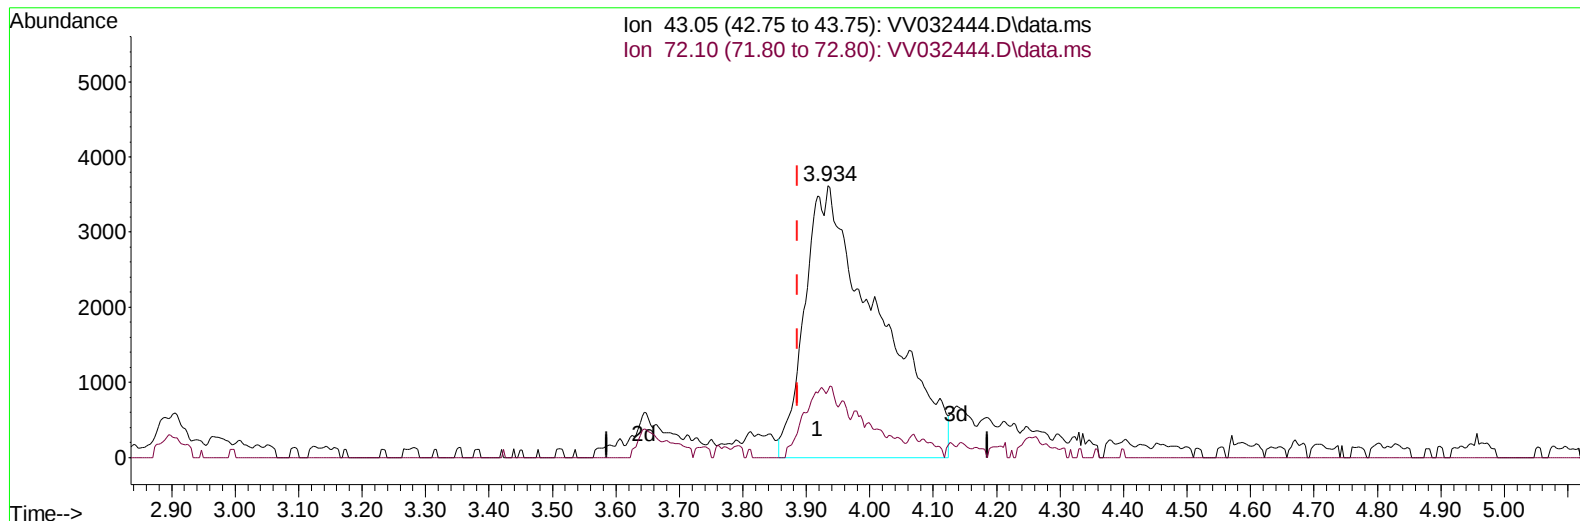

TIC: VV032444.D\data.ms

(21) 2-Butanone (T)

3.934min (+ 0.048) 11.74 ug/L m

response 28901

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.20	7.73#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032444.D
 Acq On : 17 Oct 2023 14:40
 Operator : SY/MD
 Sample : 04903-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 18 06:02:40 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
 Supervised By :Semsettin Yesilyurt 10/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	99318	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	107377	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	50297	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	32737	4.053	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	81.000%		
7) Chloroethane-d5	1.532	69	29908	4.561	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	91.200%		
11) 1,1-Dichloroethene-d2	2.060	65	13642	4.005	ug/L	0.01
Spiked Amount 5.000	Range 60 - 125		Recovery =	80.000%		
20) 2-Butanone-d5	3.831	46	91134	44.601	ug/L	0.03
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.200%		
24) Chloroform-d	4.252	84	66994	4.702	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.000%		
26) 1,2-Dichloroethane-d4	4.950	65	31215	4.625	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	92.400%		
32) Benzene-d6	4.966	84	117930	3.733	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	74.600%		
36) 1,2-Dichloropropane-d6	5.992	67	39720	3.794	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	75.800%		
41) Toluene-d8	7.249	98	105821	3.663	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	73.200%		
43) trans-1,3-Dichloroprop...	7.561	79	14705	3.964	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	79.200%		
46) 2-Hexanone-d5	8.034	63	87041	49.871	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	99.740%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	37063	5.062	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.200%		
66) 1,2-Dichlorobenzene-d4	11.564	152	44844	4.805	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	96.000%		
Target Compounds						
13) Acetone	2.156	43	19350m	12.287	ug/L	
21) 2-Butanone	3.934	43	28901m	11.735	ug/L	
25) Chloroform	4.281	83	8354	0.542	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032444.D
Acq On : 17 Oct 2023 14:40
Operator : SY/MD
Sample : 04903-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Manual IntegrationsAPPROVED

Quant Time: Oct 18 06:04:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 18 06:02:40 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/18/2023
Supervised By :Semsettin Yesilyurt 10/20/2023

