

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032439.D
 Acq On : 17 Oct 2023 12:39
 Operator : SY/MD
 Sample : VV1017WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK371

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	31	rVB	6336	8006	1.72%	0.238%
2	1.278	67	74	89	rVB	55314	59037	12.65%	1.757%
3	1.532	146	153	171	rVB	49754	59629	12.78%	1.774%
4	2.060	308	317	329	rBV	82009	120610	25.85%	3.589%
5	2.175	346	353	363	rVB2	5285	9365	2.01%	0.279%
6	2.452	431	439	451	rBV6	4025	7411	1.59%	0.221%
7	3.802	850	859	888	rBV	51360	158204	33.91%	4.707%
8	4.252	983	999	1021	rBV	63129	167315	35.86%	4.978%
9	4.371	1029	1036	1046	rVB3	2656	5074	1.09%	0.151%
10	4.960	1202	1219	1238	rBV3	140903	366663	78.59%	10.910%
11	5.539	1386	1399	1416	rBV	120791	252953	54.22%	7.527%
12	5.992	1527	1540	1556	rBV2	84712	185363	39.73%	5.515%
13	6.921	1819	1829	1857	rBV	36909	83713	17.94%	2.491%
14	7.249	1920	1931	1959	rBV	155332	307084	65.82%	9.137%
15	7.561	2019	2028	2051	rBV	21854	45479	9.75%	1.353%
16	8.030	2162	2174	2204	rBV	215533	466531	100.00%	13.882%
17	8.789	2397	2410	2433	rBV	199684	351055	75.25%	10.446%
18	10.156	2825	2835	2849	rBV	69916	114804	24.61%	3.416%
19	11.188	3145	3156	3176	rBV	194117	312290	66.94%	9.292%
20	11.564	3262	3273	3296	rBV	168465	274041	58.74%	8.154%
21	13.451	3852	3860	3868	rBV2	3840	6179	1.32%	0.184%




Sum of corrected areas: 3360806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032439.D
Acq On : 17 Oct 2023 12:39
Operator : SY/MD
Sample : VV1017WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

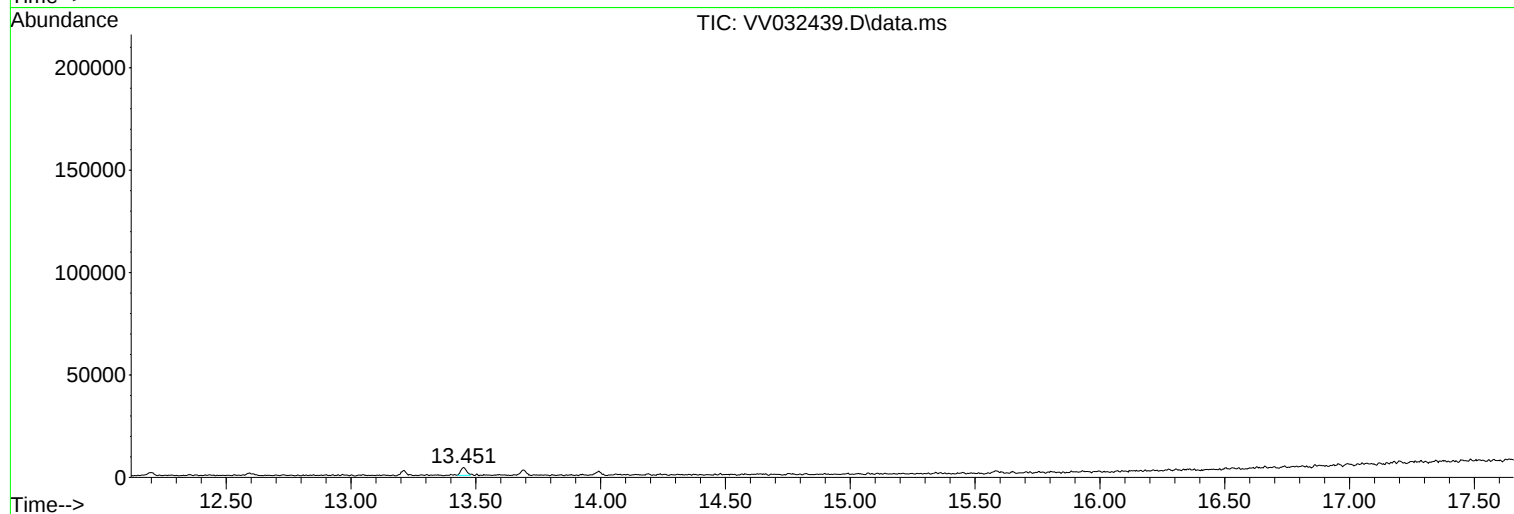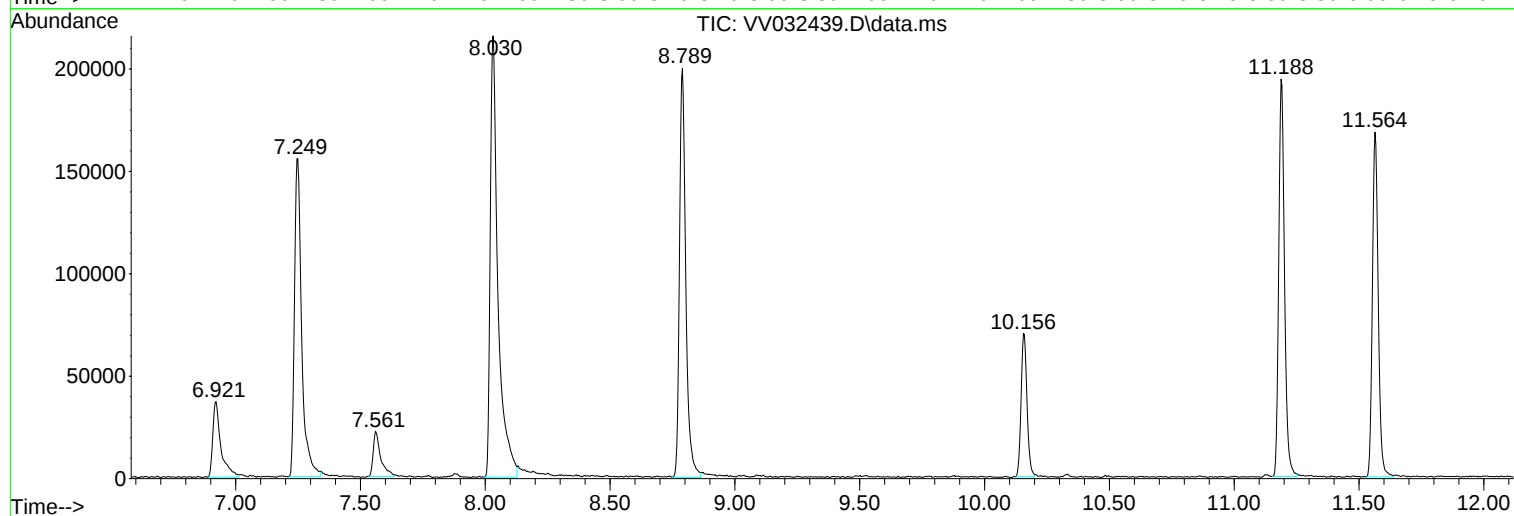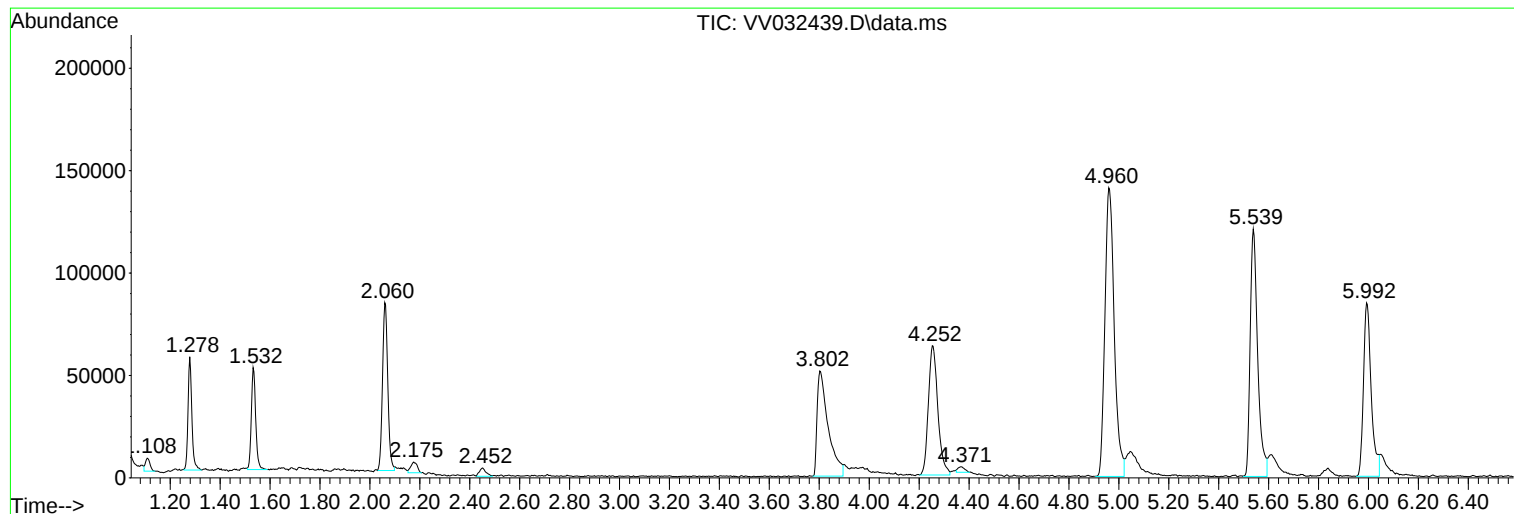

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032439.D
Acq On : 17 Oct 2023 12:39
Operator : SY/MD
Sample : VV1017WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032439.D
Acq On : 17 Oct 2023 12:39
Operator : SY/MD
Sample : VV1017WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc