

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032447.D
 Acq On : 17 Oct 2023 15:54
 Operator : SY/MD
 Sample : 04903-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	19	rVV	9120	8418	1.65%	0.246%
2	1.121	19	25	33	rVB	11477	16186	3.17%	0.473%
3	1.278	66	74	88	rBV2	57446	70471	13.79%	2.058%
4	1.536	146	154	168	rVB	46304	56516	11.06%	1.651%
5	1.729	209	214	222	rVB3	6597	7810	1.53%	0.228%
6	2.063	307	318	329	rBV	73320	110542	21.63%	3.229%
7	2.185	350	356	369	rVB3	5916	10882	2.13%	0.318%
8	2.709	509	519	532	rBV4	7379	15986	3.13%	0.467%
9	3.802	849	859	885	rBV	57775	172007	33.66%	5.024%
10	4.256	984	1000	1024	rBV2	60436	162413	31.79%	4.744%
11	4.963	1204	1220	1239	rBV3	127501	335939	65.75%	9.812%
12	5.060	1243	1250	1264	rVB3	9705	23205	4.54%	0.678%
13	5.211	1286	1297	1313	rVB4	5259	13095	2.56%	0.382%
14	5.539	1388	1399	1416	rBV	116030	244258	47.80%	7.134%
15	5.995	1526	1541	1556	rBV2	78364	171573	33.58%	5.011%
16	6.921	1819	1829	1844	rBV	34225	69993	13.70%	2.044%
17	7.249	1917	1931	1956	rBV	139442	275604	53.94%	8.049%
18	7.561	2018	2028	2054	rBV2	20412	46258	9.05%	1.351%
19	7.879	2113	2127	2141	rBV2	7895	17070	3.34%	0.499%
20	8.031	2162	2174	2211	rBV2	239619	510972	100.00%	14.924%
21	8.789	2398	2410	2436	rBV	191755	339557	66.45%	9.917%
22	10.159	2825	2836	2852	rBV	71121	116990	22.90%	3.417%
23	10.329	2876	2889	2900	rVB2	16530	27680	5.42%	0.808%
24	11.188	3145	3156	3175	rBV	193362	310492	60.76%	9.068%
25	11.564	3262	3273	3291	rVV	165875	265059	51.87%	7.741%
26	12.201	3460	3471	3481	rVB2	8943	16048	3.14%	0.469%
27	17.043	4972	4977	4985	rVB	7048	8858	1.73%	0.259%




Sum of corrected areas: 3423882

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032447.D
Acq On : 17 Oct 2023 15:54
Operator : SY/MD
Sample : 04903-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

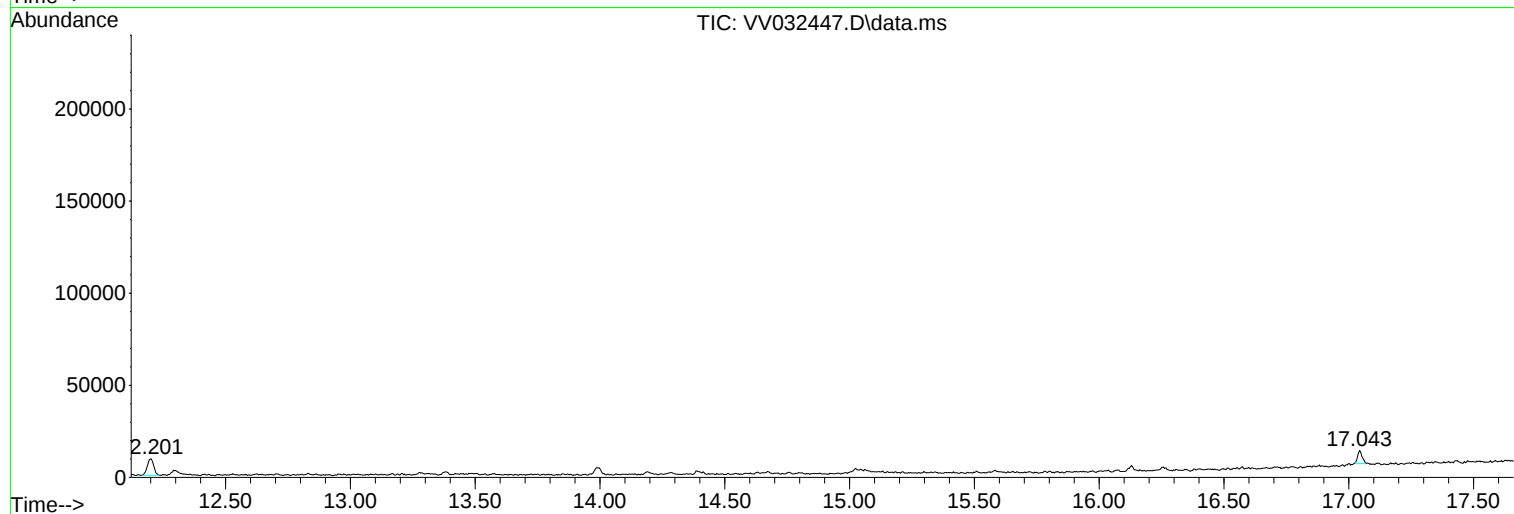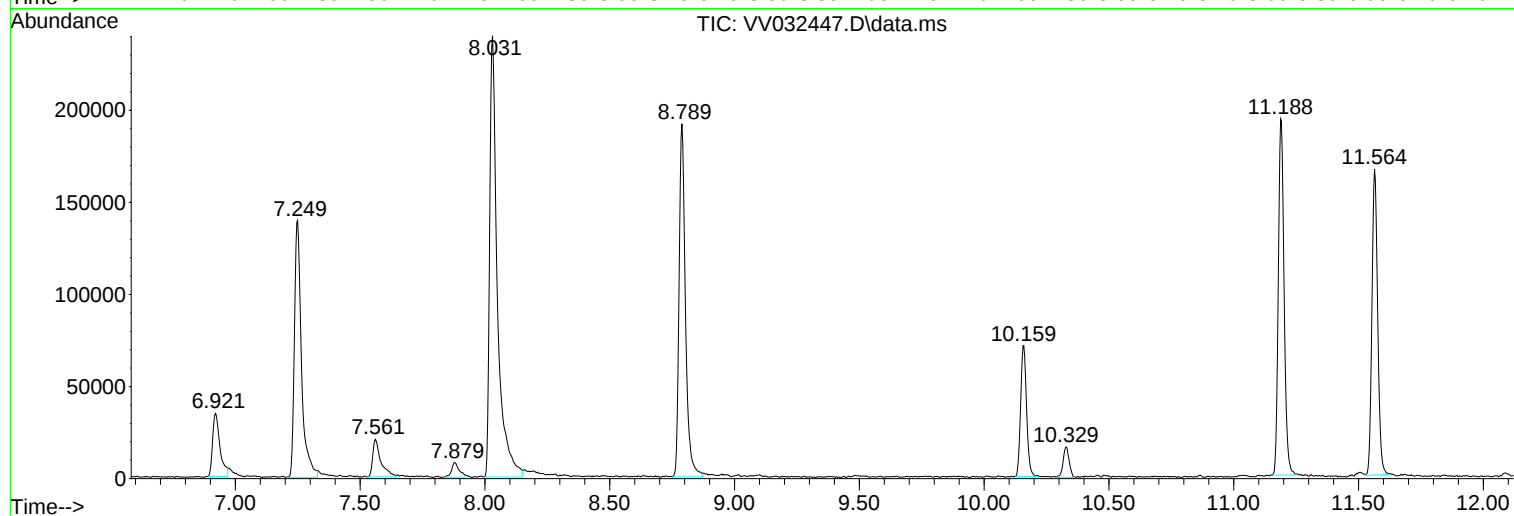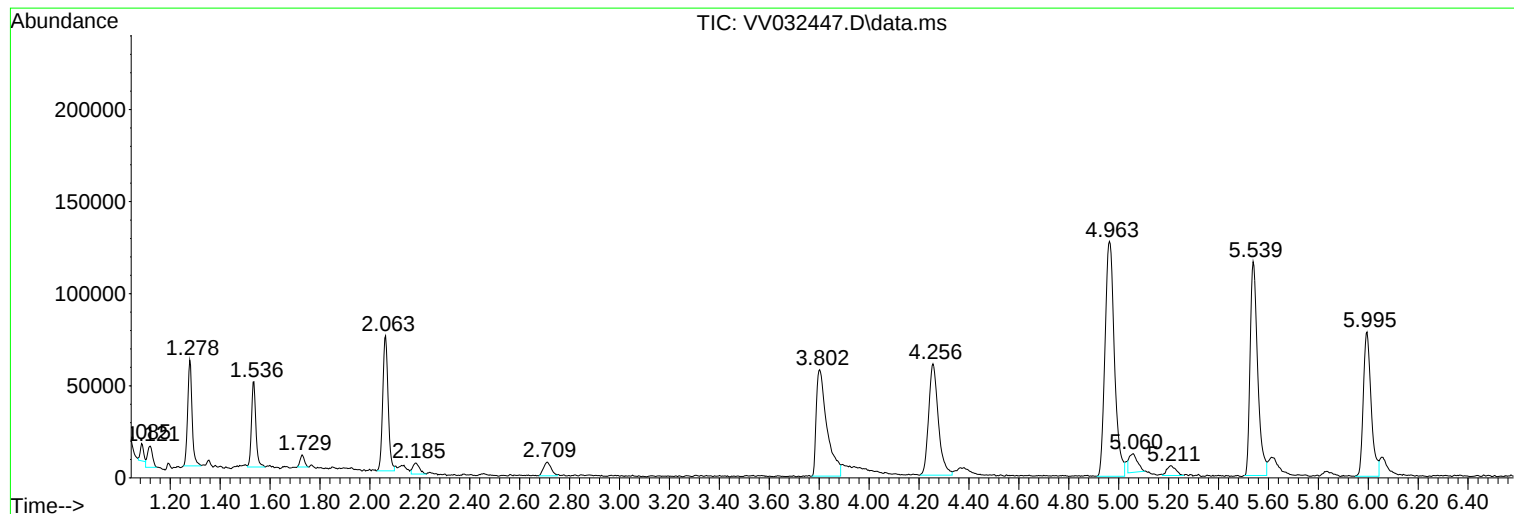

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032447.D
Acq On : 17 Oct 2023 15:54
Operator : SY/MD
Sample : 04903-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032447.D
Acq On : 17 Oct 2023 15:54
Operator : SY/MD
Sample : 04903-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc