

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032449.D
 Acq On : 17 Oct 2023 16:40
 Operator : SY/MD
 Sample : 04903-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	18	rBV2	9940	9758	2.05%	0.295%
2	1.114	19	23	35	rVB	11621	15772	3.31%	0.477%
3	1.275	64	73	89	rBV2	56662	74890	15.74%	2.267%
4	1.352	93	97	104	rVB	5762	5643	1.19%	0.171%
5	1.532	146	153	164	rVB	44681	51363	10.79%	1.555%
6	1.728	207	214	222	rBV2	7869	10199	2.14%	0.309%
7	2.060	306	317	331	rBV	72465	109492	23.01%	3.314%
8	2.178	349	354	365	rVB3	4516	7816	1.64%	0.237%
9	2.712	506	520	535	rBV	7135	17311	3.64%	0.524%
10	3.799	845	858	882	rBV	55778	162090	34.06%	4.906%
11	4.256	984	1000	1024	rBV2	55856	151680	31.87%	4.591%
12	4.963	1203	1220	1239	rBV3	122954	320741	67.40%	9.708%
13	5.050	1244	1247	1263	rVB7	8841	19010	3.99%	0.575%
14	5.211	1289	1297	1305	rBV3	3610	6779	1.42%	0.205%
15	5.538	1387	1399	1416	rBV	110301	236508	49.70%	7.158%
16	5.609	1417	1421	1441	rVB5	8713	22881	4.81%	0.693%
17	5.995	1526	1541	1555	rBV	75970	162560	34.16%	4.920%
18	6.921	1818	1829	1842	rBV2	32853	65420	13.75%	1.980%
19	7.249	1919	1931	1958	rBV	133274	260588	54.76%	7.887%
20	7.564	2019	2029	2055	rBV	20398	44258	9.30%	1.340%
21	7.882	2115	2128	2146	rVB3	9383	20543	4.32%	0.622%
22	8.030	2164	2174	2212	rBV	222009	475862	100.00%	14.403%
23	8.789	2398	2410	2432	rBV	184192	325229	68.35%	9.844%
24	10.159	2822	2836	2852	rBV	67924	111926	23.52%	3.388%
25	10.329	2879	2889	2899	rBV2	20985	33411	7.02%	1.011%
26	11.191	3142	3157	3178	rBV	186367	303832	63.85%	9.196%
27	11.564	3261	3273	3289	rBV	154889	249434	52.42%	7.550%
28	12.197	3461	3470	3480	rBV	11161	18365	3.86%	0.556%
29	13.988	4021	4027	4040	rVB2	3187	5556	1.17%	0.168%
30	17.043	4972	4977	4985	rVB6	3746	5017	1.05%	0.152%




Sum of corrected areas: 3303934

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032449.D
Acq On : 17 Oct 2023 16:40
Operator : SY/MD
Sample : 04903-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

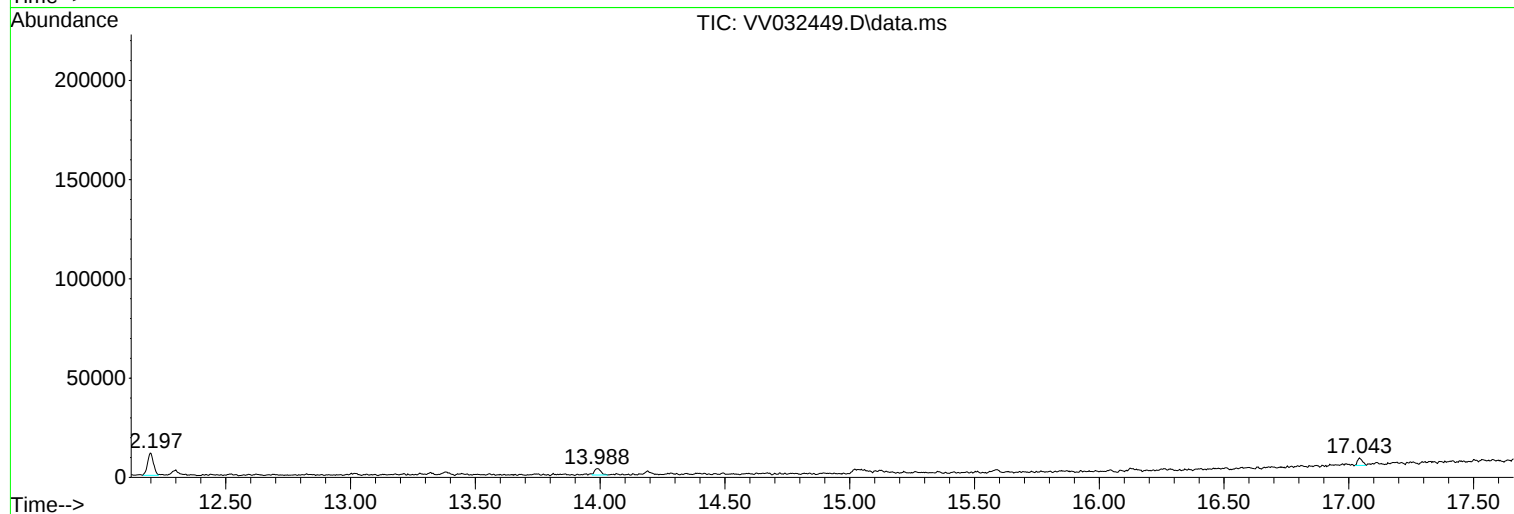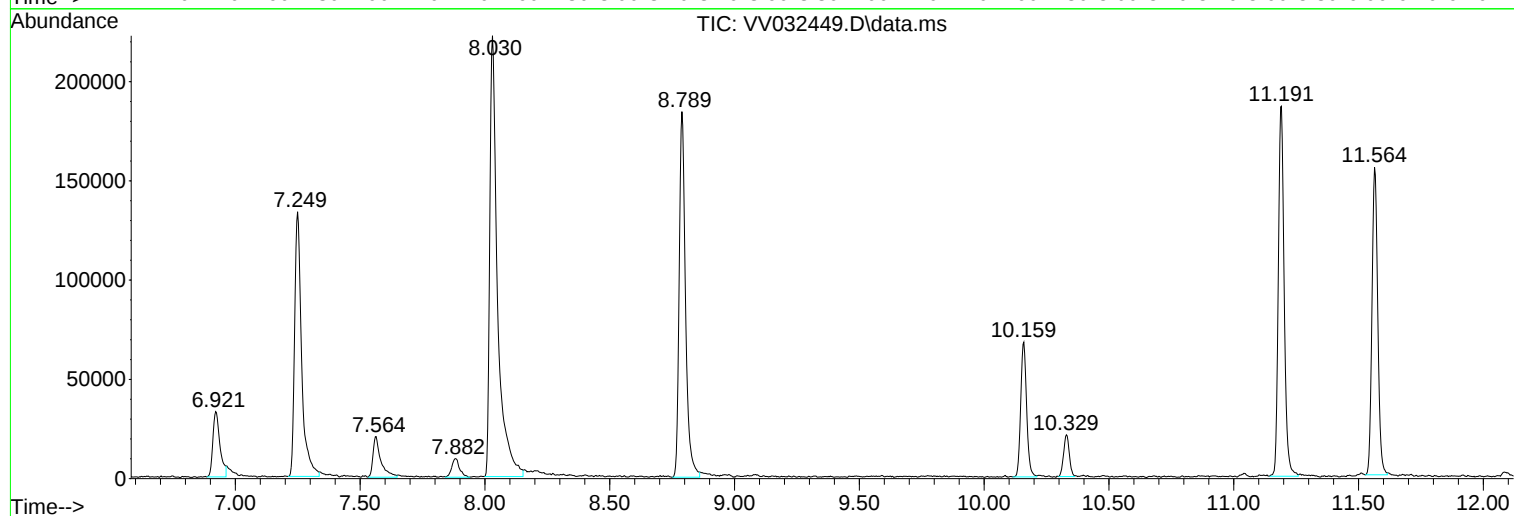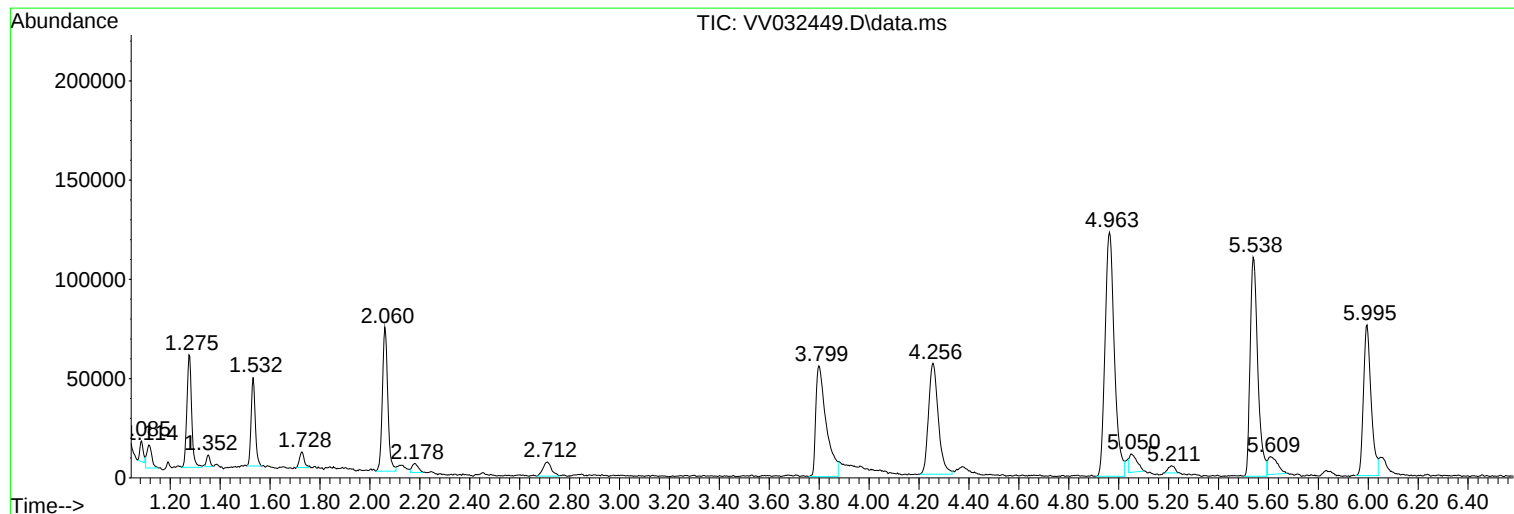

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032449.D
Acq On : 17 Oct 2023 16:40
Operator : SY/MD
Sample : 04903-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032449.D
Acq On : 17 Oct 2023 16:40
Operator : SY/MD
Sample : 04903-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
