

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
 Data File : VV032450.D
 Acq On : 17 Oct 2023 17:05
 Operator : SY/MD
 Sample : 04903-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	19	rBV	6577	6240	1.30%	0.188%
2	1.114	19	23	32	rVB	6833	8445	1.76%	0.254%
3	1.278	65	74	87	rBV	52909	61138	12.73%	1.842%
4	1.352	91	97	105	rBV	9826	11538	2.40%	0.348%
5	1.532	146	153	167	rVB	45373	52637	10.96%	1.586%
6	2.060	306	317	329	rBV	72331	106491	22.18%	3.208%
7	2.182	350	355	363	rVB3	5095	7585	1.58%	0.228%
8	3.802	849	859	884	rBV	52756	163610	34.07%	4.928%
9	4.256	984	1000	1026	rBV2	60907	175532	36.55%	5.288%
10	4.372	1028	1036	1055	rVB7	3422	10401	2.17%	0.313%
11	4.960	1204	1219	1240	rBV3	123348	323243	67.32%	9.737%
12	5.056	1242	1249	1269	rVB6	10132	28863	6.01%	0.869%
13	5.539	1388	1399	1416	rBV	117419	244024	50.82%	7.351%
14	5.828	1483	1489	1503	rVB7	2837	5254	1.09%	0.158%
15	5.995	1528	1541	1555	rBV	74900	162774	33.90%	4.903%
16	6.921	1816	1829	1863	rBV2	32570	74918	15.60%	2.257%
17	7.249	1918	1931	1952	rBV	134302	258358	53.80%	7.783%
18	7.561	2017	2028	2041	rBV2	20745	39385	8.20%	1.186%
19	7.879	2115	2127	2147	rBV3	9029	22478	4.68%	0.677%
20	8.031	2163	2174	2209	rBV	219120	480187	100.00%	14.465%
21	8.789	2400	2410	2437	rBV	189087	333354	69.42%	10.042%
22	10.156	2825	2835	2855	rBV	68455	112431	23.41%	3.387%
23	10.329	2875	2889	2900	rVB	20790	33667	7.01%	1.014%
24	11.188	3146	3156	3178	rBV	193021	309489	64.45%	9.323%
25	11.500	3242	3253	3262	rBV4	7487	16765	3.49%	0.505%
26	11.564	3262	3273	3292	rVB	157452	255596	53.23%	7.699%
27	12.198	3461	3470	3479	rVB	9557	15286	3.18%	0.460%




Sum of corrected areas: 3319689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032450.D
Acq On : 17 Oct 2023 17:05
Operator : SY/MD
Sample : 04903-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

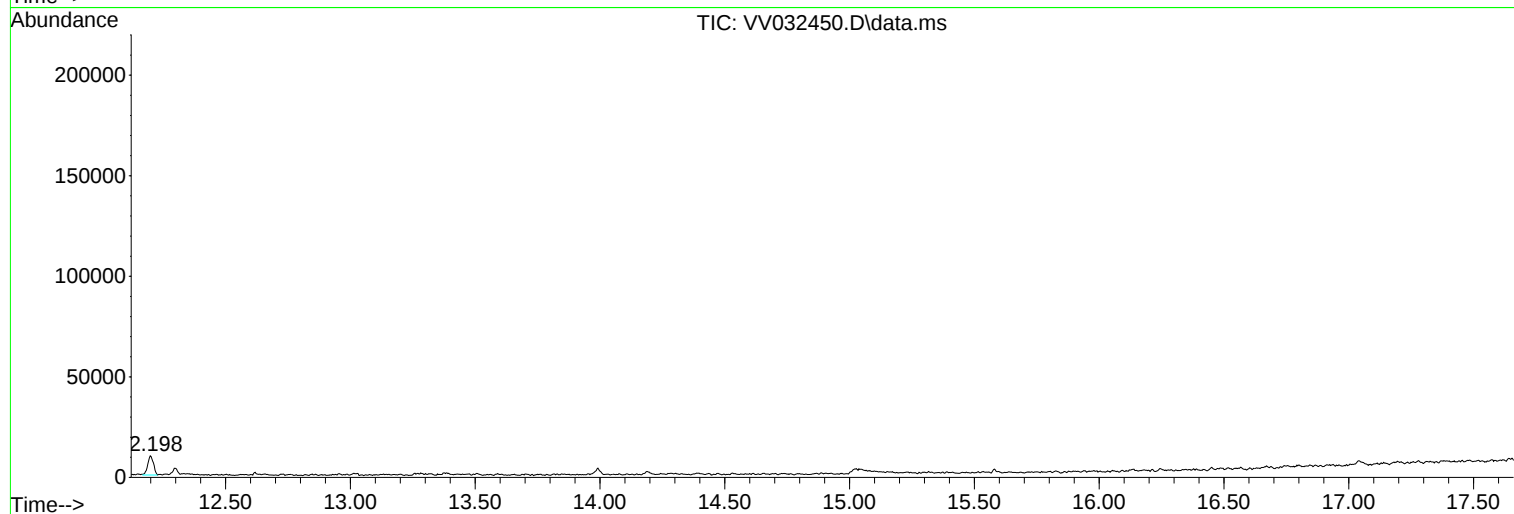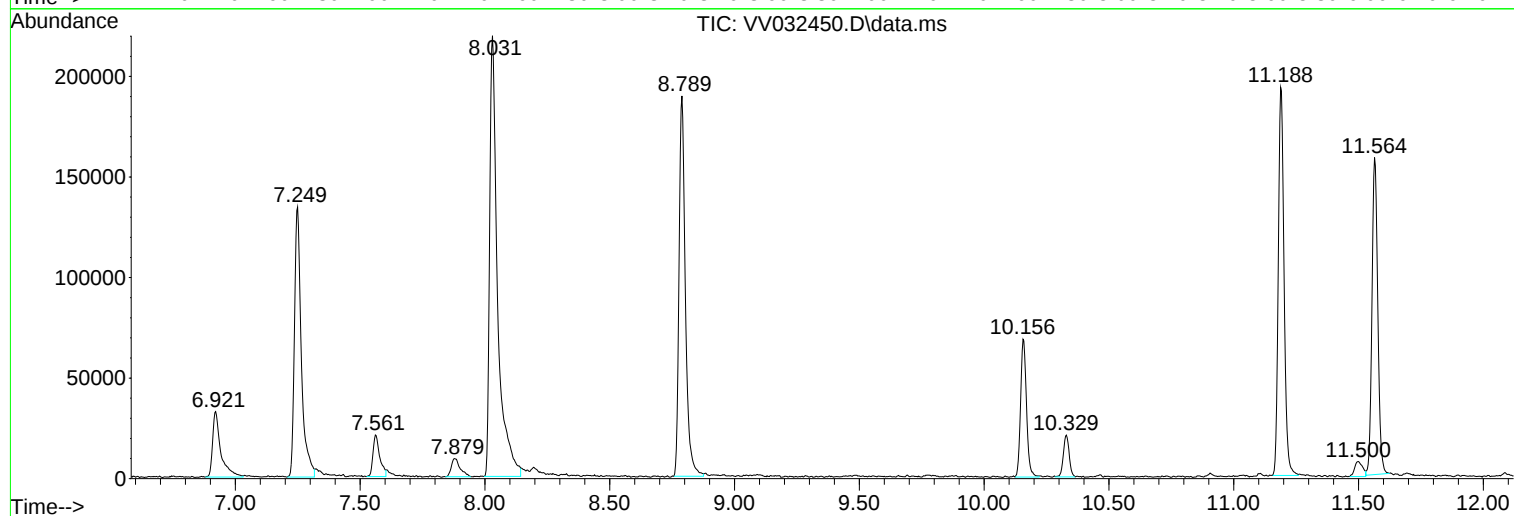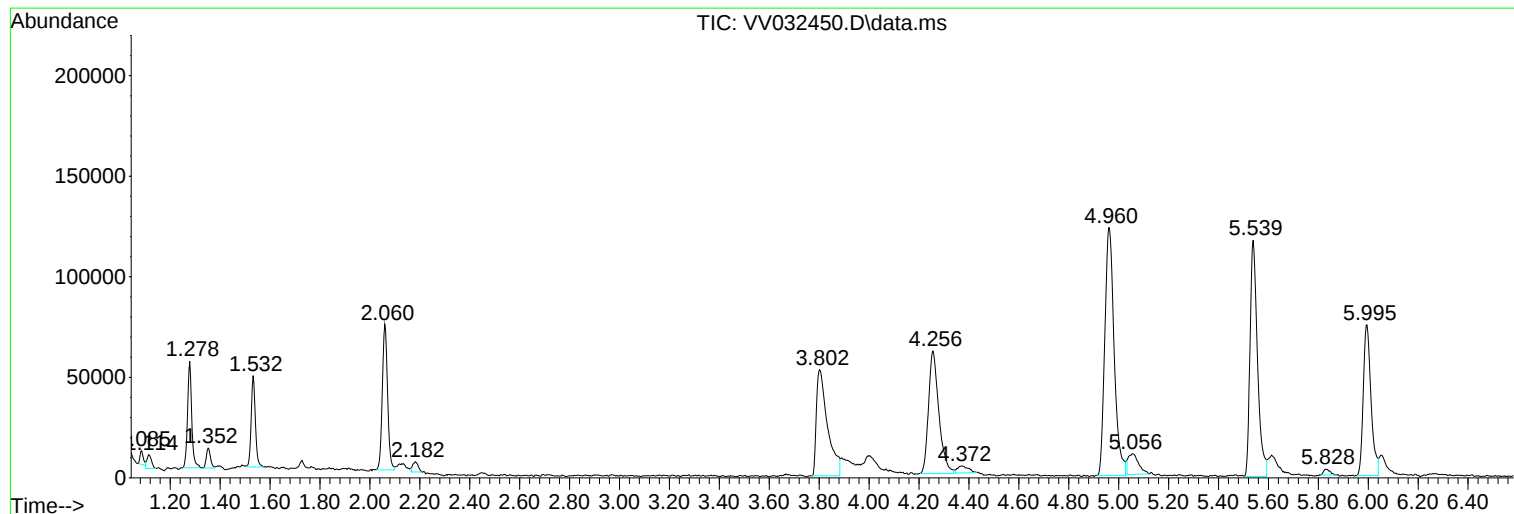

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032450.D
Acq On : 17 Oct 2023 17:05
Operator : SY/MD
Sample : 04903-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032450.D
Acq On : 17 Oct 2023 17:05
Operator : SY/MD
Sample : 04903-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------