
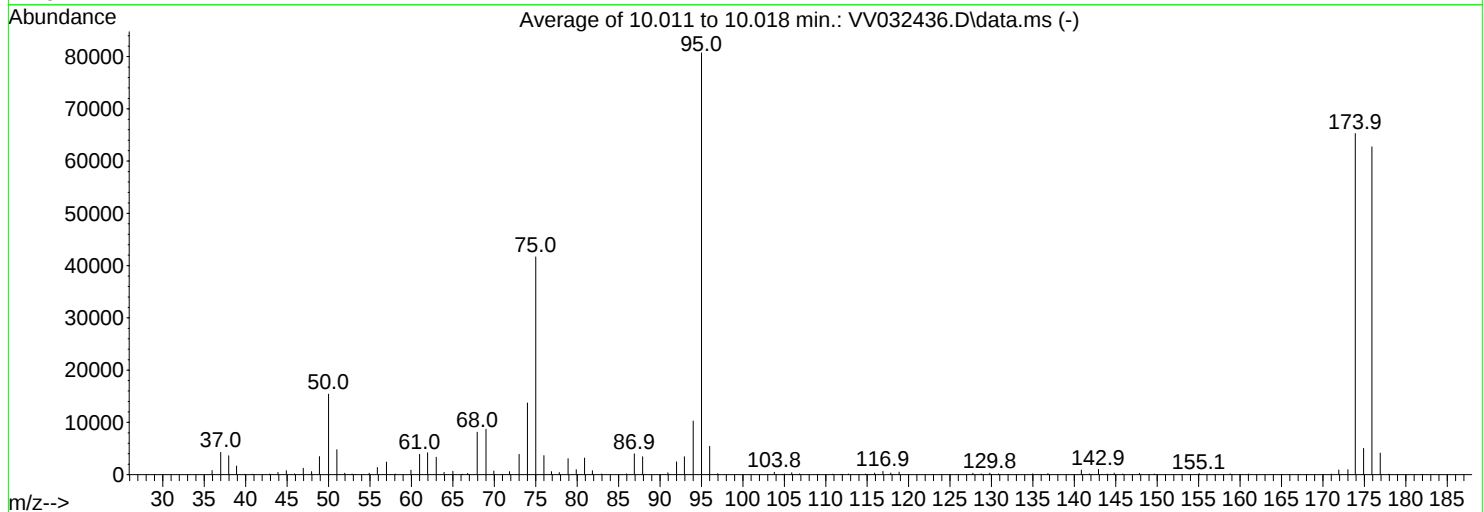


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101723\
Data File : VV032436.D
Acq On : 17 Oct 2023 08:43
Operator : SY/MD
Sample : BFB221
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB221

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 20 06:17:42 2023

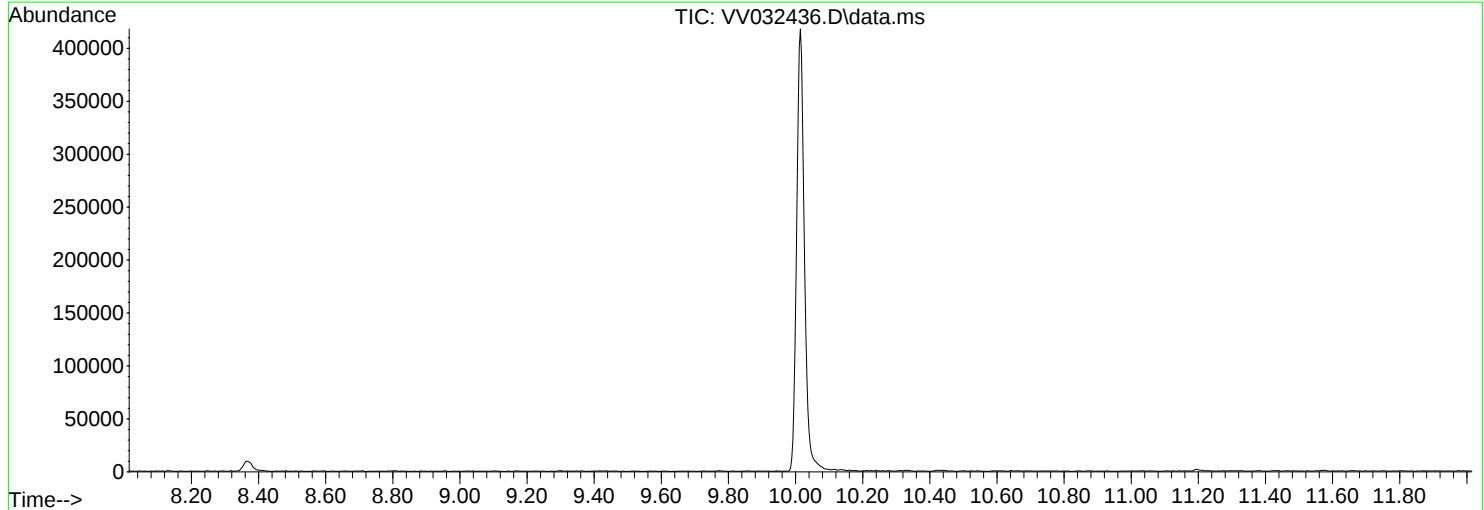

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	15394	PASS
75	95	30	80	51.6	41685	PASS
95	95	100	100	100.0	80717	PASS
96	95	5	9	6.7	5414	PASS
173	174	0.00	2	1.4	940	PASS
174	95	50	120	80.9	65277	PASS
175	174	5	9	7.7	5013	PASS
176	174	95	105	96.1	62731	PASS
177	176	5	10	6.6	4124	PASS

m/z	Abundance
35.80	103.0
37.00	109.0
40.00	179.0
43.90	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	920.0
37.00	4512.0
38.00	3666.0
38.90	1573.0
39.80	293.0
42.90	126.0
43.90	742.0
44.90	803.0
45.90	155.0
46.90	1283.0
47.90	594.0
48.90	3509.0
50.00	15733.0
51.00	4791.0
51.90	334.0
53.00	119.0
54.90	264.0
55.90	1380.0
57.00	2510.0
58.00	124.0
59.90	859.0
61.00	3833.0
62.00	4278.0
63.00	3429.0
63.90	497.0
65.00	615.0
66.80	229.0
67.90	8367.0
69.00	8811.0
70.00	678.0
71.90	625.0
73.00	3966.0
74.00	13728.0
75.00	41928.0
76.00	3641.0
76.90	573.0
77.80	379.0
78.90	3045.0
79.90	894.0
80.90	3100.0
81.90	697.0
82.90	128.0
86.00	167.0
86.90	4041.0
87.90	3486.0
90.90	385.0
92.00	2425.0
93.00	3545.0
94.00	10038.0
95.00	81024.0
96.00	5381.0
96.90	170.0
103.80	485.0
104.80	168.0
105.90	380.0
106.80	169.0
110.80	130.0
112.80	108.0
114.80	127.0
115.90	297.0
116.90	634.0
117.90	321.0
118.90	552.0
127.70	249.0
128.70	159.0
129.80	309.0
130.80	137.0
135.00	146.0
136.80	212.0
140.80	835.0
141.80	143.0
142.90	948.0
143.90	125.0
144.80	293.0
145.90	125.0
147.80	224.0
149.70	134.0
155.00	207.0
158.80	145.0
161.00	101.0
170.90	116.0
171.90	900.0
173.00	936.0
173.90	62952.0
174.90	4970.0
175.90	60744.0
176.90	4179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	955.0
37.00	4510.0
38.00	3748.0
38.90	1694.0
39.90	258.0
40.80	100.0
42.90	115.0
43.90	778.0
44.90	784.0
45.90	176.0
47.00	1271.0
48.00	600.0
48.90	3598.0
50.00	15853.0
51.00	4921.0
52.00	259.0
52.80	116.0
54.90	283.0
55.90	1415.0
57.00	2520.0
58.10	132.0
59.90	863.0
61.00	4063.0
61.90	4319.0
63.00	3408.0
64.00	454.0
65.00	640.0
66.20	128.0
66.80	253.0
67.90	8318.0
69.00	9015.0
70.00	761.0
71.90	593.0
73.00	4018.0
74.00	14159.0
75.00	43088.0
76.00	3783.0
76.90	580.0
77.90	411.0
78.90	3135.0
79.90	970.0
80.90	3235.0
81.90	793.0
82.90	131.0
85.90	160.0
86.90	4104.0
87.90	3510.0
91.00	362.0
92.00	2545.0
93.00	3553.0
94.00	10649.0
95.00	83800.0
96.00	5572.0
97.00	168.0
103.80	478.0
105.00	169.0
105.90	368.0
106.80	167.0
110.80	113.0
111.80	103.0
112.80	120.0
114.80	141.0
115.90	310.0
116.90	633.0
117.90	294.0
118.90	524.0
127.70	285.0
128.70	153.0
129.80	319.0
130.90	163.0
135.00	164.0
136.80	215.0
140.80	929.0
141.80	158.0
142.90	1032.0
143.90	118.0
144.80	308.0
145.90	143.0
147.80	251.0
149.60	125.0
152.90	111.0
155.00	225.0
158.80	164.0
161.00	129.0
171.00	118.0
171.90	895.0
173.00	982.0
173.90	67720.0
174.90	5222.0
175.90	64880.0
176.90	4275.0
178.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	876.0
37.00	4086.0
37.90	3434.0
38.90	1679.0
39.90	236.0
40.80	147.0
42.90	112.0
43.90	765.0
44.90	711.0
45.90	168.0
47.00	1135.0
48.00	569.0
48.90	3281.0
50.00	14597.0
51.00	4622.0
52.00	221.0
52.80	133.0
53.30	105.0
54.90	249.0
55.90	1379.0
57.00	2247.0
58.10	124.0
60.00	836.0
61.00	3806.0
61.90	4009.0
63.00	3154.0
64.00	388.0
65.00	651.0
66.10	131.0
66.80	247.0
68.00	7667.0
69.00	8285.0
69.90	724.0
71.80	512.0
73.00	3648.0
74.00	13283.0
75.00	40040.0
76.00	3529.0
76.90	582.0
77.90	412.0
78.90	2983.0
79.90	1019.0
80.90	3180.0
81.80	820.0
83.00	117.0
85.90	172.0
86.90	3777.0
87.90	3278.0
91.00	341.0
92.00	2389.0
92.90	3213.0
94.00	10126.0
95.00	77328.0
96.00	5288.0
97.00	193.0
103.80	437.0
105.00	172.0
105.90	344.0
106.90	140.0
111.90	125.0
112.70	129.0
114.80	132.0
115.90	309.0
116.90	636.0
117.80	262.0
118.80	438.0
127.80	283.0
128.80	143.0
129.80	292.0
130.90	165.0
134.90	172.0
136.80	176.0
140.90	921.0
141.80	172.0
142.90	1023.0
144.00	104.0
144.80	320.0
145.80	119.0
147.90	231.0
149.60	105.0
155.10	212.0
156.90	116.0
158.80	172.0
161.00	113.0
171.10	145.0
171.90	853.0
173.00	901.0
173.90	65160.0
174.90	4847.0
175.90	62568.0
176.90	3918.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221