


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101818\
Data File : VV008331.D
Acq On : 18 Oct 2018 09:06
Operator : SY/MD
Sample : BFB88
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB88

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 19 05:24:39 2018

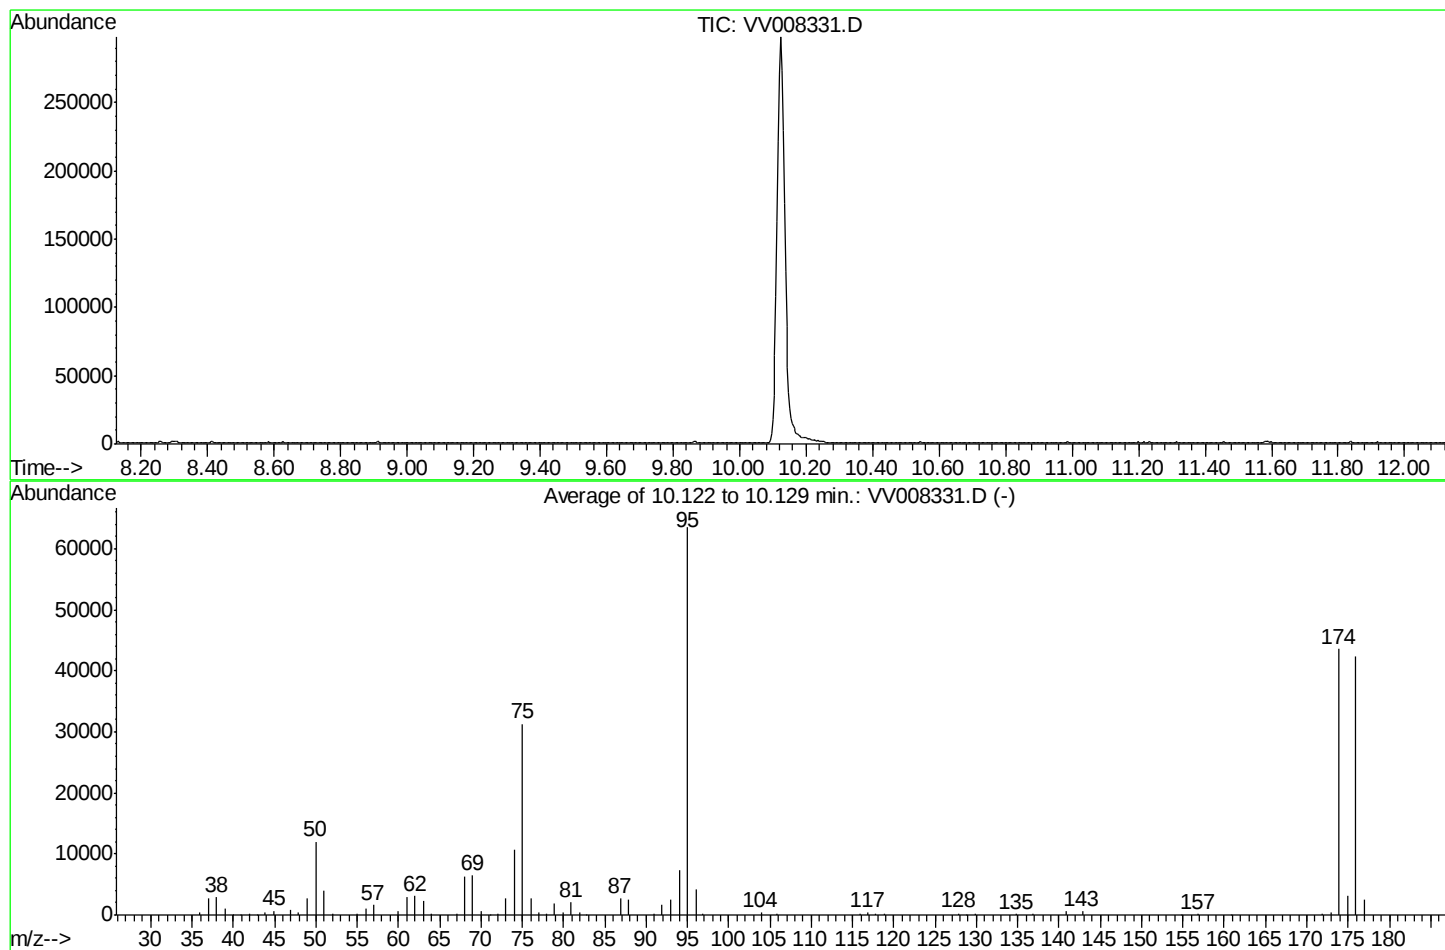

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	11956	PASS
75	95	30	80	49.3	31288	PASS
95	95	100	100	100.0	63496	PASS
96	95	5	9	6.5	4120	PASS
173	174	0.00	2	1.1	476	PASS
174	95	50	120	68.6	43568	PASS
175	174	5	9	7.2	3149	PASS
176	174	95	101	97.2	42349	PASS
177	176	5	9	5.9	2511	PASS

m/z	Abundance
39.90	127.0
41.10	114.0
42.90	119.0
43.90	443.0
55.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
35.90	576.0
37.00	2952.0
38.00	2869.0
39.00	1280.0
39.90	184.0
40.90	190.0
41.90	149.0
43.00	189.0
43.90	778.0
45.00	680.0
47.00	816.0
47.90	360.0
49.00	2627.0
50.00	12518.0
51.00	4088.0
52.00	204.0
55.00	226.0
56.00	1049.0
57.00	1688.0
59.90	628.0
61.00	3203.0
62.00	3080.0
63.00	2606.0
64.00	236.0
67.00	155.0
68.00	6757.0
69.00	6724.0
70.00	671.0
71.10	113.0
72.00	324.0
73.00	2815.0
74.00	10737.0
75.00	32960.0
76.00	2752.0
76.90	422.0
78.00	215.0
78.90	2047.0
79.90	538.0
80.90	2147.0
81.90	473.0
86.90	2817.0
87.90	2656.0
90.90	321.0
91.90	1853.0
93.00	2788.0
94.00	7634.0
95.00	65016.0
96.00	4250.0
96.90	135.0
103.90	345.0
105.90	297.0
115.90	280.0
116.90	312.0
117.80	218.0
118.80	357.0
127.80	234.0
128.80	108.0
129.80	182.0
134.90	137.0
136.80	121.0
140.90	543.0
142.90	531.0
154.80	127.0
156.90	135.0
160.90	104.0
171.90	123.0
172.90	505.0
173.90	43640.0
174.90	3285.0
175.90	42872.0
176.90	2629.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
35.90	467.0
37.00	2895.0
38.00	3025.0
39.00	1170.0
40.00	175.0
40.90	204.0
42.00	159.0
43.10	210.0
43.90	877.0
45.00	707.0
47.00	883.0
47.90	399.0
49.00	2752.0
50.00	12266.0
51.00	4116.0
52.00	153.0
55.00	296.0
56.00	1091.0
57.00	1665.0
59.90	617.0
61.00	3139.0
62.00	3176.0
63.00	2486.0
63.90	236.0
67.00	170.0
68.00	6600.0
69.00	6653.0
70.00	638.0
71.10	107.0
72.00	331.0
73.00	2738.0
74.00	10960.0
75.00	32152.0
76.00	2743.0
76.90	384.0
77.90	267.0
78.90	2023.0
79.90	540.0
80.90	2121.0
81.90	449.0
82.80	108.0
86.90	2744.0
87.90	2601.0
91.00	306.0
91.90	1849.0
93.00	2714.0
94.00	7477.0
95.00	65368.0
96.00	4256.0
96.90	138.0
103.90	340.0
105.90	307.0
115.90	271.0
116.90	325.0
117.80	202.0
118.80	313.0
127.80	235.0
129.80	196.0
134.80	123.0
136.80	120.0
140.90	535.0
142.90	568.0
156.90	138.0
171.90	116.0
172.90	478.0
173.90	44872.0
174.90	3195.0
175.90	43632.0
176.90	2500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
35.90	401.0
37.00	2591.0
38.00	2737.0
39.00	995.0
40.00	165.0
40.90	213.0
42.00	152.0
43.00	205.0
43.90	915.0
44.90	599.0
47.00	877.0
47.90	381.0
49.00	2525.0
50.00	11085.0
51.00	3800.0
52.00	104.0
55.00	318.0
56.00	987.0
57.00	1533.0
59.90	520.0
61.00	2751.0
62.00	2944.0
63.00	2149.0
63.90	218.0
67.00	187.0
68.00	5837.0
69.00	6105.0
70.00	540.0
72.00	304.0
73.00	2459.0
74.00	10258.0
75.00	28752.0
76.00	2564.0
77.00	356.0
77.90	252.0
78.90	1872.0
79.90	477.0
80.90	1887.0
81.90	437.0
86.90	2483.0
87.90	2300.0
90.90	246.0
91.90	1661.0
92.90	2311.0
94.00	6727.0
95.00	60104.0
96.00	3856.0
96.90	137.0
103.90	306.0
105.90	300.0
115.90	217.0
116.80	353.0
117.80	187.0
118.80	234.0
127.90	191.0
129.90	202.0
134.90	114.0
136.80	112.0
140.90	525.0
142.80	549.0
156.90	118.0
171.80	112.0
172.90	447.0
173.90	42192.0
174.90	2967.0
175.90	40544.0
176.90	2404.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88