

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101819\
Quantitation Report (QT Reviewed)


Data File : VV013209.D
Acq On : 18 Oct 2019 18:23
Operator : SY/MD
Sample : K5321-11MS
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 01 02:54:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
E0AA6MS

Manual Integrations
APPROVED

MMDadoda
11/1/2019 8:08:04 AM

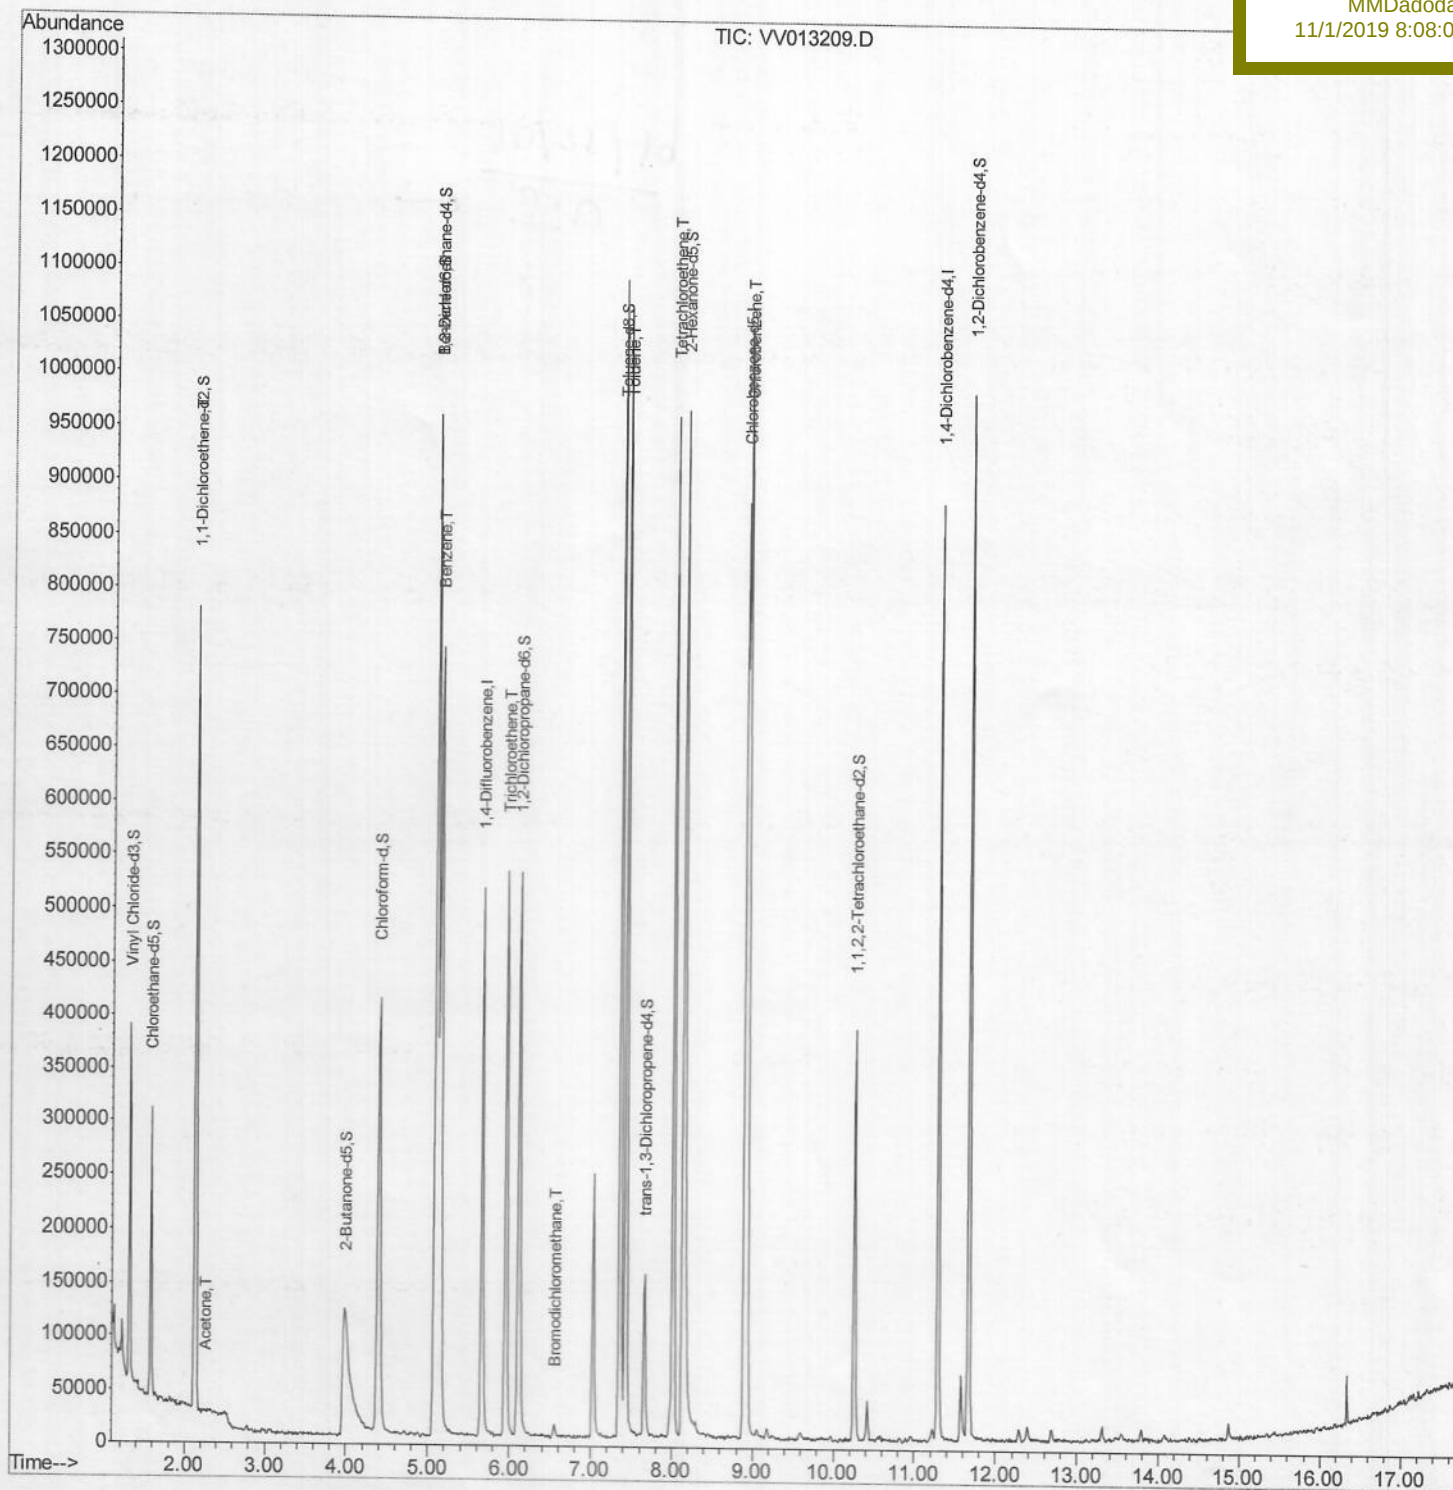

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101819\
Quantitation Report (Qedit)




Data File : VV013209.D
Acq On : 18 Oct 2019 18:23
Operator : SY/MD
Sample : K5321-11MS
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 01 02:50:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
E0AA6MS

Manual Integrations
APPROVED

MMDadoda
11/1/2019 8:08:04 AM

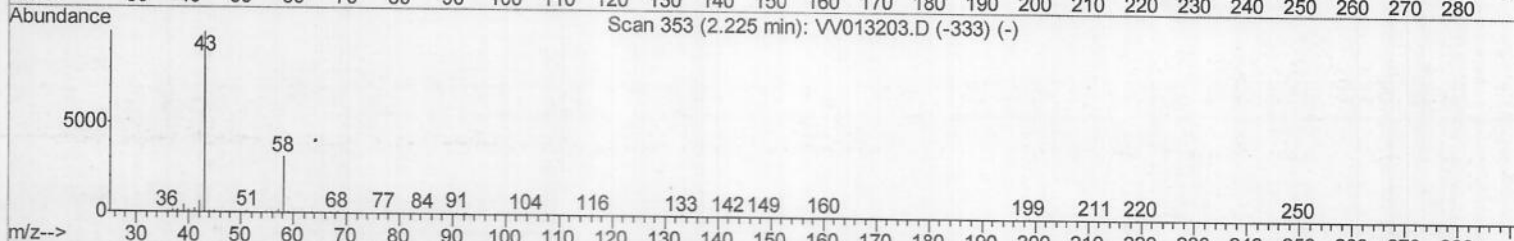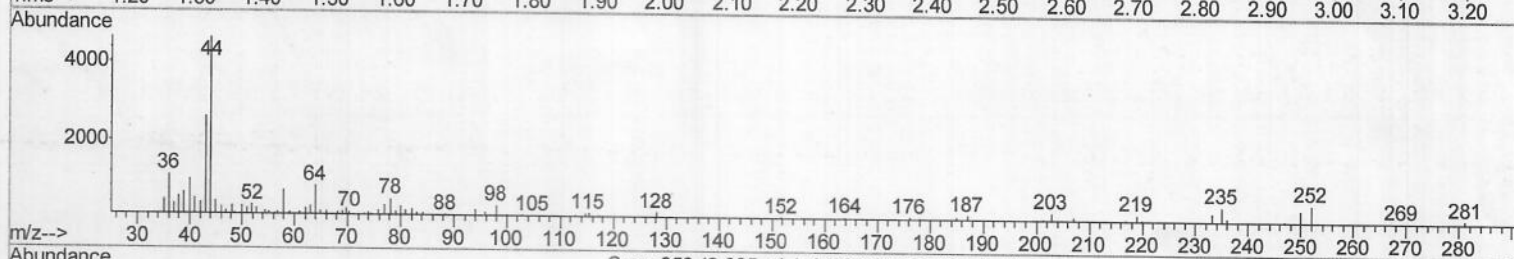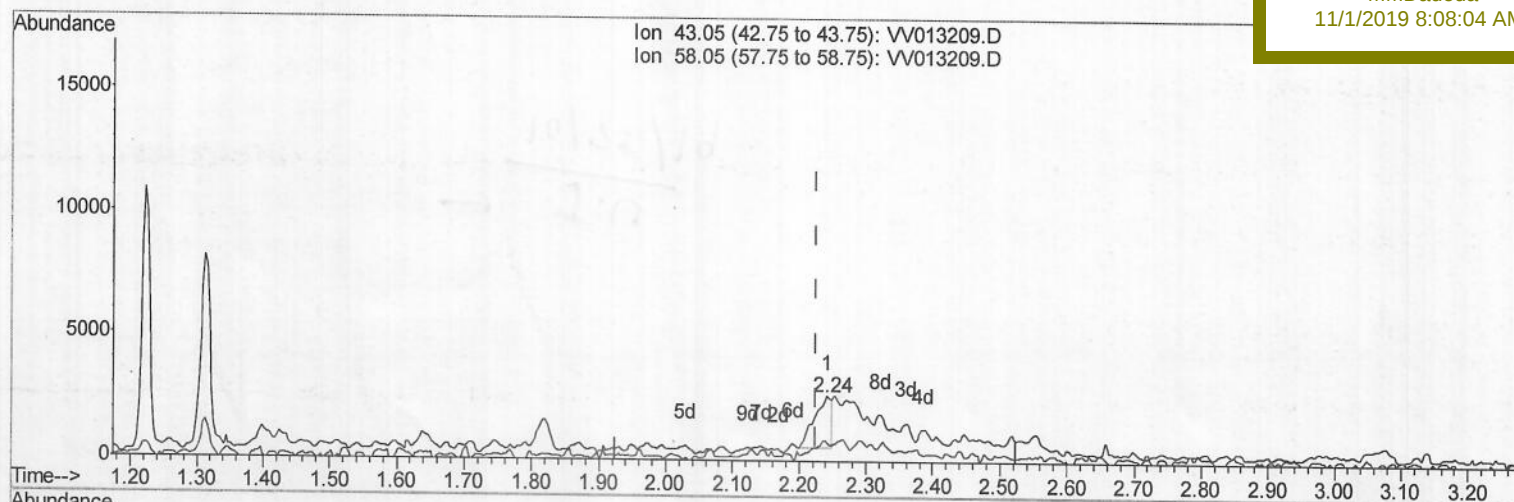

TIC: VV013209.D

(13) Acetone (T)

2.241min (+0.016) 0.79ug/L

response 3666

Ion	Exp%	Act%
43.05	100	100
58.05	26.20	21.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101819\
Quantitation Report (Qedit)




Data File : VV013209.D
Acq On : 18 Oct 2019 18:23
Operator : SY/MD
Sample : K5321-11MS
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 01 02:50:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
E0AA6MS

Manual Integrations
APPROVED

MMDadoda
11/1/2019 8:08:04 AM

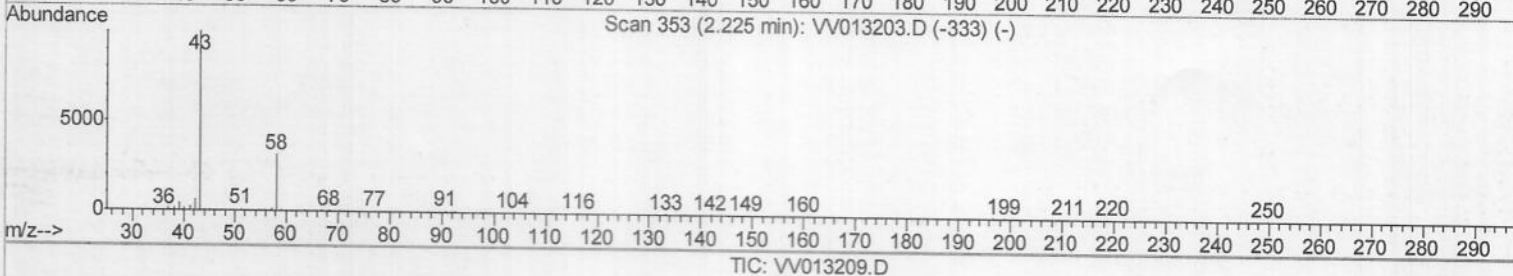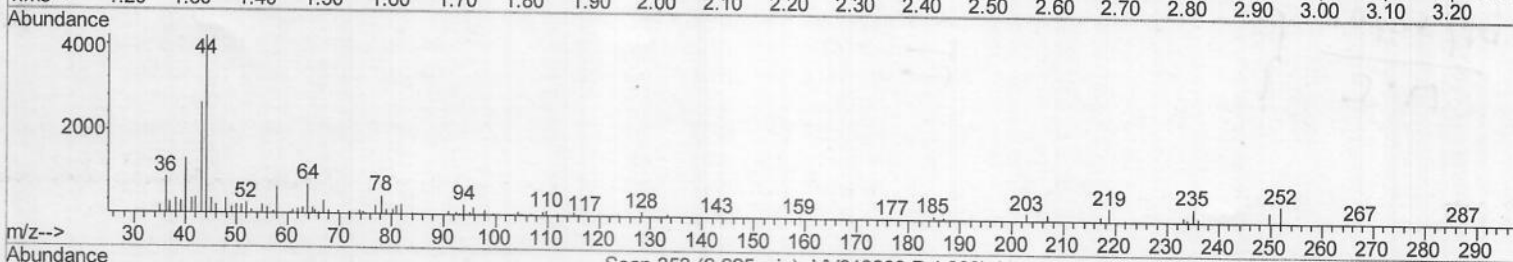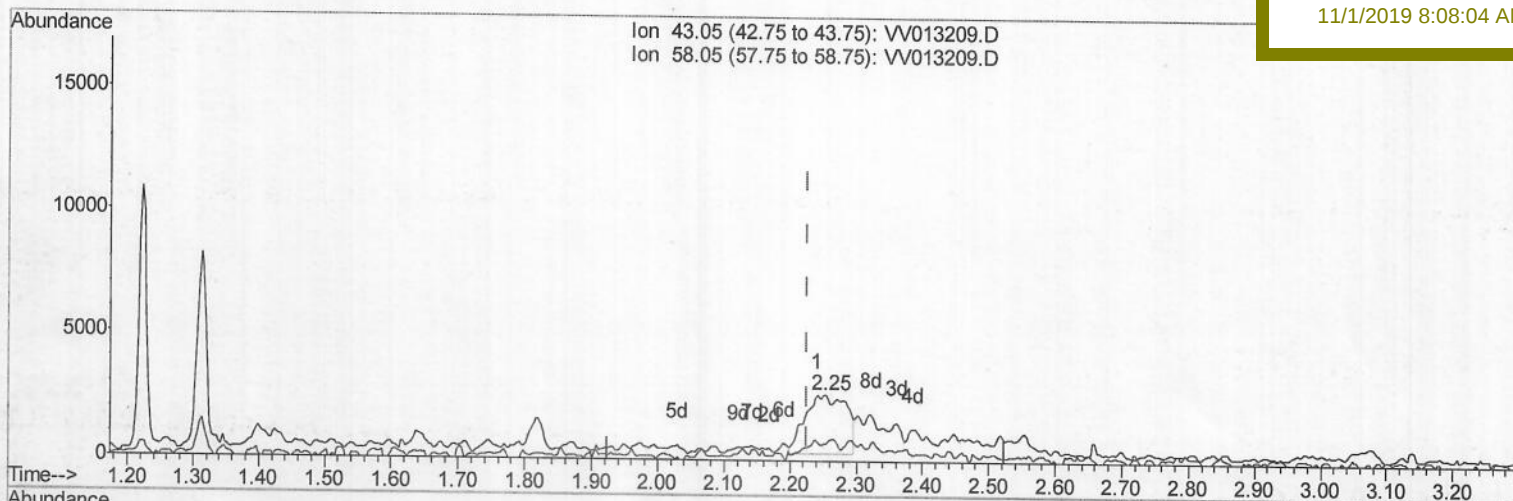

(13) Acetone (T)

2.254min (+0.029) 2.19ug/L m

M.D 10/21/19

response 10138

Ion	Exp%	Act%
43.05	100	100
58.05	26.20	7.72
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV013209.D
Acq On : 18 Oct 2019 18:23
Operator : SY/MD
Sample : K5321-11MS
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6MS

Manual Integrations
APPROVED

MMDadoda
11/1/2019 8:08:04 AM

Quant Time: Nov 01 02:54:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	447586	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	475477	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	233997	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	210550	4.58	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	91.60%		
7) Chloroethane-d5	1.58	69	174015	4.79	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	95.80%		
11) 1,1-Dichloroethene-d2	2.13	63	311339	4.38	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	87.60%		
20) 2-Butanone-d5	3.98	46	444264	46.98	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	93.96%		
24) Chloroform-d	4.40	84	409843	4.65	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.00%		
26) 1,2-Dichloroethane-d4	5.08	65	202702	4.85	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.00%		
32) Benzene-d6	5.09	84	851048	4.69	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.80%		
36) 1,2-Dichloropropane-d6	6.11	67	262679	4.85	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.00%		
41) Toluene-d8	7.36	98	714074	4.42	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	88.40%		
43) trans-1,3-Dichloropropene-	7.66	79	90717	4.70	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	94.00%		
46) 2-Hexanone-d5	8.14	63	355335	45.81	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	91.62%		
57) 1,1,2,2-Tetrachloroethane-	10.26	84	179444	4.64	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	92.80%		
64) 1,2-Dichlorobenzene-d4	11.67	152	265711	5.36	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	107.20%		

Target Compounds

					Qvalue
12) 1,1-Dichloroethene	2.14	96	126291	3.513 ug/L #	83
13) Acetone	2.25	43	10138m	2.189 ug/L	
33) Benzene	5.14	78	731771	3.822 ug/L	100
34) Trichloroethene	5.96	95	182597	3.677 ug/L	99
38) Bromodichloromethane	6.56	83	7894	0.132 ug/L #	95
42) Toluene	7.43	91	762737	3.875 ug/L	99
47) Tetrachloroethene	8.02	164	229491	5.285 ug/L	96
51) Chlorobenzene	8.92	112	532748	4.210 ug/L	99

M.D 10/21/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed