

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
 Data File : VV013215.D
 Acq On : 18 Oct 2019 20:48
 Operator : SY/MD
 Sample : K5404-01
 Misc : 25.00ML/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA5

Quant Time: Nov 01 03:58:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 01 02:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	399940	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	432773	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	221296	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	220009	5.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.00%
7) Chloroethane-d5	1.58	69	179688	5.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.80%
11) 1,1-Dichloroethene-d2	2.13	63	251061	3.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.00%
20) 2-Butanone-d5	3.97	46	474627	56.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.34%
24) Chloroform-d	4.40	84	408455	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.08	65	197537	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.80%
32) Benzene-d6	5.10	84	828933	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	252024	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.40%
41) Toluene-d8	7.36	98	661400	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.66	79	82729	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.14	63	330522	46.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.62%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	173395	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	272120	5.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.00%


Target Compounds					Qvalue
13) Acetone	2.25	43	30953	7.481 ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
Data File : VV013215.D
Acq On : 18 Oct 2019 20:48
Operator : SY/MD
Sample : K5404-01
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA5

Quant Time: Nov 01 03:58:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

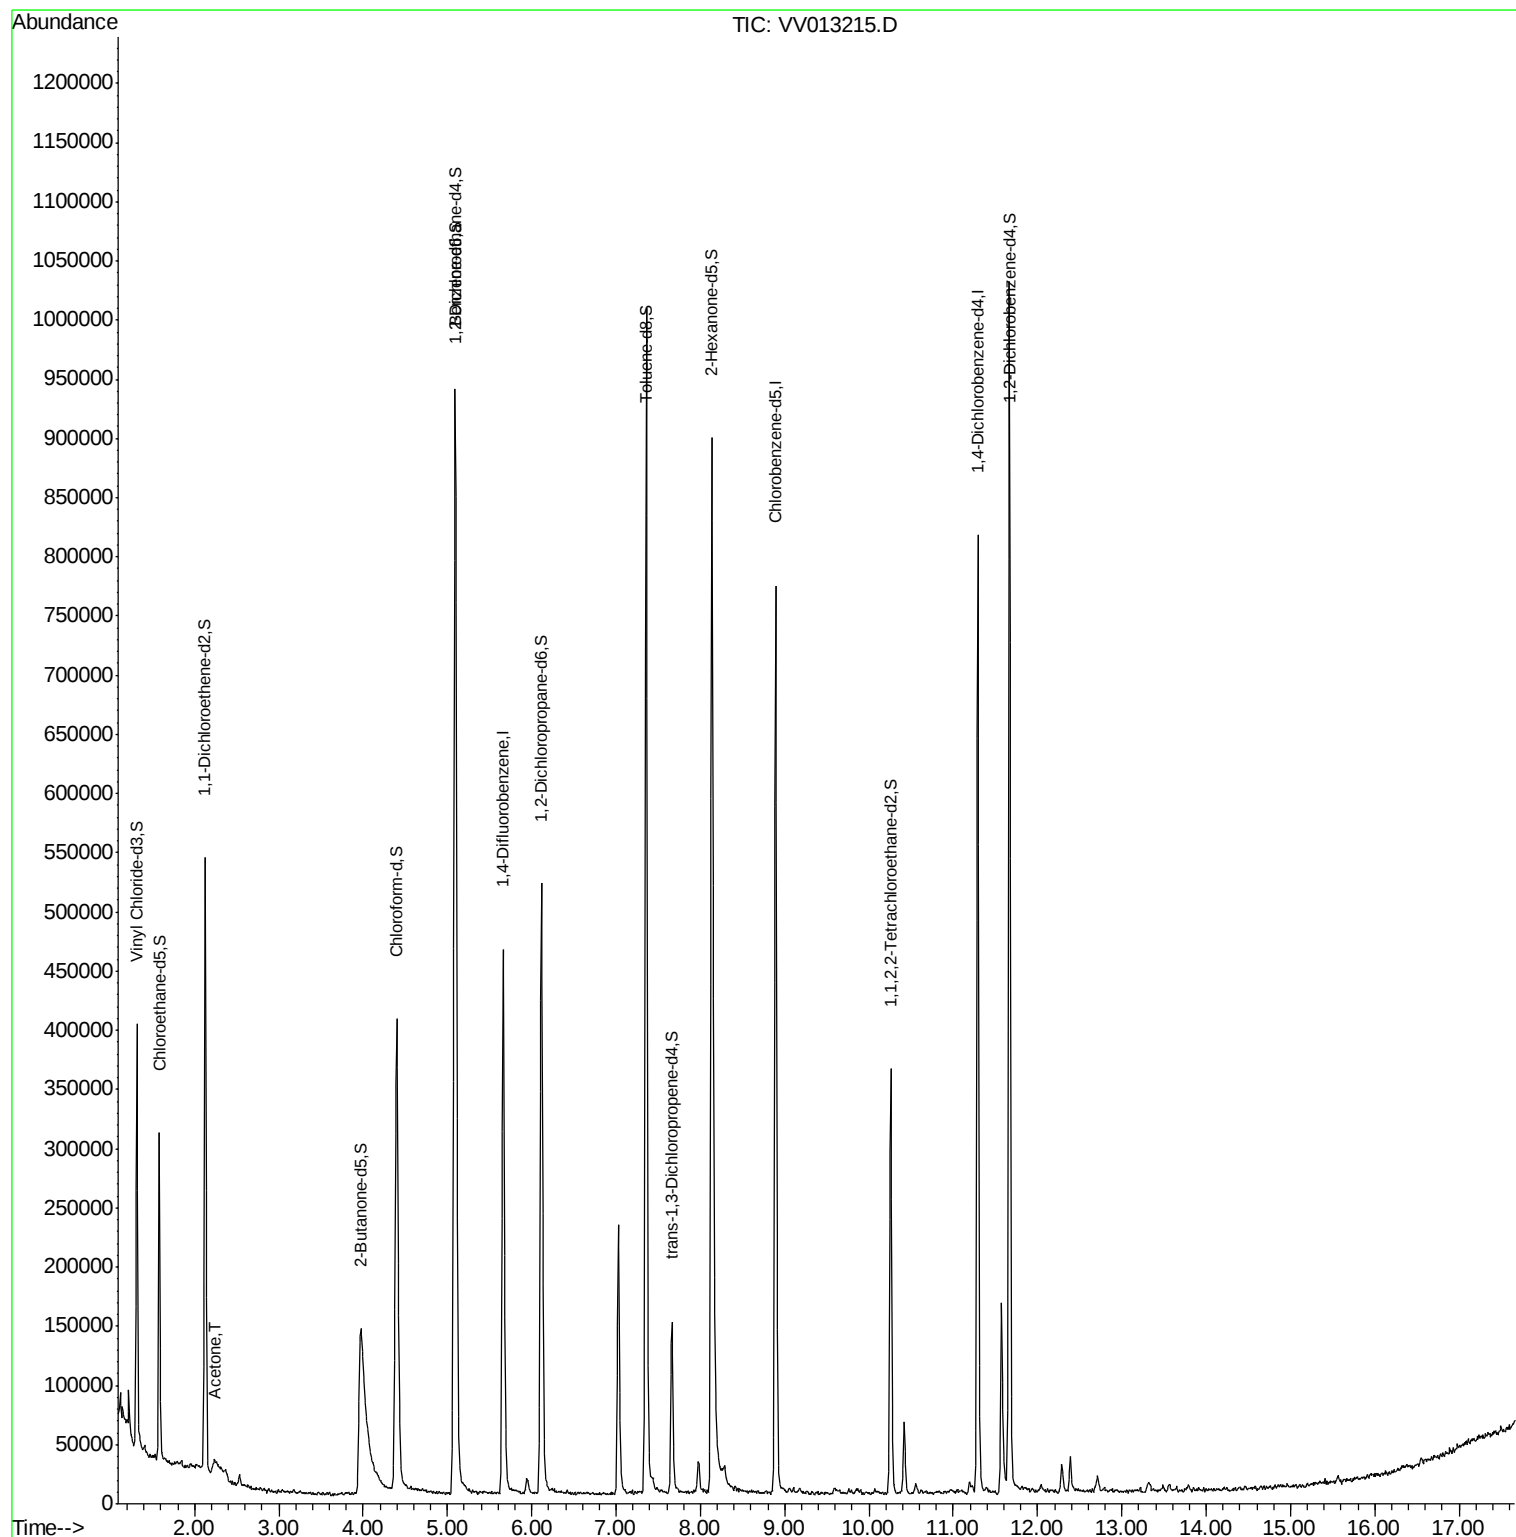

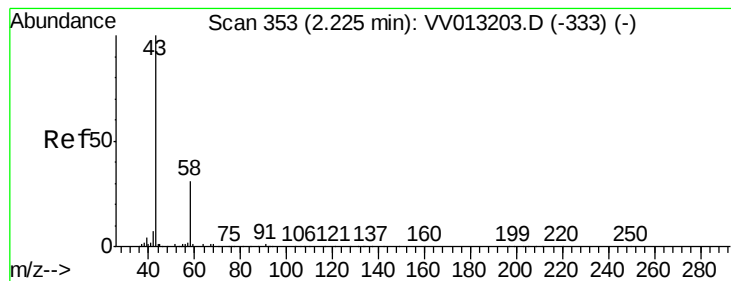

#13

Acetone

Concen: 7.481 ug/L

RT: 2.25 min Scan# 360

Delta R.T. 0.02 min

Lab File: VV013215.D

Acq: 18 Oct 2019 20:48

Instrument :
MSVOA_V
ClientSampleId :
C0AA5

Tgt Ion: 43 Resp: 30953

Ion Ratio Lower Upper

43 100

58 11.7 0.0 52.4

