

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
 Data File : VV013216.D
 Acq On : 18 Oct 2019 21:12
 Operator : SY/MD
 Sample : K5404-07
 Misc : 25.00ML/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB7

Quant Time: Nov 01 04:00:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 01 02:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	426979	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	455109	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	231639	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	234066	5.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.60%
7) Chloroethane-d5	1.58	69	189588	5.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.40%
11) 1,1-Dichloroethene-d2	2.13	63	283921	4.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.60%
20) 2-Butanone-d5	3.96	46	480011	53.21	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.42%
24) Chloroform-d	4.40	84	456008	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.08	65	216905	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.80%
32) Benzene-d6	5.09	84	916050	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
36) 1,2-Dichloropropane-d6	6.12	67	280105	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.36	98	740723	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
43) trans-1,3-Dichloropropene-	7.66	79	90453	4.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.00%
46) 2-Hexanone-d5	8.13	63	361138	48.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.28%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	190401	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	293485	5.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.60%


Target Compounds					Qvalue
13) Acetone	2.22	43	43858	9.928 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
Data File : VV013216.D
Acq On : 18 Oct 2019 21:12
Operator : SY/MD
Sample : K5404-07
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Quant Time: Nov 01 04:00:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

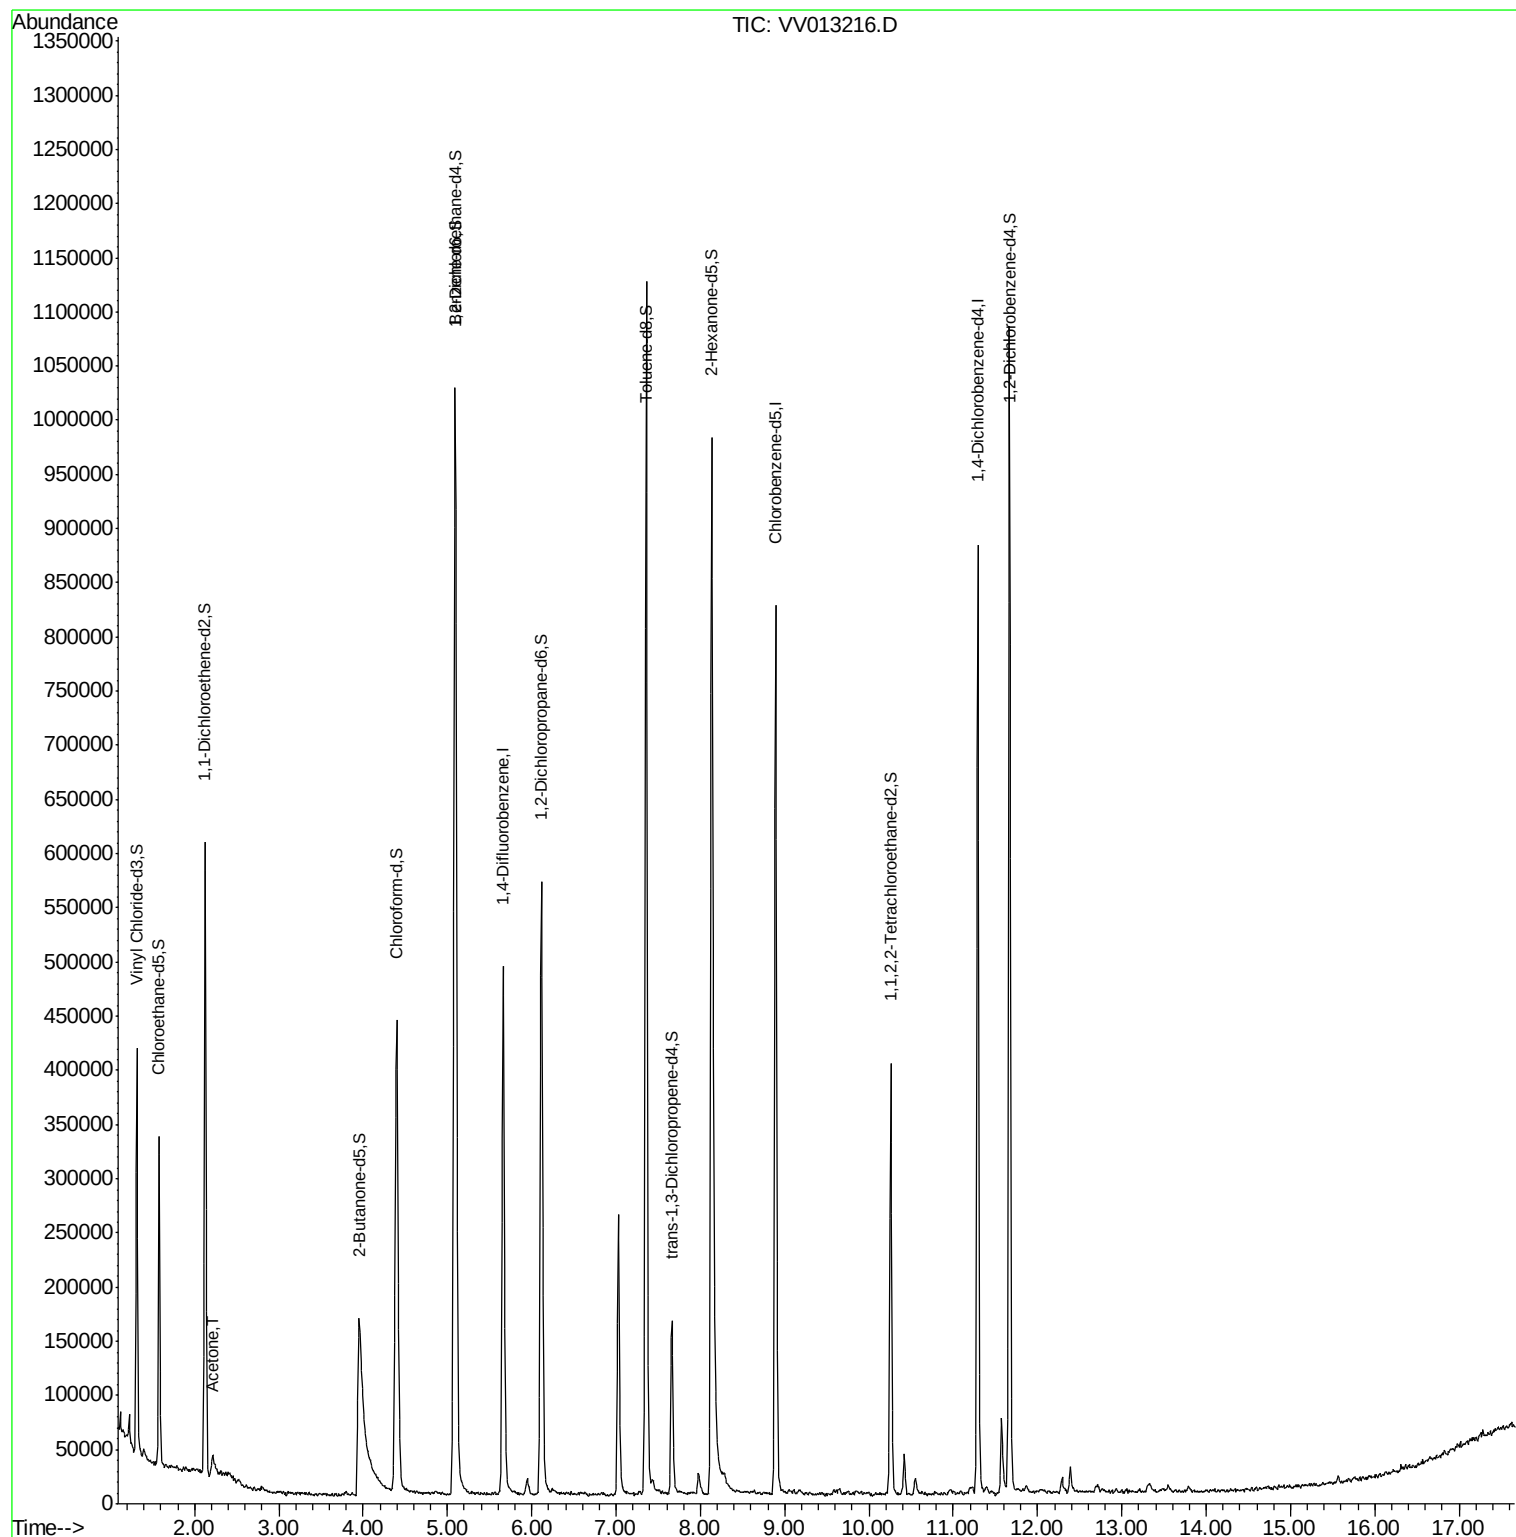

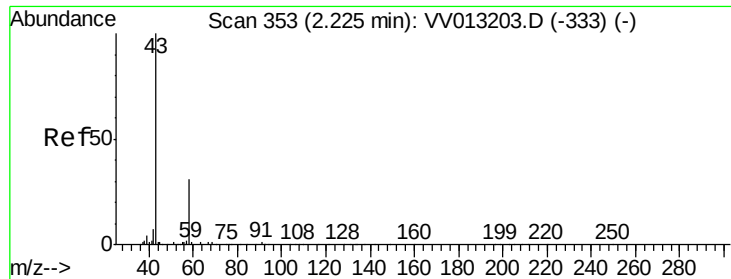

#13

Acetone

Concen: 9.928 ug/L

RT: 2.22 min Scan# 350

Delta R.T. -0.01 min

Lab File: VV013216.D

Acq: 18 Oct 2019 21:12

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Tgt Ion: 43 Resp: 43858

Ion Ratio Lower Upper

43 100

58 24.3 0.0 52.4

