

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
 Data File : VV013229.D
 Acq On : 19 Oct 2019 03:15
 Operator : SY/MD
 Sample : K5457-13
 Misc : 25.00ML/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0K18

Quant Time: Nov 01 04:29:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 01 02:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	415779	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	457168	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	234125	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	208141	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.58	69	165826	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	247119	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.97	46	527649	60.06	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.12%
24) Chloroform-d	4.40	84	401799	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
26) 1,2-Dichloroethane-d4	5.08	65	205576	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.09	84	827501	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.12	67	251328	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.36	98	660290	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.00%
43) trans-1,3-Dichloropropene-	7.66	79	84205	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.14	63	363554	48.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.48%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	189184	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	260081	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Qvalue
3) Chloromethane	1.25	50	6402	0.128 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101819\
Data File : VV013229.D
Acq On : 19 Oct 2019 03:15
Operator : SY/MD
Sample : K5457-13
Misc : 25.00ML/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0K18

Quant Time: Nov 01 04:29:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 02:14:39 2019
Response via : Initial Calibration

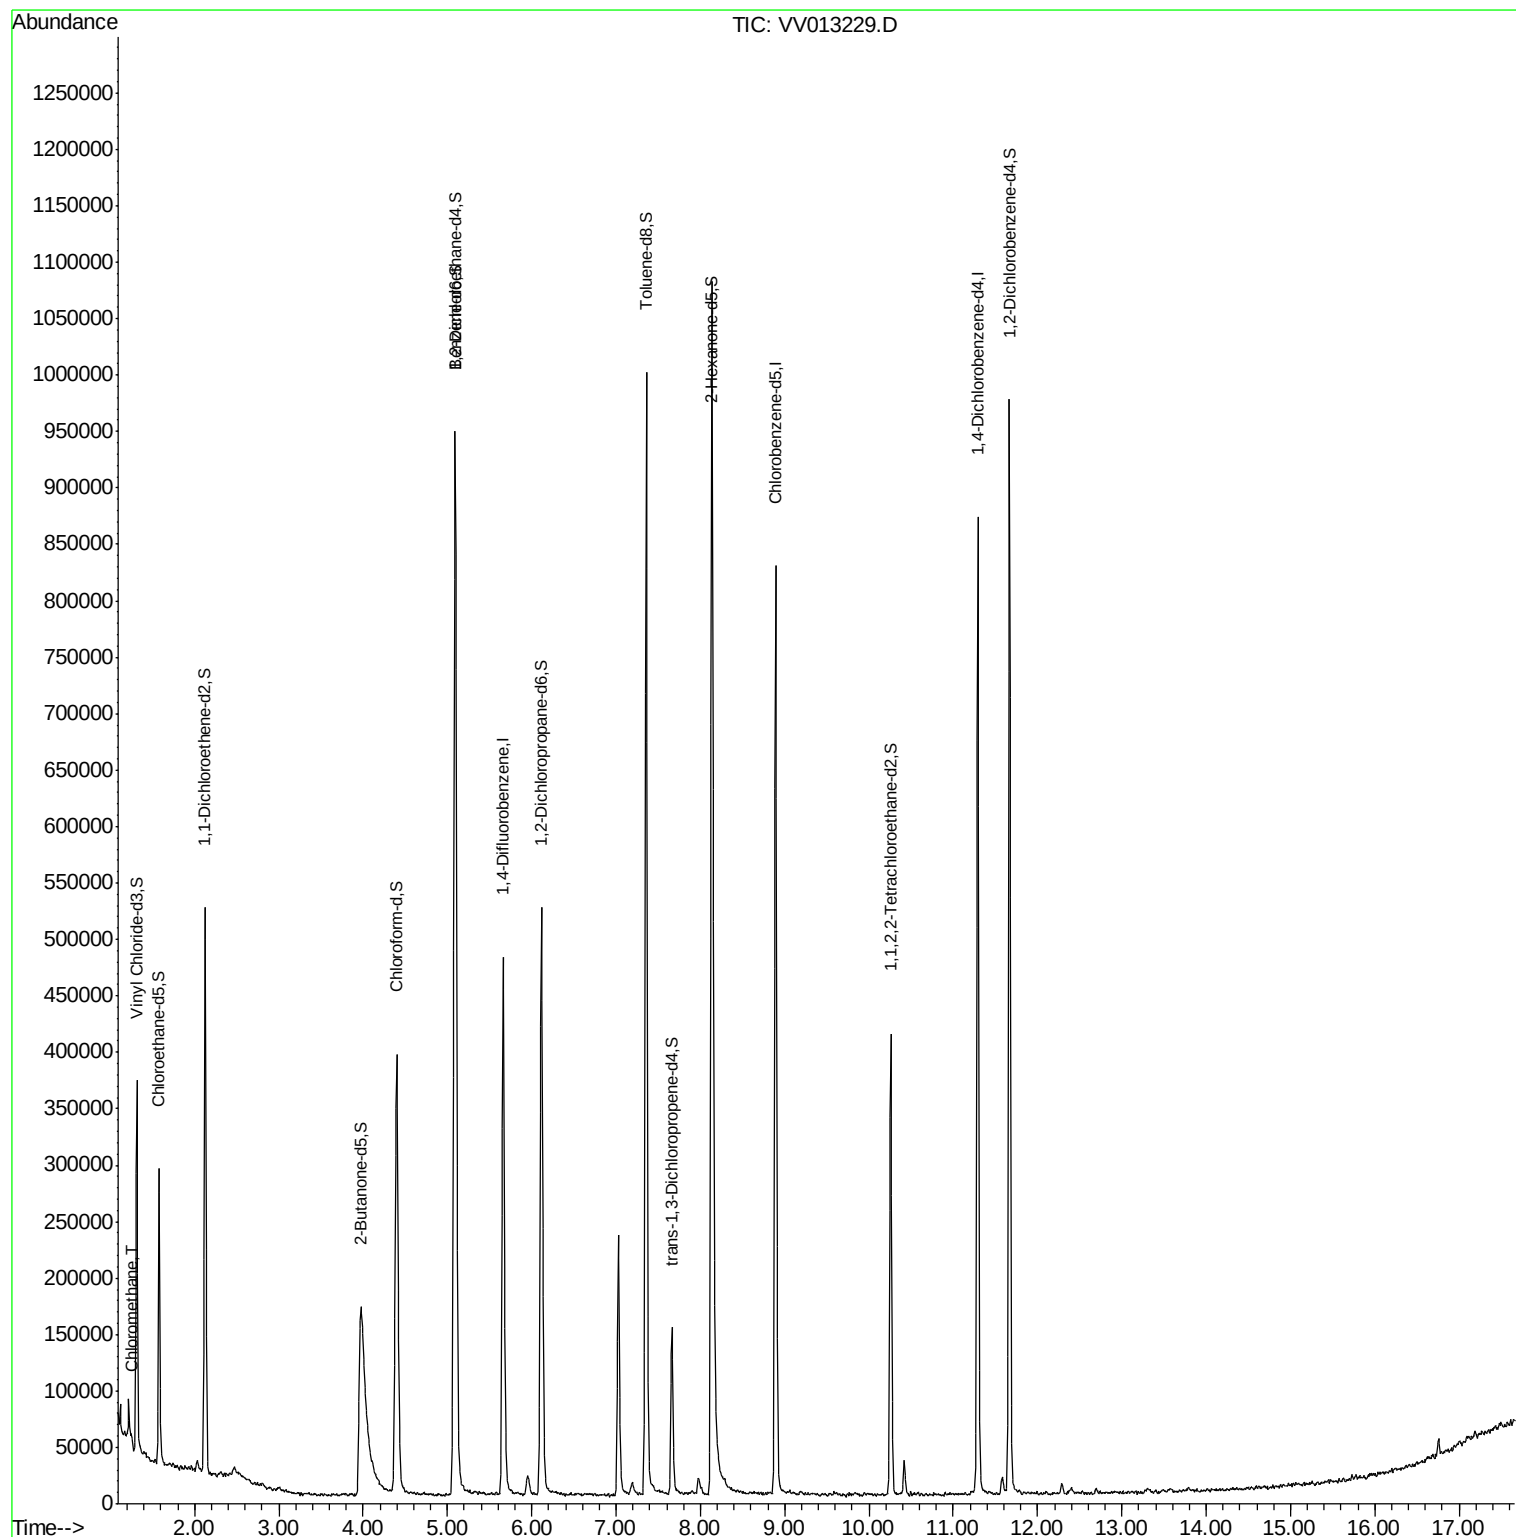

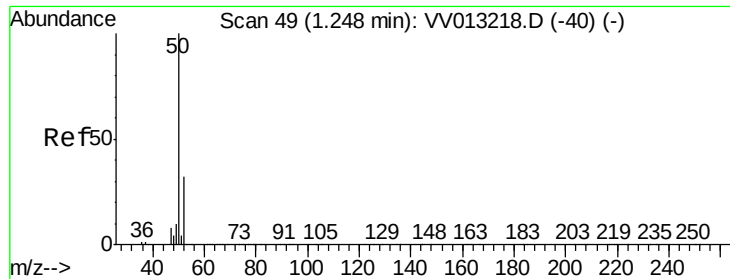

#3
 Chloromethane
 Concen: 0.128 ug/L
 RT: 1.25 min Scan# 50
 Delta R.T. 0.00 min
 Lab File: VV013229.D
 Acq: 19 Oct 2019 03:15

Instrument :
 MSVOA_V
 ClientSampleId :
 C0K18

Tgt Ion: 50 Resp: 6402
 Ion Ratio Lower Upper
 50 100
 52 40.7 23.0 42.8

