


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101819\
 Data File : VV013196.D
 Acq On : 18 Oct 2019 08:24
 Operator : SY/MD
 Sample : BFB44
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Oct 21 01:27:38 2019

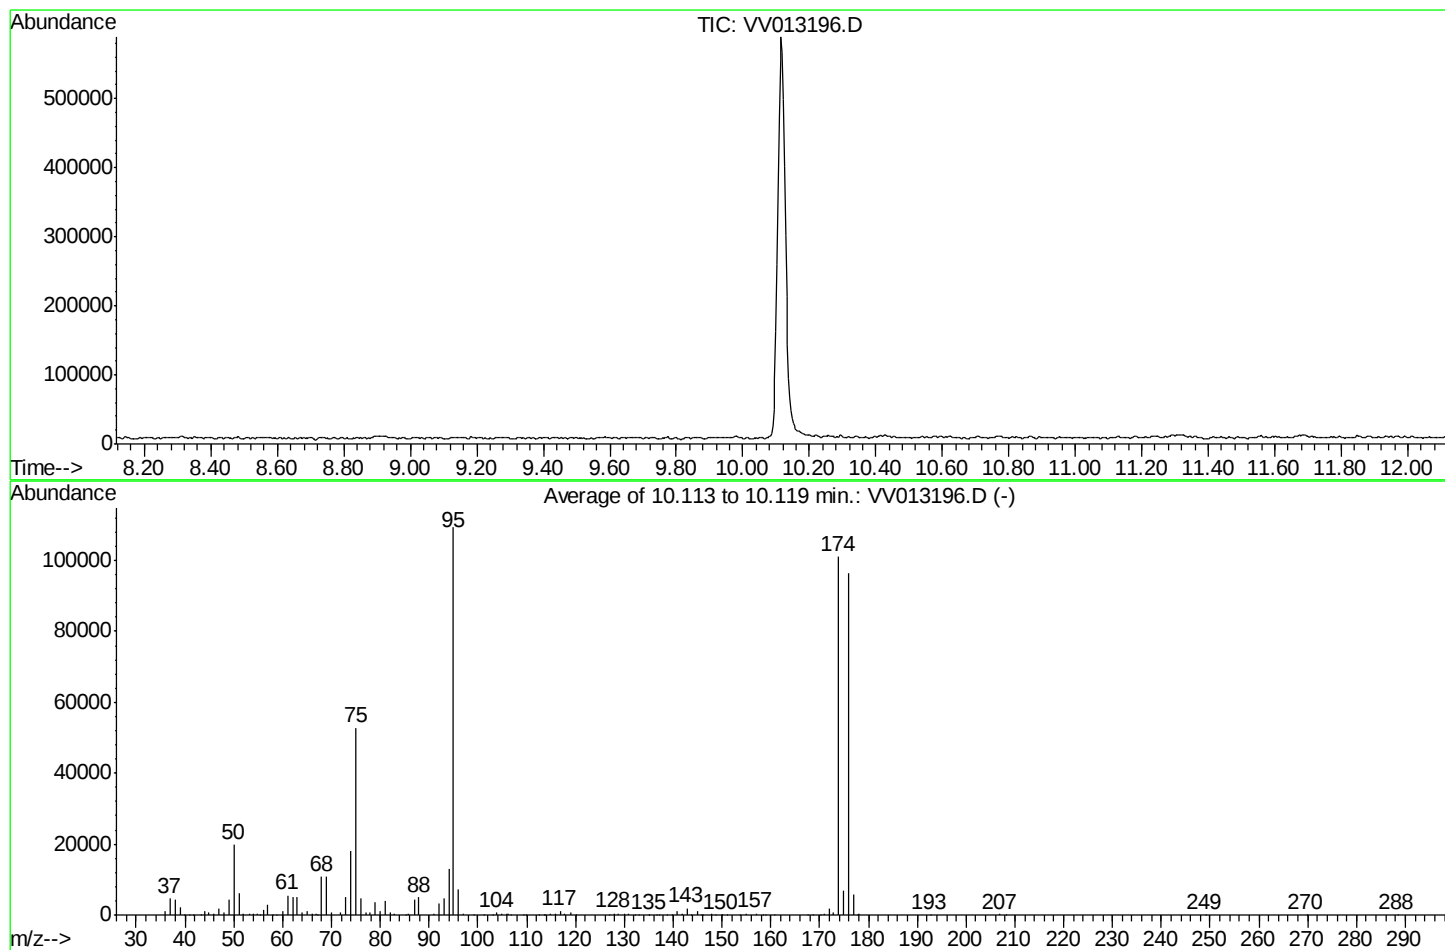

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	19723	PASS
75	95	30	80	48.4	52896	PASS
95	95	100	100	100.0	109362	PASS
96	95	5	9	6.6	7263	PASS
173	174	0.00	2	0.9	914	PASS
174	95	50	120	92.4	101061	PASS
175	174	5	9	7.0	7034	PASS
176	174	95	101	95.4	96461	PASS
177	176	5	9	6.1	5888	PASS

m/z	Abundance
35.90	1042.0
37.00	4933.0
38.10	4386.0
39.00	2253.0
40.00	1886.0
41.10	240.0
41.80	152.0
43.00	111.0
44.00	2239.0
45.00	812.0
46.00	294.0
47.00	1869.0
47.90	726.0
49.00	4264.0
50.00	19576.0
51.00	6429.0
52.00	475.0
53.10	328.0
54.00	223.0
54.70	210.0
55.20	196.0
56.10	1573.0
57.00	2824.0
58.10	152.0
58.80	129.0
60.00	1378.0
61.00	5422.0
62.00	5081.0
63.00	4877.0
64.10	934.0
65.00	1279.0
66.10	357.0
66.70	301.0
68.00	10807.0
69.00	11242.0
70.00	700.0
72.00	628.0
73.00	4526.0
74.00	17640.0
75.00	52336.0
76.00	4676.0
77.10	686.0
78.00	803.0
78.90	3668.0
79.90	1188.0
80.90	3773.0
82.00	896.0
82.90	255.0
85.80	483.0
87.00	3925.0
88.00	4499.0
90.10	150.0
91.00	337.0
92.00	3111.0
93.00	5086.0
94.00	12172.0
95.00	107576.0
96.00	7307.0
97.00	278.0
103.10	151.0
103.90	672.0
104.90	253.0
106.10	386.0
106.70	190.0
109.20	101.0
109.80	174.0
112.70	141.0
113.50	112.0
113.80	134.0
114.80	199.0
115.90	411.0
116.90	1183.0
117.80	454.0
118.90	884.0
120.00	106.0
126.90	111.0
127.90	509.0
128.80	360.0
130.00	342.0
130.80	195.0
132.90	110.0
134.90	267.0
137.10	128.0
140.80	1110.0
141.90	295.0
142.90	1957.0
143.80	103.0
144.90	935.0
146.00	154.0
147.90	345.0
148.70	142.0
149.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

150.10	172.0
153.70	109.0
155.00	417.0
157.00	381.0
158.30	105.0
158.90	109.0
167.50	108.0
168.60	164.0
170.90	341.0
172.00	1780.0
172.90	1370.0
173.90	95840.0
174.90	7154.0
175.90	92432.0
176.90	5680.0
178.10	284.0
207.00	176.0
249.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	1125.0
37.00	4947.0
38.10	4814.0
39.00	2312.0
40.10	1834.0
41.00	260.0
41.80	182.0
43.00	123.0
43.30	131.0
44.00	2250.0
45.00	859.0
46.00	358.0
47.00	1807.0
47.90	965.0
49.00	4400.0
50.00	20496.0
51.00	6649.0
52.00	509.0
53.20	367.0
54.00	208.0
54.80	313.0
56.10	1524.0
57.00	2955.0
58.10	173.0
58.80	184.0
59.90	1347.0
61.00	5778.0
62.00	5304.0
63.00	5072.0
64.00	886.0
65.10	1240.0
66.10	358.0
66.70	332.0
67.20	265.0
68.00	11045.0
69.00	11426.0
70.10	745.0
72.00	659.0
73.00	5101.0
74.00	18896.0
75.00	54864.0
76.00	4783.0
77.20	706.0
78.00	913.0
78.90	3819.0
79.90	1268.0
80.90	3986.0
82.00	915.0
82.90	296.0
85.80	453.0
87.00	4458.0
87.90	5300.0
90.10	140.0
91.10	413.0
92.00	3381.0
93.00	5283.0
94.00	13329.0
95.00	112808.0
96.00	7522.0
96.90	282.0
101.20	105.0
103.10	147.0
103.90	649.0
104.90	260.0
105.80	395.0
106.10	405.0
106.70	174.0
112.50	142.0
113.40	128.0
114.90	232.0
115.80	486.0
116.90	1194.0
117.80	495.0
118.90	924.0
120.00	130.0
127.90	540.0
128.90	299.0
130.00	477.0
130.80	193.0
132.20	103.0
134.90	187.0
136.70	134.0
137.10	200.0
138.60	105.0
139.70	154.0
140.80	1064.0
141.90	335.0
142.90	2043.0
144.90	1051.0
146.00	200.0
147.80	363.0
149.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

150.10	162.0
150.90	114.0
153.70	138.0
155.00	380.0
157.00	448.0
158.20	101.0
168.60	115.0
170.30	183.0
170.90	365.0
172.00	1891.0
172.90	1374.0
173.90	104264.0
174.90	7092.0
175.90	99584.0
176.90	5908.0
178.10	248.0
206.90	215.0
208.10	112.0
249.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.10	160.0
36.00	1043.0
37.00	4443.0
38.00	4497.0
39.00	2130.0
40.10	1704.0
40.90	239.0
41.80	157.0
43.00	141.0
44.00	2142.0
45.00	792.0
45.90	431.0
47.00	1527.0
48.00	1114.0
49.00	4194.0
50.00	19536.0
51.00	6031.0
52.00	537.0
53.20	347.0
54.00	158.0
54.80	398.0
56.10	1392.0
57.00	2811.0
58.10	225.0
58.80	217.0
59.90	1237.0
61.00	5378.0
62.00	5088.0
63.00	4946.0
64.00	788.0
65.10	1291.0
66.10	343.0
66.80	345.0
68.00	10634.0
69.00	10399.0
70.10	710.0
71.90	743.0
73.00	5121.0
74.00	18376.0
75.00	51856.0
76.00	4453.0
77.10	682.0
78.00	879.0
78.90	3569.0
79.90	1209.0
80.90	3968.0
82.00	887.0
82.80	251.0
85.10	107.0
85.80	348.0
87.00	4788.0
87.90	5367.0
91.10	444.0
92.00	3240.0
93.00	4624.0
94.00	13344.0
95.00	107704.0
96.00	6962.0
96.90	272.0
99.00	104.0
101.20	111.0
103.10	117.0
103.90	500.0
104.80	208.0
105.80	481.0
112.50	120.0
114.90	236.0
115.80	481.0
116.90	1128.0
117.80	504.0
118.90	824.0
120.00	107.0
127.90	498.0
128.90	182.0
130.10	502.0
130.90	227.0
132.10	107.0
135.10	178.0
136.60	180.0
137.10	227.0
138.60	116.0
139.70	165.0
140.80	962.0
142.00	259.0
142.90	1909.0
144.90	978.0
145.70	275.0
147.70	347.0
150.10	180.0
150.90	105.0
153.70	137.0
155.00	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

157.00	381.0
158.80	119.0
160.60	107.0
170.20	227.0
170.90	377.0
171.90	1881.0
173.90	103080.0
174.90	6856.0
175.90	97368.0
176.90	6077.0
177.80	216.0
178.00	215.0
192.70	111.0
206.90	241.0
208.10	128.0
269.80	109.0
288.40	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.30	148.0
36.20	241.0
36.90	151.0
38.00	353.0
39.90	1631.0
40.90	175.0
41.80	127.0
42.30	104.0
42.90	272.0
44.00	1233.0
44.90	139.0
46.40	118.0
47.50	167.0
48.10	128.0
48.50	130.0
49.30	147.0
49.90	146.0
51.00	210.0
53.60	194.0
56.10	155.0
57.90	119.0
60.00	176.0
61.50	149.0
63.80	149.0
65.70	128.0
73.80	100.0
75.00	122.0
77.30	102.0
77.90	121.0
78.10	110.0
79.70	107.0
83.60	158.0
85.90	105.0
90.00	116.0
93.00	110.0
93.70	136.0
100.40	119.0
100.80	102.0
114.10	119.0
118.40	115.0
135.00	128.0
146.00	107.0
152.10	125.0
171.50	111.0
206.70	131.0
207.50	128.0
255.40	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44