
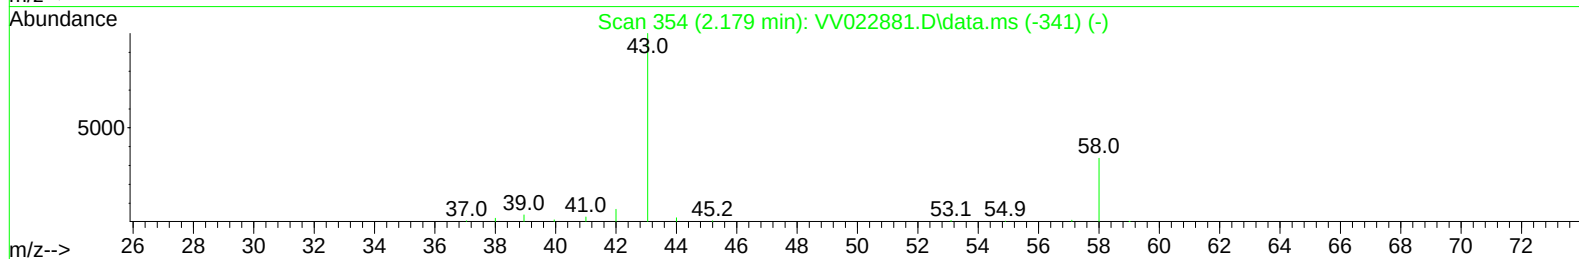
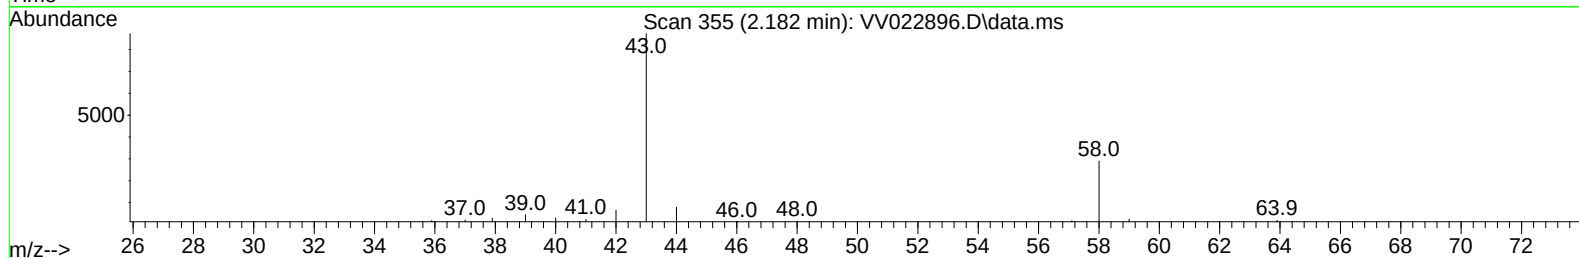


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022896.D
 Acq On : 19 Oct 2021 03:29
 Operator : SY/MD
 Sample : M4137-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Quant Time: Oct 19 04:09:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 04:07:06 2021
 Response via : Initial Calibration

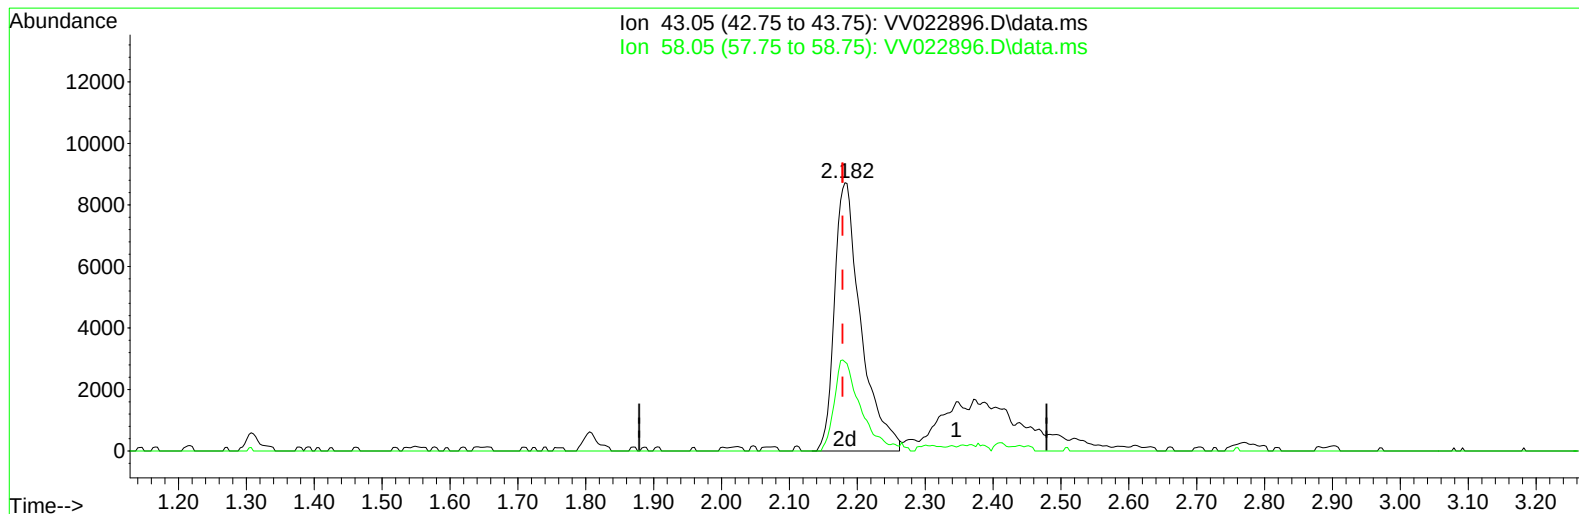

TIC: VV022896.D\data.ms

(13) Acetone (T)**2.182min (+ 0.003) 19.01 ug/L m****response 23533**

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	1.36
0.00	0.00	0.00
0.00	0.00	0.00