

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VW022873.D
 Acq On : 18 Oct 2021 17:51
 Operator : SY/MD
 Sample : M4246-06MSD
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53MSD

Quant Time: Oct 19 01:45:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124831	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126369	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71667	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35838	4.173	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.400%
7) Chloroethane-d5	1.568	69	33535	4.345	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%
11) 1,1-Dichloroethene-d2	2.108	63	64126	3.806	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.200%
20) 2-Butanone-d5	3.886	46	102812	45.655	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.300%
24) Chloroform-d	4.349	84	93537	5.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.600%
26) 1,2-Dichloroethane-d4	5.037	65	41417	4.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%
32) Benzene-d6	5.053	84	179818	4.780	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.072	67	56204	5.045	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.317	98	167318	5.145	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
43) trans-1,3-Dichloroprop...	7.625	79	18429	4.987	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.800%
46) 2-Hexanone-d5	8.088	63	85577	57.459	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.920%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40719	5.395	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	64324	4.841	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.127	85	45590	5.011	ug/L	98
3) Chloromethane	1.240	50	48471	5.301	ug/L	100
5) Vinyl chloride	1.310	62	49496	5.239	ug/L	98
6) Bromomethane	1.519	94	25572	4.342	ug/L	98
8) Chloroethane	1.584	64	26479	4.530	ug/L	97
9) Trichlorofluoromethane	1.751	101	68229	4.930	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.117	101	36999	4.596	ug/L	94
12) 1,1-Dichloroethene	2.117	96	34514	4.577	ug/L	83
13) Acetone	2.175	43	46358	36.917	ug/L	# 45
14) Carbon disulfide	2.294	76	96778	4.567	ug/L	99
15) Methyl Acetate	2.436	43	11667	3.247	ug/L	100
16) Methylene chloride	2.507	84	38158	3.676	ug/L	92
17) Methyl tert-butyl Ether	2.767	73	80764	4.426	ug/L	97
18) trans-1,2-Dichloroethene	2.764	96	43199	5.268	ug/L	95
19) 1,1-Dichloroethane	3.191	63	78842	5.338	ug/L	98
21) 2-Butanone	3.973	43	82817	40.279	ug/L	96
22) cis-1,2-Dichloroethene	3.912	96	44763	5.199	ug/L	95
23) Bromochloromethane	4.252	128	20819	5.442	ug/L	96
25) Chloroform	4.378	83	82838	4.838	ug/L	99


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VV022873.D
 Acq On : 18 Oct 2021 17:51
 Operator : SY/MD
 Sample : M4246-06MSD
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53MSD

Quant Time: Oct 19 01:45:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	5.133	62	42486	4.972	ug/L	96
29) 1,1,1-Trichloroethane	4.609	97	71278	4.939	ug/L	99
30) Cyclohexane	4.680	56	61873	4.647	ug/L	99
31) Carbon tetrachloride	4.831	117	63424	5.064	ug/L	100
33) Benzene	5.101	78	176582	5.188	ug/L	100
34) Trichloroethene	5.918	95	43947	4.748	ug/L	97
35) Methylcyclohexane	6.133	83	66442	5.124	ug/L	96
37) 1,2-Dichloropropane	6.175	63	42396	5.179	ug/L	99
38) Bromodichloromethane	6.513	83	54089	5.363	ug/L	98
39) cis-1,3-Dichloropropene	7.030	75	56238	5.190	ug/L	99
40) 4-Methyl-2-pentanone	7.227	43	210676	47.900	ug/L	99
42) Toluene	7.391	91	191598	5.545	ug/L	100
44) trans-1,3-Dichloropropene	7.654	75	48491	5.489	ug/L	92
45) 1,1,2-Trichloroethane	7.841	97	29859	4.916	ug/L	97
47) Tetrachloroethene	7.979	164	38650	5.164	ug/L	97
48) 2-Hexanone	8.140	43	151907	47.237	ug/L	97
49) Dibromochloromethane	8.246	129	36990	5.202	ug/L	90
50) 1,2-Dibromoethane	8.355	107	28423	5.011	ug/L	98
51) Chlorobenzene	8.882	112	122185	5.382	ug/L	98
52) Ethylbenzene	9.014	91	189783	5.410	ug/L	98
53) m,p-xylene	9.140	106	75800	5.506	ug/L	99
54) o-xylene	9.545	106	72045	5.563	ug/L	98
55) Styrene	9.561	104	128161	5.743	ug/L	99
57) 1,1,2,2-Tetrachloroethane	10.243	83	34600	5.630	ug/L	94
59) Bromoform	9.735	173	20225	5.038	ug/L	99
60) Isopropylbenzene	9.934	105	195734	5.377	ug/L	99
61) 1,2,3-Trichloropropane	10.275	75	23538	4.727	ug/L	99
62) 1,3,5-Trimethylbenzene	10.542	105	153207	5.209	ug/L	98
63) 1,2,4-Trimethylbenzene	10.915	105	160742	5.461	ug/L	99
64) 1,3-Dichlorobenzene	11.181	146	101466	5.311	ug/L	99
65) 1,4-Dichlorobenzene	11.275	146	104194	5.371	ug/L	98
67) 1,2-Dichlorobenzene	11.644	146	91817	5.123	ug/L	100
68) 1,2-Dibromo-3-chloropr...	12.429	75	4888	5.393	ug/L	90
69) 1,3,5-Trichlorobenzene	12.648	180	79246	5.506	ug/L	99
70) 1,2,4-trichlorobenzene	13.262	180	62128	5.651	ug/L	99
71) Naphthalene	13.503	128	92345	5.284	ug/L	97
72) 1,2,3-Trichlorobenzene	13.744	180	56617	5.461	ug/L	100





(#) = qualifier out of range (m) = manual integration (+) = signals summed

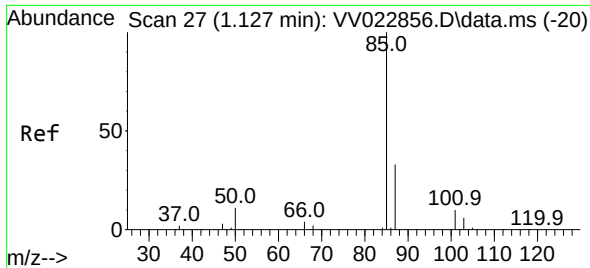

#2
 Dichlorodifluoromethane
 Concen: 5.011 ug/L
 RT: 1.127 min Scan# 27
 Delta R.T. 0.000 min
 Lab File: VV022873.D
 Acq: 18 Oct 2021 17:51




Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53MSD


Tgt Ion: 85 Resp: 45590
 Ion Ratio Lower Upper
 85 100
 87 31.8 26.3 39.5

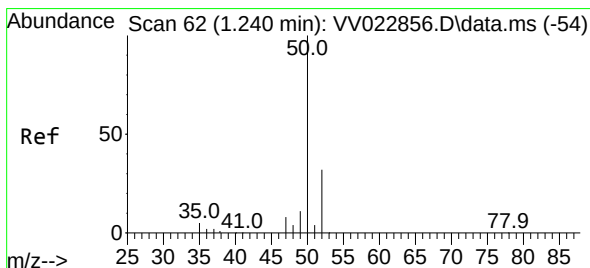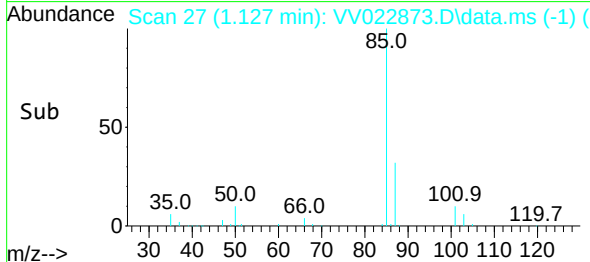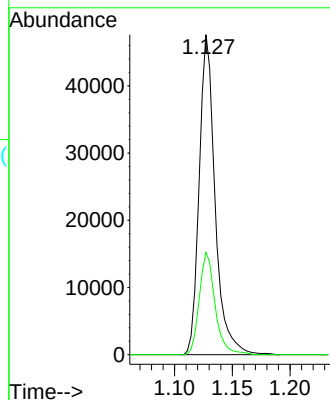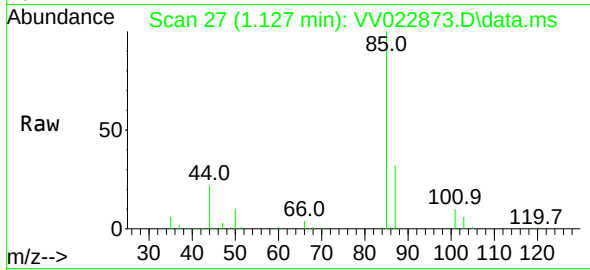

#3
 Chloromethane
 Concen: 5.301 ug/L
 RT: 1.240 min Scan# 62
 Delta R.T. 0.000 min
 Lab File: VV022873.D
 Acq: 18 Oct 2021 17:51

Tgt Ion: 50 Resp: 48471
 Ion Ratio Lower Upper
 50 100
 52 32.9 22.9 42.5


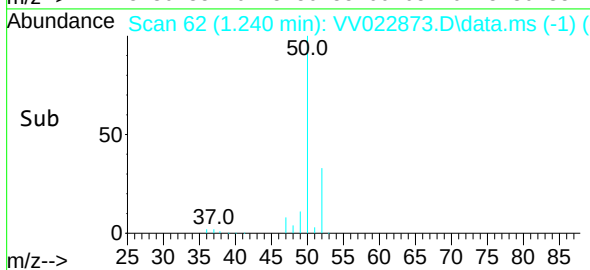
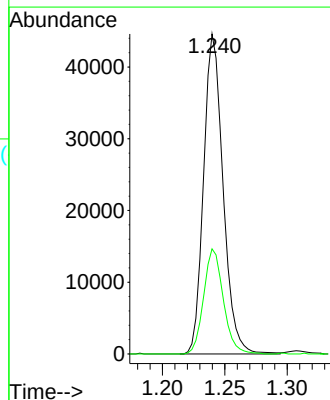
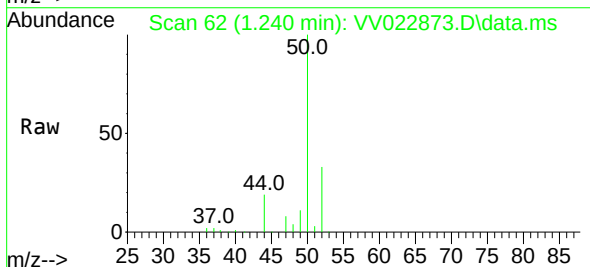


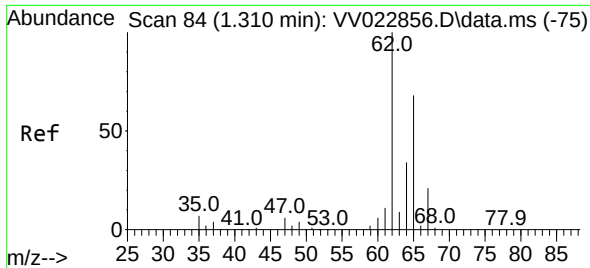

#5
 Vinyl chloride
 Concen: 5.239 ug/L
 RT: 1.310 min Scan# 84
 Delta R.T. 0.000 min
 Lab File: VV022873.D
 Acq: 18 Oct 2021 17:51




Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53MSD


Tgt Ion: 62 Resp: 49496
 Ion Ratio Lower Upper
 62 100
 64 31.6 23.0 42.8

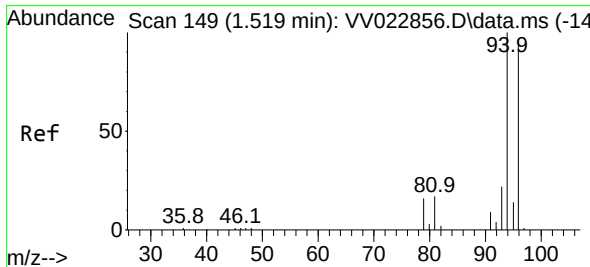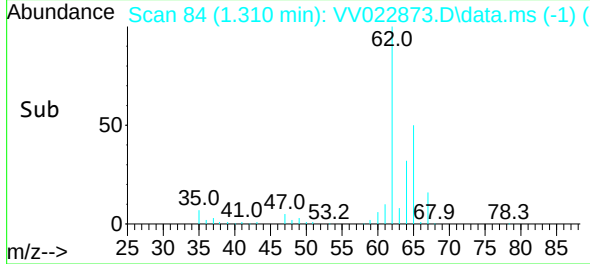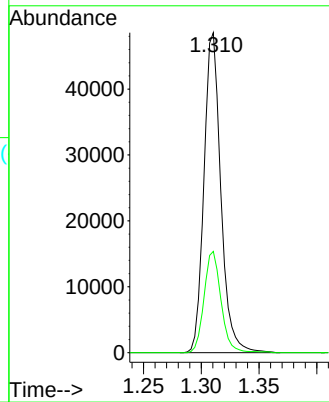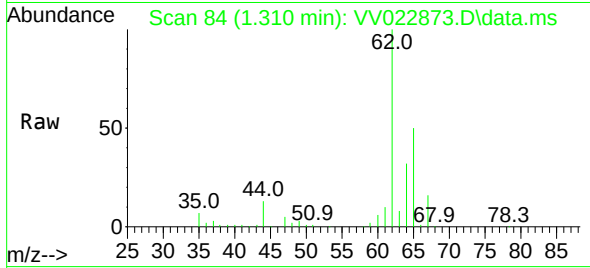

#6
 Bromomethane
 Concen: 4.342 ug/L
 RT: 1.519 min Scan# 149
 Delta R.T. 0.000 min
 Lab File: VV022873.D
 Acq: 18 Oct 2021 17:51

Tgt Ion: 94 Resp: 25572
 Ion Ratio Lower Upper
 94 100
 96 93.8 67.2 124.8


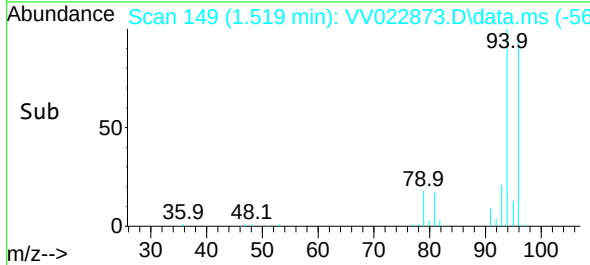
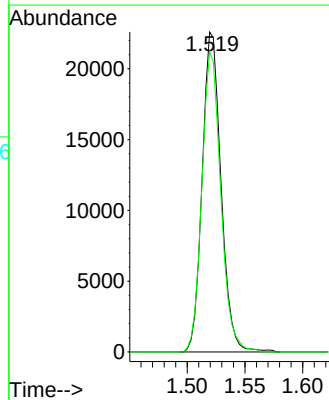
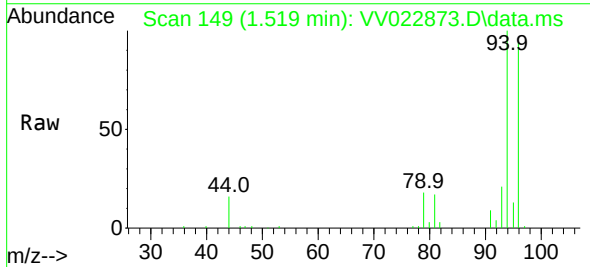


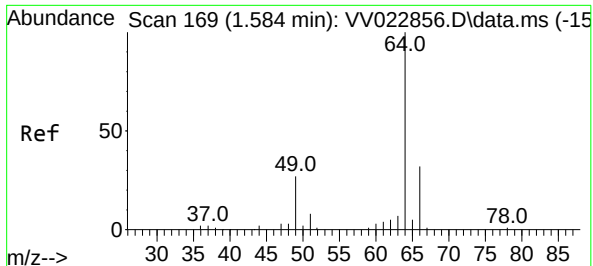

#8
Chloroethane
Concen: 4.530 ug/L
RT: 1.584 min Scan# 169
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 64 Resp: 26479
Ion Ratio Lower Upper
64 100
66 31.0 22.9 42.5

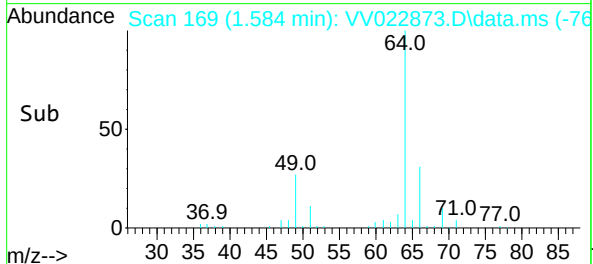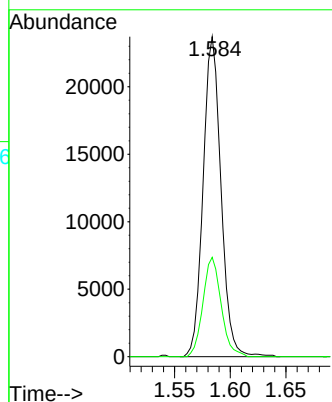

#9
Trichlorofluoromethane
Concen: 4.930 ug/L
RT: 1.751 min Scan# 221
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 101 Resp: 68229
Ion Ratio Lower Upper
101 100
103 63.7 50.3 75.5




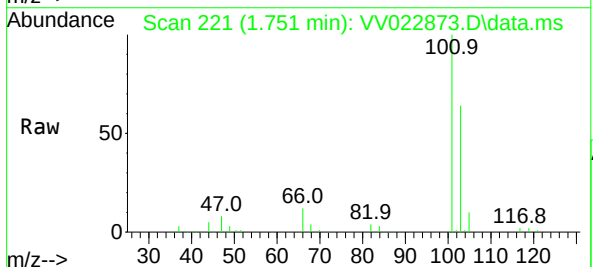




#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 4.596 ug/L
RT: 2.117 min Scan# 335
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:101 Resp: 36999
Ion Ratio Lower Upper
101 100
85 42.4 34.6 52.0
151 82.9 60.9 91.3

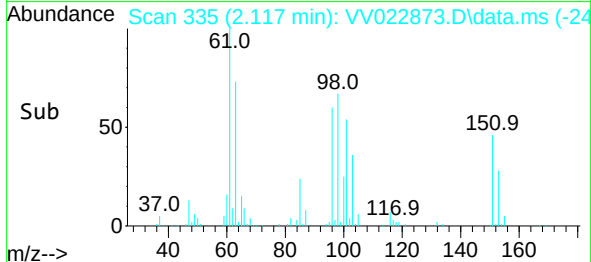

#12
1,1-Dichloroethene
Concen: 4.577 ug/L
RT: 2.117 min Scan# 335
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 96 Resp: 34514
Ion Ratio Lower Upper
96 100
61 165.5 127.3 236.5
63 121.4 106.2 197.2


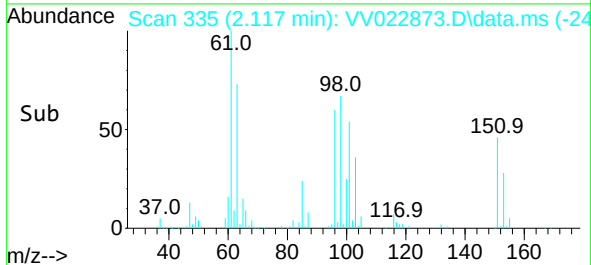






#13
Acetone
Concen: 36.917 ug/L
RT: 2.175 min Scan# 353
Delta R.T. -0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 43 Resp: 46358
Ion Ratio Lower Upper
43 100
58 33.6 0.0 24.2#

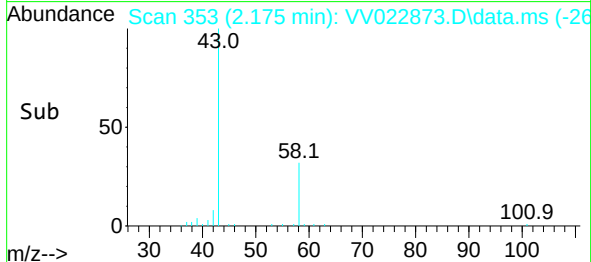

#14
Carbon disulfide
Concen: 4.567 ug/L
RT: 2.294 min Scan# 390
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 76 Resp: 96778
Ion Ratio Lower Upper
76 100
78 9.5 7.4 11.0




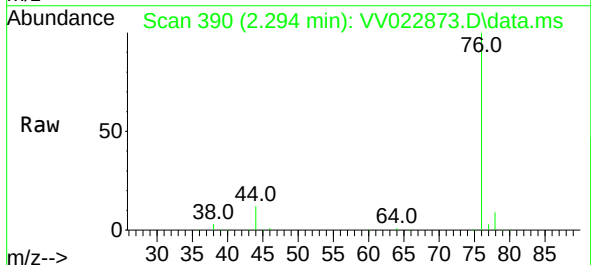




#15
Methyl Acetate
Concen: 3.247 ug/L
RT: 2.436 min Scan# 434
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampled :
YAT53MSD


Tgt Ion: 43 Resp: 11667
Ion Ratio Lower Upper
43 100
74 24.7 19.9 29.9



#16
Methylene chloride
Concen: 3.676 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 84 Resp: 38158
Ion Ratio Lower Upper
84 100
86 63.4 45.8 85.2
49 116.2 90.3 167.7


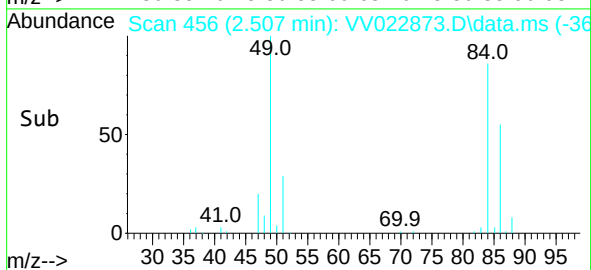






#17
Methyl tert-butyl Ether
Concen: 4.426 ug/L
RT: 2.767 min Scan# 537
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 73	Resp: 80764
Ion Ratio	Lower Upper
73 100	
43 18.8	17.1 25.7
57 21.8	17.2 25.8

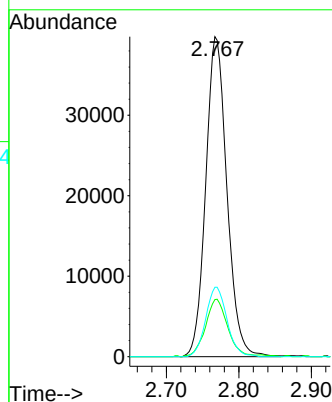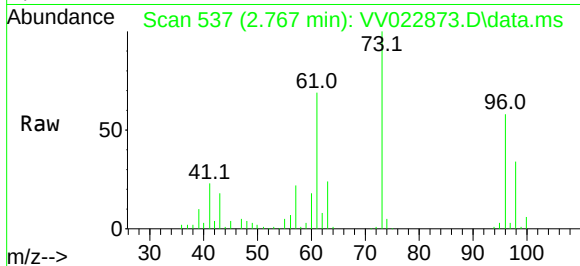

#18
trans-1,2-Dichloroethene
Concen: 5.268 ug/L
RT: 2.764 min Scan# 536
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 96	Resp: 43199
Ion Ratio	Lower Upper
96 100	
61 127.0	94.5 175.5
98 60.9	44.2 82.0

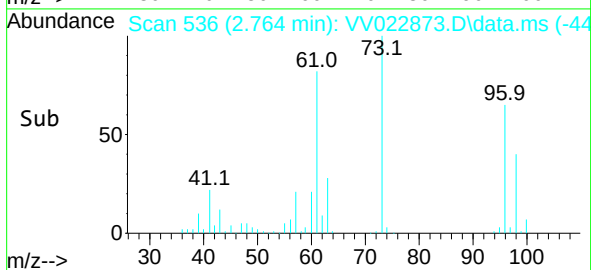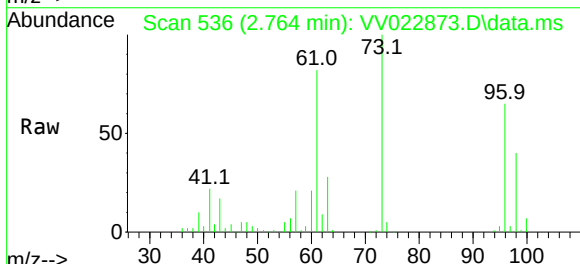



#19

1,1-Dichloroethane

Concen: 5.338 ug/L

RT: 3.191 min Scan# 669





Delta R.T. 0.006 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 63 Resp: 78842

Ion	Ratio	Lower	Upper
63	100		
65	32.1	23.5	43.7
83	13.9	10.1	18.7

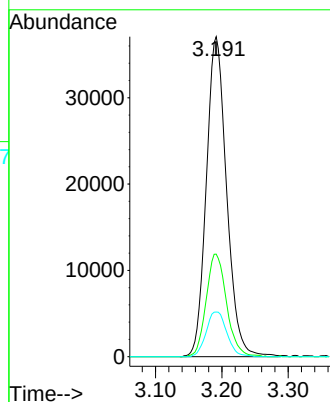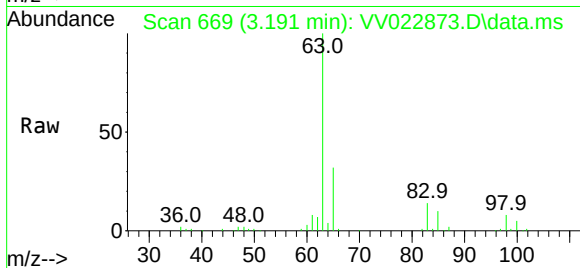

#21

2-Butanone

Concen: 40.279 ug/L

RT: 3.973 min Scan# 912




Delta R.T. -0.003 min


Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 43 Resp: 82817


Ion	Ratio	Lower	Upper
43	100		
72	26.7	12.3	36.8

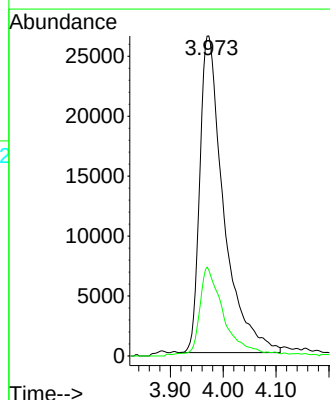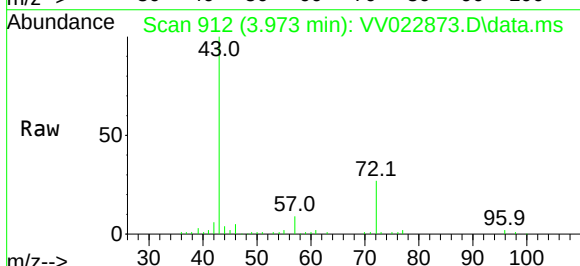






#22
cis-1,2-Dichloroethene
Concen: 5.199 ug/L
RT: 3.912 min Scan# 893
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD



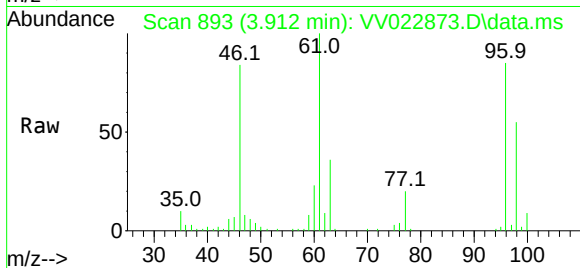



Tgt Ion:	96	Resp:	44763
Ion	Ratio	Lower	Upper
96	100		
61	117.4	86.0	159.6
68	0.0	0.0	0.0

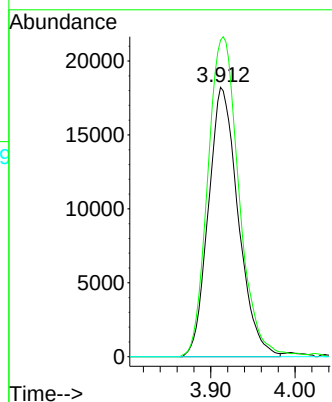

#23
Bromochloromethane
Concen: 5.442 ug/L
RT: 4.252 min Scan# 999
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:	128	Resp:	20819
Ion	Ratio	Lower	Upper
128	100		
49	149.0	106.9	198.5
130	126.5	91.9	170.7
51	46.3	40.3	60.5

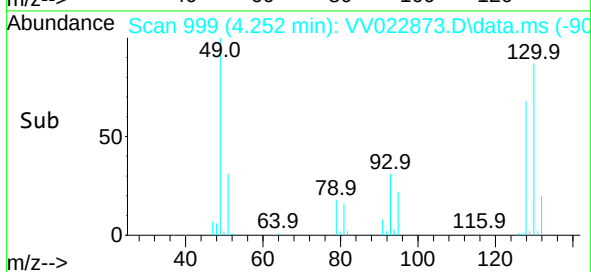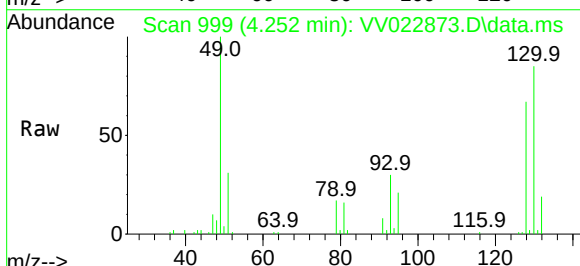



#25

Chloroform

Concen: 4.838 ug/L

RT: 4.378 min Scan# 1038

Delta R.T. 0.006 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 83 Resp: 82838

Ion Ratio Lower Upper

83 100





85 66.0 45.7 84.9

Instrument :

MSVOA_V

ClientSampleId :

YAT53MSD

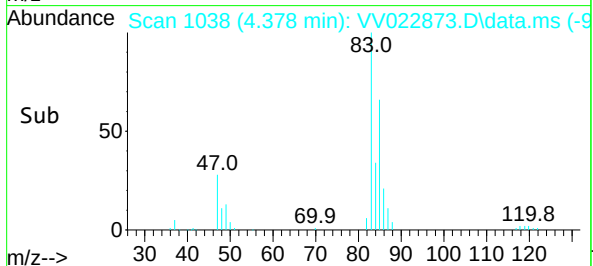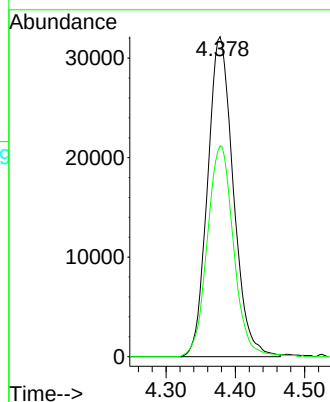

#27

1,2-Dichloroethane

Concen: 4.972 ug/L

RT: 5.133 min Scan# 1273

Delta R.T. 0.003 min

Lab File: VV022873.D




Acq: 18 Oct 2021 17:51


Tgt Ion: 62 Resp: 42486

Ion Ratio Lower Upper

62 100

98 10.6 9.7 14.5

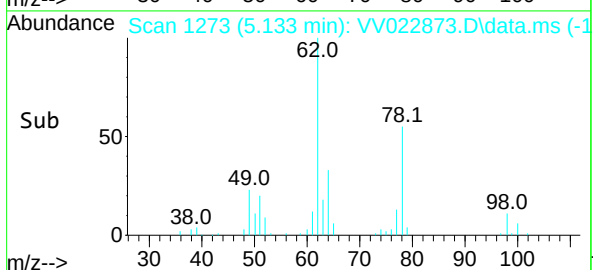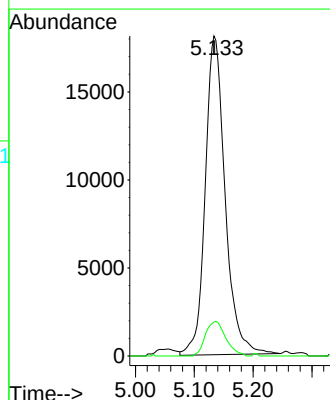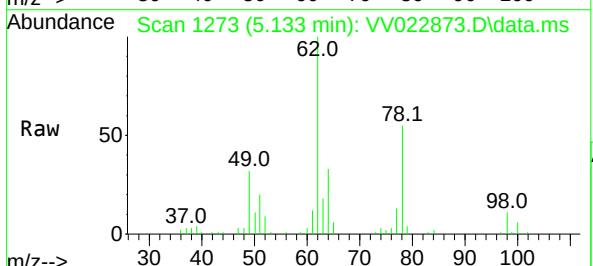



#29

1,1,1-Trichloroethane

Concen: 4.939 ug/L

RT: 4.609 min Scan# 1110





Delta R.T. 0.003 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 97	Resp: 71278
Ion Ratio	Lower Upper
97 100	
99 65.5	51.2 76.8
61 41.2	33.2 49.8

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD

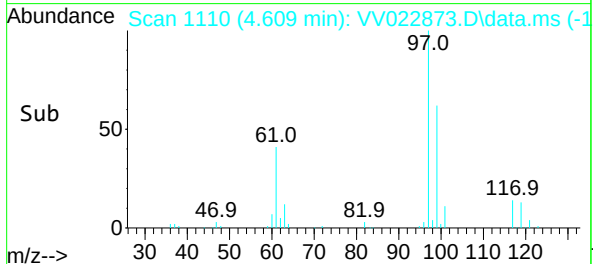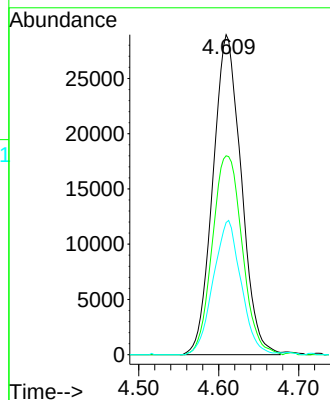

#30

Cyclohexane

Concen: 4.647 ug/L




RT: 4.680 min Scan# 1132


Delta R.T. 0.006 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 56	Resp: 61873
Ion Ratio	Lower Upper
56 100	
69 29.7	24.9 37.3
84 89.7	72.5 108.7



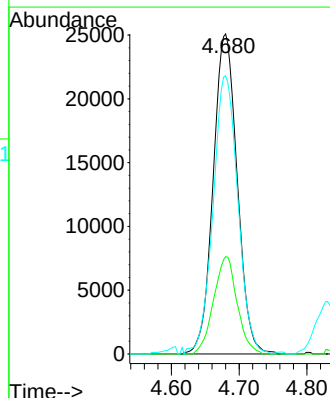
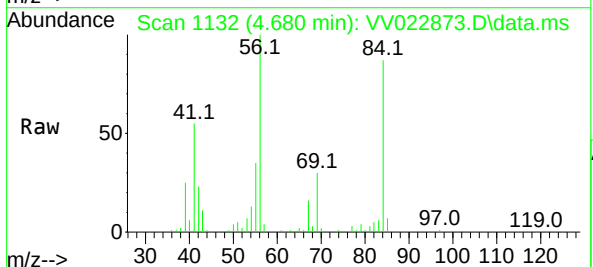




#31
Carbon tetrachloride
Concen: 5.064 ug/L
RT: 4.831 min Scan# 1179
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:117 Resp: 63424
Ion Ratio Lower Upper
117 100
119 96.9 77.4 116.0

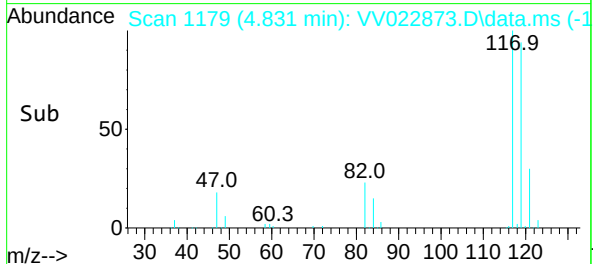

#33
Benzene
Concen: 5.188 ug/L
RT: 5.101 min Scan# 1263
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 78 Resp: 176582

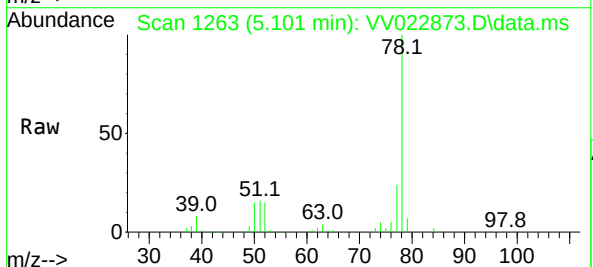



#34

Trichloroethene

Concen: 4.748 ug/L

RT: 5.918 min Scan# 1517

Delta R.T. 0.006 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion: 95 Resp: 43947





Ion Ratio Lower Upper

95 100

97 68.3 45.8 85.2

132 107.3 72.2 134.0

130 105.9 73.4 136.4

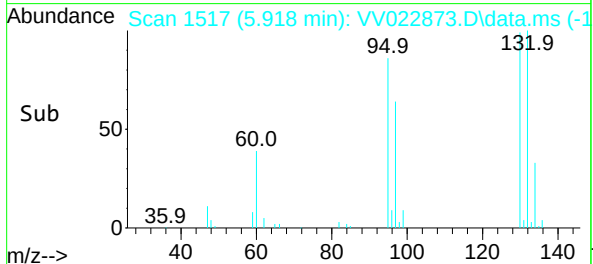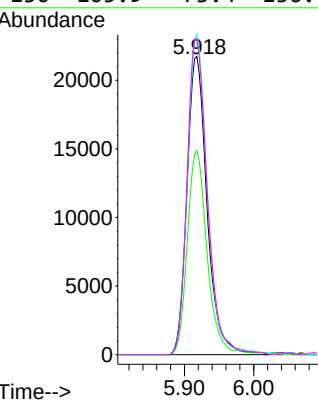

#35

Methylcyclohexane

Concen: 5.124 ug/L

RT: 6.133 min Scan# 1584

Delta R.T. 0.006 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51




Tgt Ion: 83 Resp: 66442


Ion Ratio Lower Upper

83 100

55 76.2 63.8 95.6

98 49.8 42.1 63.1


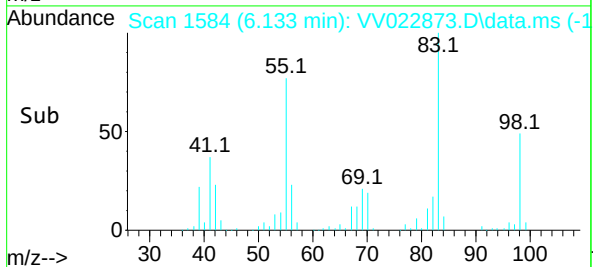
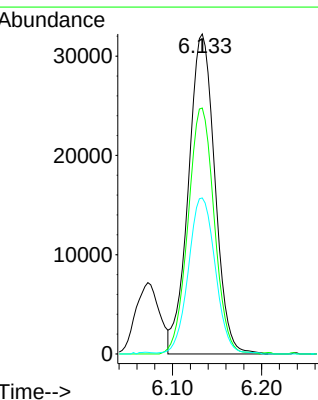
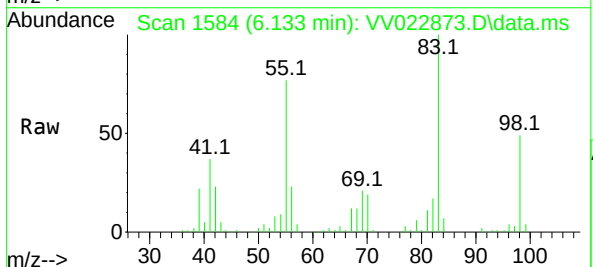




#37
1,2-Dichloropropane
Concen: 5.179 ug/L
RT: 6.175 min Scan# 1597
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 63 Resp: 42396
Ion Ratio Lower Upper
63 100
112 5.1 4.4 6.6



#38
Bromodichloromethane
Concen: 5.363 ug/L
RT: 6.513 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 83 Resp: 54089
Ion Ratio Lower Upper
83 100
85 61.7 44.3 82.3
127 9.1 7.7 11.5


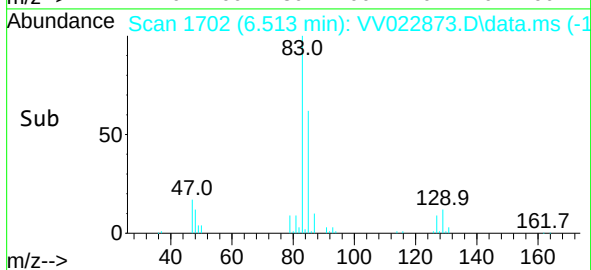




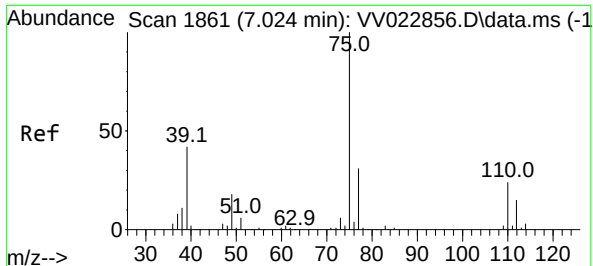

#39
cis-1,3-Dichloropropene
Concen: 5.190 ug/L
RT: 7.030 min Scan# 1863
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 75 Resp: 56238
Ion Ratio Lower Upper
75 100
77 32.3 22.3 41.3

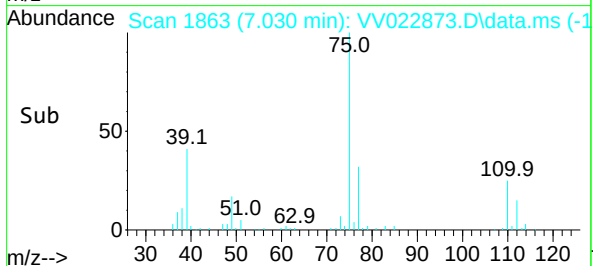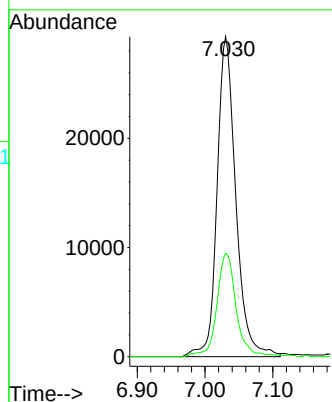

#40
4-Methyl-2-pentanone
Concen: 47.900 ug/L
RT: 7.227 min Scan# 1924
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 43 Resp: 210676
Ion Ratio Lower Upper
43 100
58 40.4 32.0 48.0
100 17.1 14.2 21.2


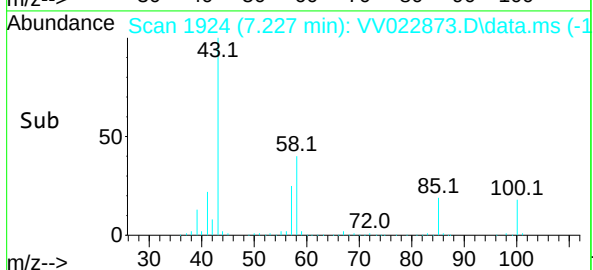

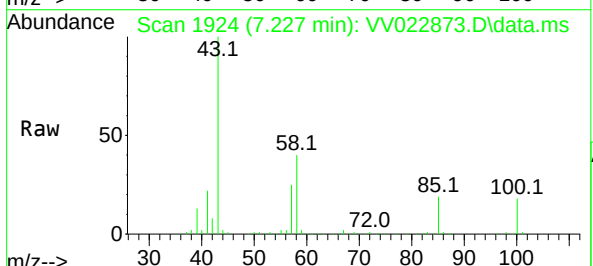


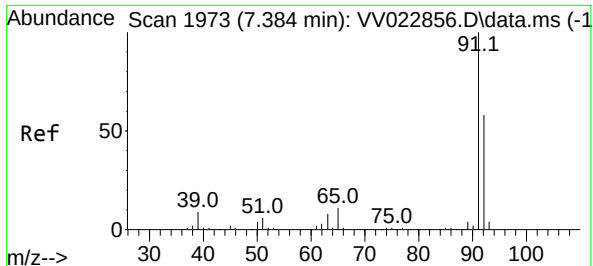

#42
Toluene
Concen: 5.545 ug/L
RT: 7.391 min Scan# 1975
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 91 Resp: 191598
Ion Ratio Lower Upper
91 100
92 58.1 40.7 75.7

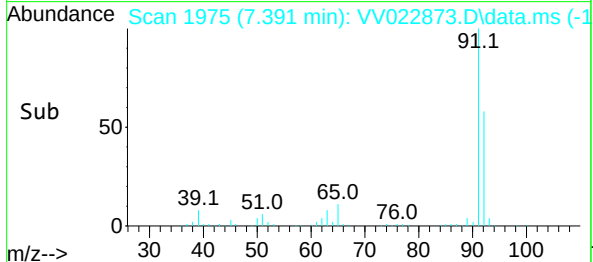

#44
trans-1,3-Dichloropropene
Concen: 5.489 ug/L
RT: 7.654 min Scan# 2057
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 75 Resp: 48491
Ion Ratio Lower Upper
75 100
77 29.6 23.9 44.5


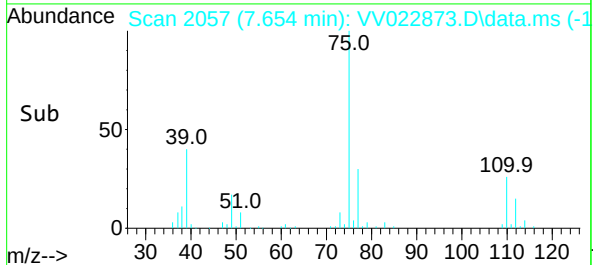

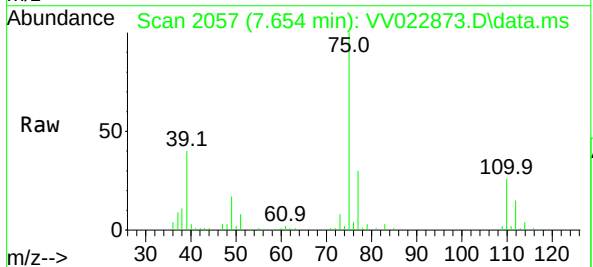




#45
1,1,2-Trichloroethane
Concen: 4.916 ug/L
RT: 7.841 min Scan# 2115
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 97	Resp:	29859
Ion Ratio	Lower	Upper
97	100	
99	64.1	44.5 82.7
83	86.6	56.6 105.0
85	54.3	37.2 69.0



#47
Tetrachloroethene
Concen: 5.164 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.006 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 164	Resp:	38650
Ion Ratio	Lower	Upper
164	100	
129	89.4	65.0 120.6
131	83.2	62.2 115.4
166	127.1	89.2 165.8

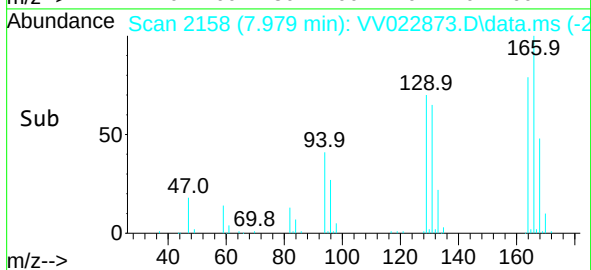




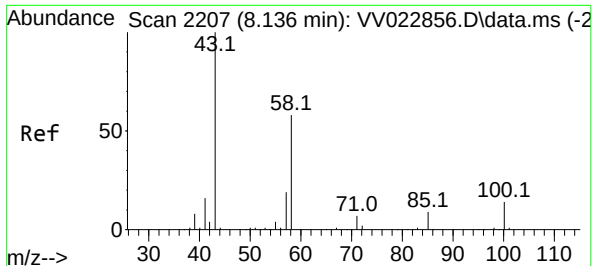


#48
2-Hexanone
Concen: 47.237 ug/L
RT: 8.140 min Scan# 2208
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD

Tgt Ion: 43 Resp: 151907




Ion	Ratio	Lower	Upper
43	100		
58	56.5	47.4	71.0
57	18.8	15.3	22.9
100	13.6	10.4	15.6

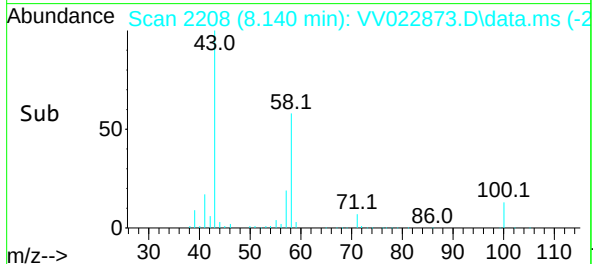


#49
Dibromochloromethane
Concen: 5.202 ug/L
RT: 8.246 min Scan# 2241
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 129 Resp: 36990

Ion	Ratio	Lower	Upper
129	100		
127	75.5	59.1	109.9

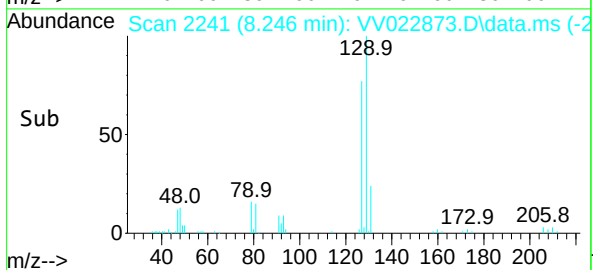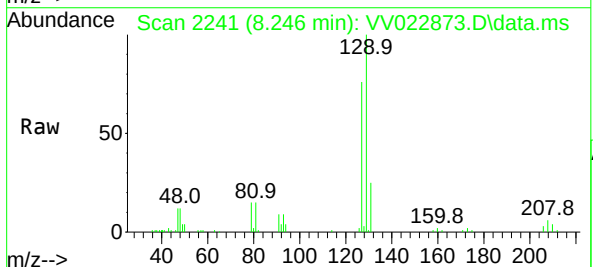



#50

1,2-Dibromoethane

Concen: 5.011 ug/L

RT: 8.355 min Scan# 2275





Delta R.T. 0.003 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion:	107	Resp:	28423
Ion	Ratio	Lower	Upper
107	100		
109	94.2	67.1	124.5
188	5.0	3.4	5.0

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD

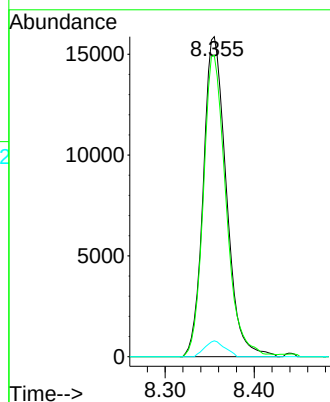

#51

Chlorobenzene

Concen: 5.382 ug/L




RT: 8.882 min Scan# 2439


Delta R.T. 0.003 min

Lab File: VV022873.D

Acq: 18 Oct 2021 17:51

Tgt Ion:	112	Resp:	122185
Ion	Ratio	Lower	Upper
112	100		
114	32.7	21.6	40.2
77	55.3	43.7	65.5

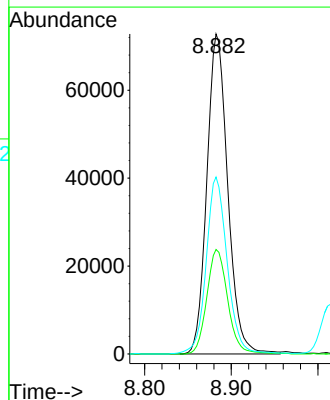



#52

Ethylbenzene

Concen: 5.410 ug/L

RT: 9.014 min Scan# 2480

Delta R.T. 0.003 min

Lab File: VV022873.D





Acq: 18 Oct 2021 17:51

Tgt Ion: 91 Resp: 189783

Ion Ratio Lower Upper

91 100

106 31.9 21.6 40.2



#53

m,p-xylene

Concen: 5.506 ug/L

RT: 9.140 min Scan# 2519

Delta R.T. 0.003 min

Lab File: VV022873.D




Acq: 18 Oct 2021 17:51


Tgt Ion: 106 Resp: 75800

Ion Ratio Lower Upper

106 100

91 199.5 138.7 257.5









#54
o-xylene
Concen: 5.563 ug/L
RT: 9.545 min Scan# 2645
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:106 Resp: 72045
Ion Ratio Lower Upper
106 100
91 213.1 151.1 280.7



#55
Styrene
Concen: 5.743 ug/L
RT: 9.561 min Scan# 2650
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:104 Resp: 128161
Ion Ratio Lower Upper
104 100
78 41.4 29.5 54.7









#57
1,1,2,2-Tetrachloroethane
Concen: 5.630 ug/L
RT: 10.243 min Scan# 2862
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion: 83 Resp: 34600
Ion Ratio Lower Upper
83 100
85 61.0 46.0 85.4
131 9.1 8.4 12.6

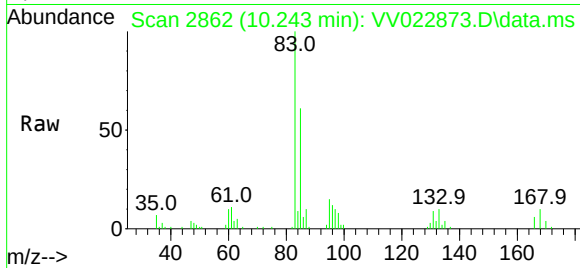

#59
Bromoform
Concen: 5.038 ug/L
RT: 9.735 min Scan# 2704
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 173 Resp: 20225
Ion Ratio Lower Upper
173 100
175 48.5 38.3 57.5
254 9.7 7.1 10.7


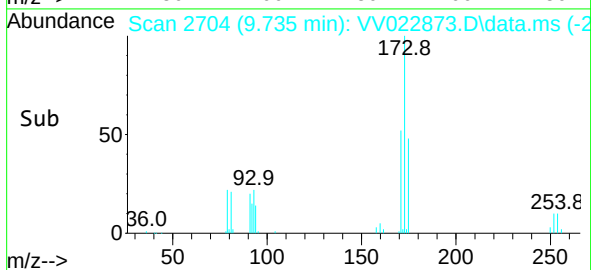

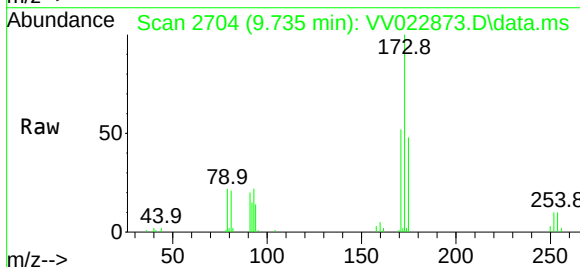




#60
Isopropylbenzene
Concen: 5.377 ug/L
RT: 9.934 min Scan# 2766
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:105 Resp: 195734
Ion Ratio Lower Upper
105 100
120 26.9 21.8 32.8
77 14.7 12.5 18.7

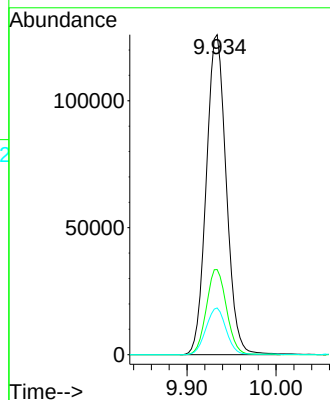

#61
1,2,3-Trichloropropane
Concen: 4.727 ug/L
RT: 10.275 min Scan# 2872
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion: 75 Resp: 23538
Ion Ratio Lower Upper
75 100
77 33.0 25.4 38.2
110 43.2 34.2 51.4


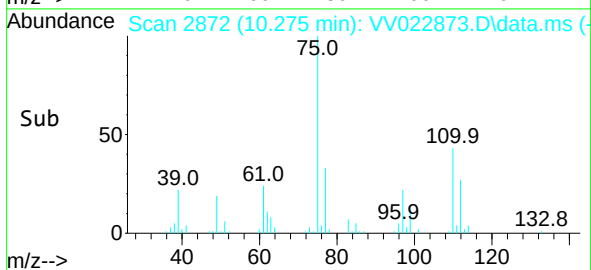
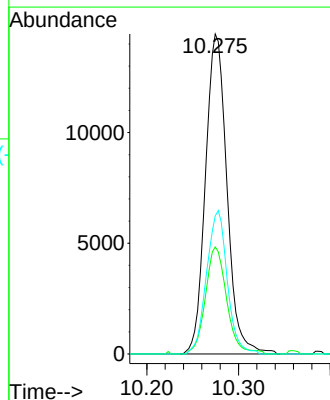



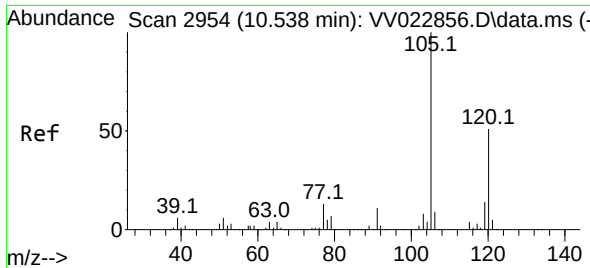

#62
1,3,5-Trimethylbenzene
Concen: 5.209 ug/L
RT: 10.542 min Scan# 2955
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:105 Resp: 153207
Ion Ratio Lower Upper
105 100
120 50.6 39.4 59.2

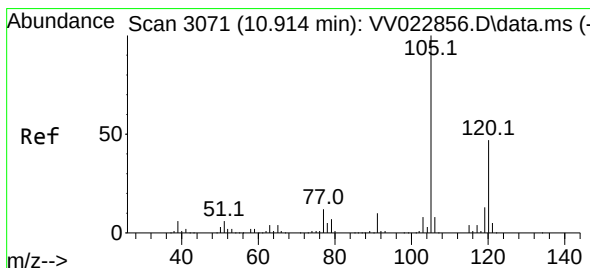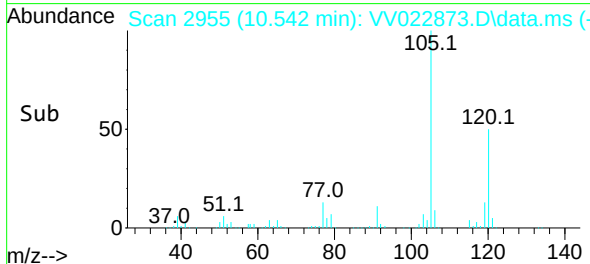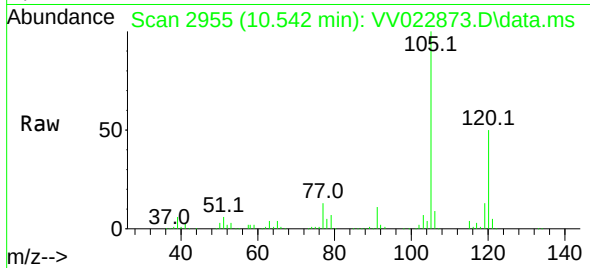

#63
1,2,4-Trimethylbenzene
Concen: 5.461 ug/L
RT: 10.915 min Scan# 3071
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:105 Resp: 160742
Ion Ratio Lower Upper
105 100
120 46.1 37.3 55.9


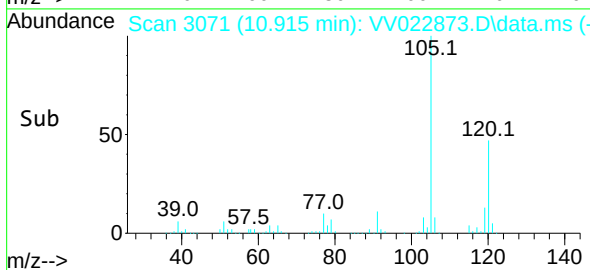

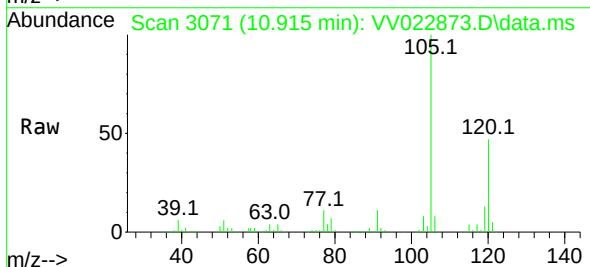




#64
1,3-Dichlorobenzene
Concen: 5.311 ug/L
RT: 11.181 min Scan# 3154
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:146 Resp: 101466
Ion Ratio Lower Upper
146 100
111 39.1 26.7 49.5
148 64.4 45.1 83.9

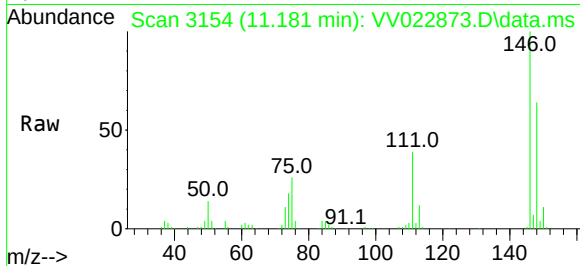

#65
1,4-Dichlorobenzene
Concen: 5.371 ug/L
RT: 11.275 min Scan# 3183
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:146 Resp: 104194
Ion Ratio Lower Upper
146 100
111 34.5 25.6 47.4
148 63.2 44.9 83.5


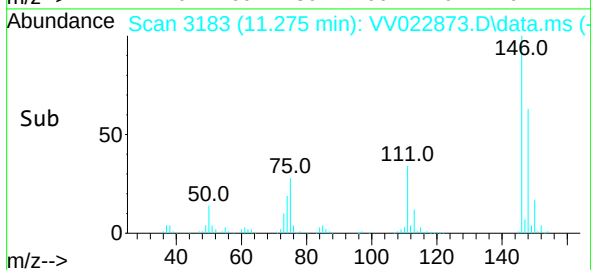

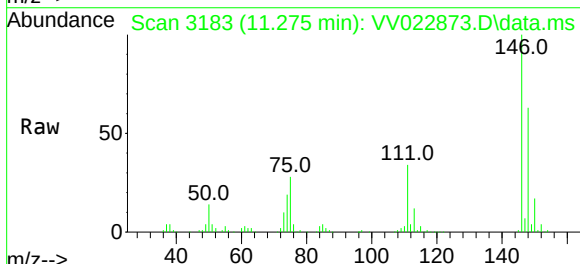




#67
1,2-Dichlorobenzene
Concen: 5.123 ug/L
RT: 11.644 min Scan# 3298
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51




Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD


Tgt Ion:146 Resp: 91817
Ion Ratio Lower Upper
146 100
111 40.3 32.3 48.5
148 65.4 52.1 78.1

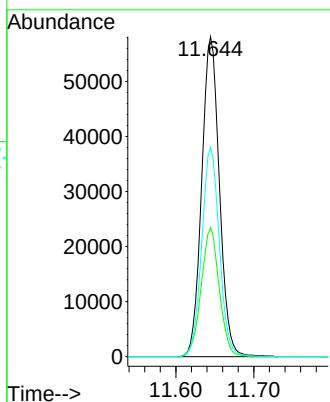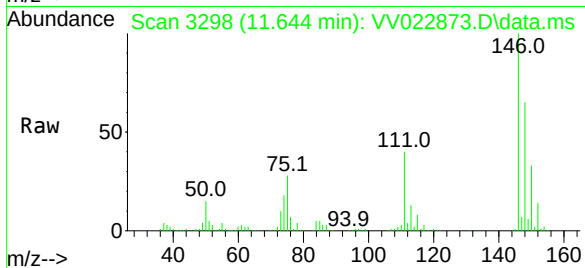

#68
1,2-Dibromo-3-chloropropane
Concen: 5.393 ug/L
RT: 12.429 min Scan# 3542
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51


Tgt Ion: 75 Resp: 4888
Ion Ratio Lower Upper
75 100
155 93.4 82.4 123.6
157 129.3 114.1 171.1

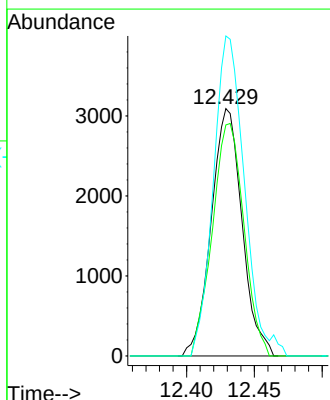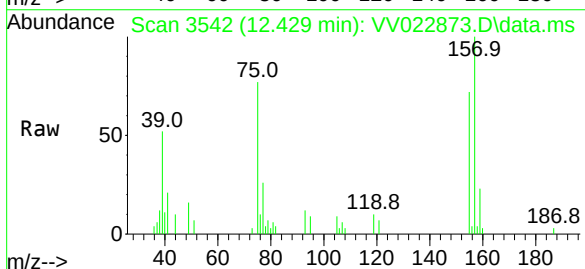






#69
1,3,5-Trichlorobenzene
Concen: 5.506 ug/L
RT: 12.648 min Scan# 3610
Delta R.T. 0.003 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD



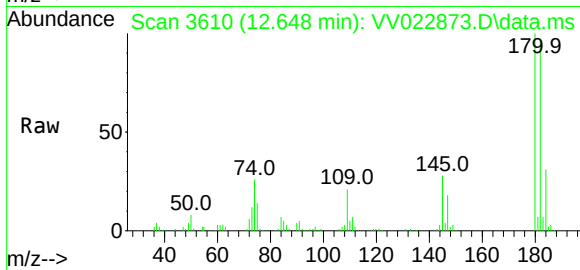



Tgt Ion:180 Resp: 79246
Ion Ratio Lower Upper
180 100
182 95.6 77.0 115.6
184 30.4 24.5 36.7
145 28.6 23.9 35.9



#70
1,2,4-trichlorobenzene
Concen: 5.651 ug/L
RT: 13.262 min Scan# 3801
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:180 Resp: 62128
Ion Ratio Lower Upper
180 100
182 96.1 76.0 114.0
145 29.1 24.1 36.1




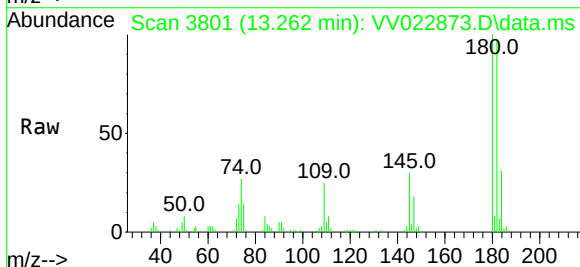




#71
Naphthalene
Concen: 5.284 ug/L
RT: 13.503 min Scan# 3876
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Instrument :
MSVOA_V
ClientSampleId :
YAT53MSD

Tgt Ion:128	Resp:	92345
Ion Ratio	Lower	Upper
128	100	
129	10.8	9.3 13.9
127	12.3	10.8 16.2

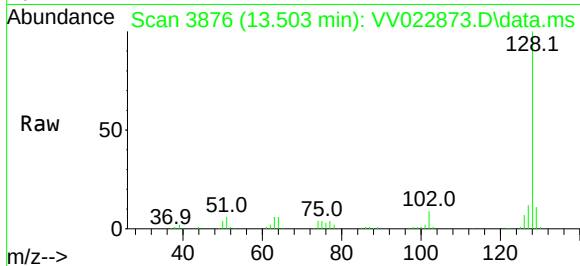

#72
1,2,3-Trichlorobenzene
Concen: 5.461 ug/L
RT: 13.744 min Scan# 3951
Delta R.T. 0.000 min
Lab File: VV022873.D
Acq: 18 Oct 2021 17:51

Tgt Ion:180	Resp:	56617
Ion Ratio	Lower	Upper
180	100	
182	93.9	75.5 113.3
145	31.0	24.7 37.1

