


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022879.D
Acq On : 18 Oct 2021 20:15
Operator : SY/MD
Sample : M4200-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGF1

Manual Integrations
APPROVED

MMDadoda
10/19/2021 3:47:55 PM

Quant Time: Oct 19 01:46:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 01:43:03 2021
Response via : Initial Calibration

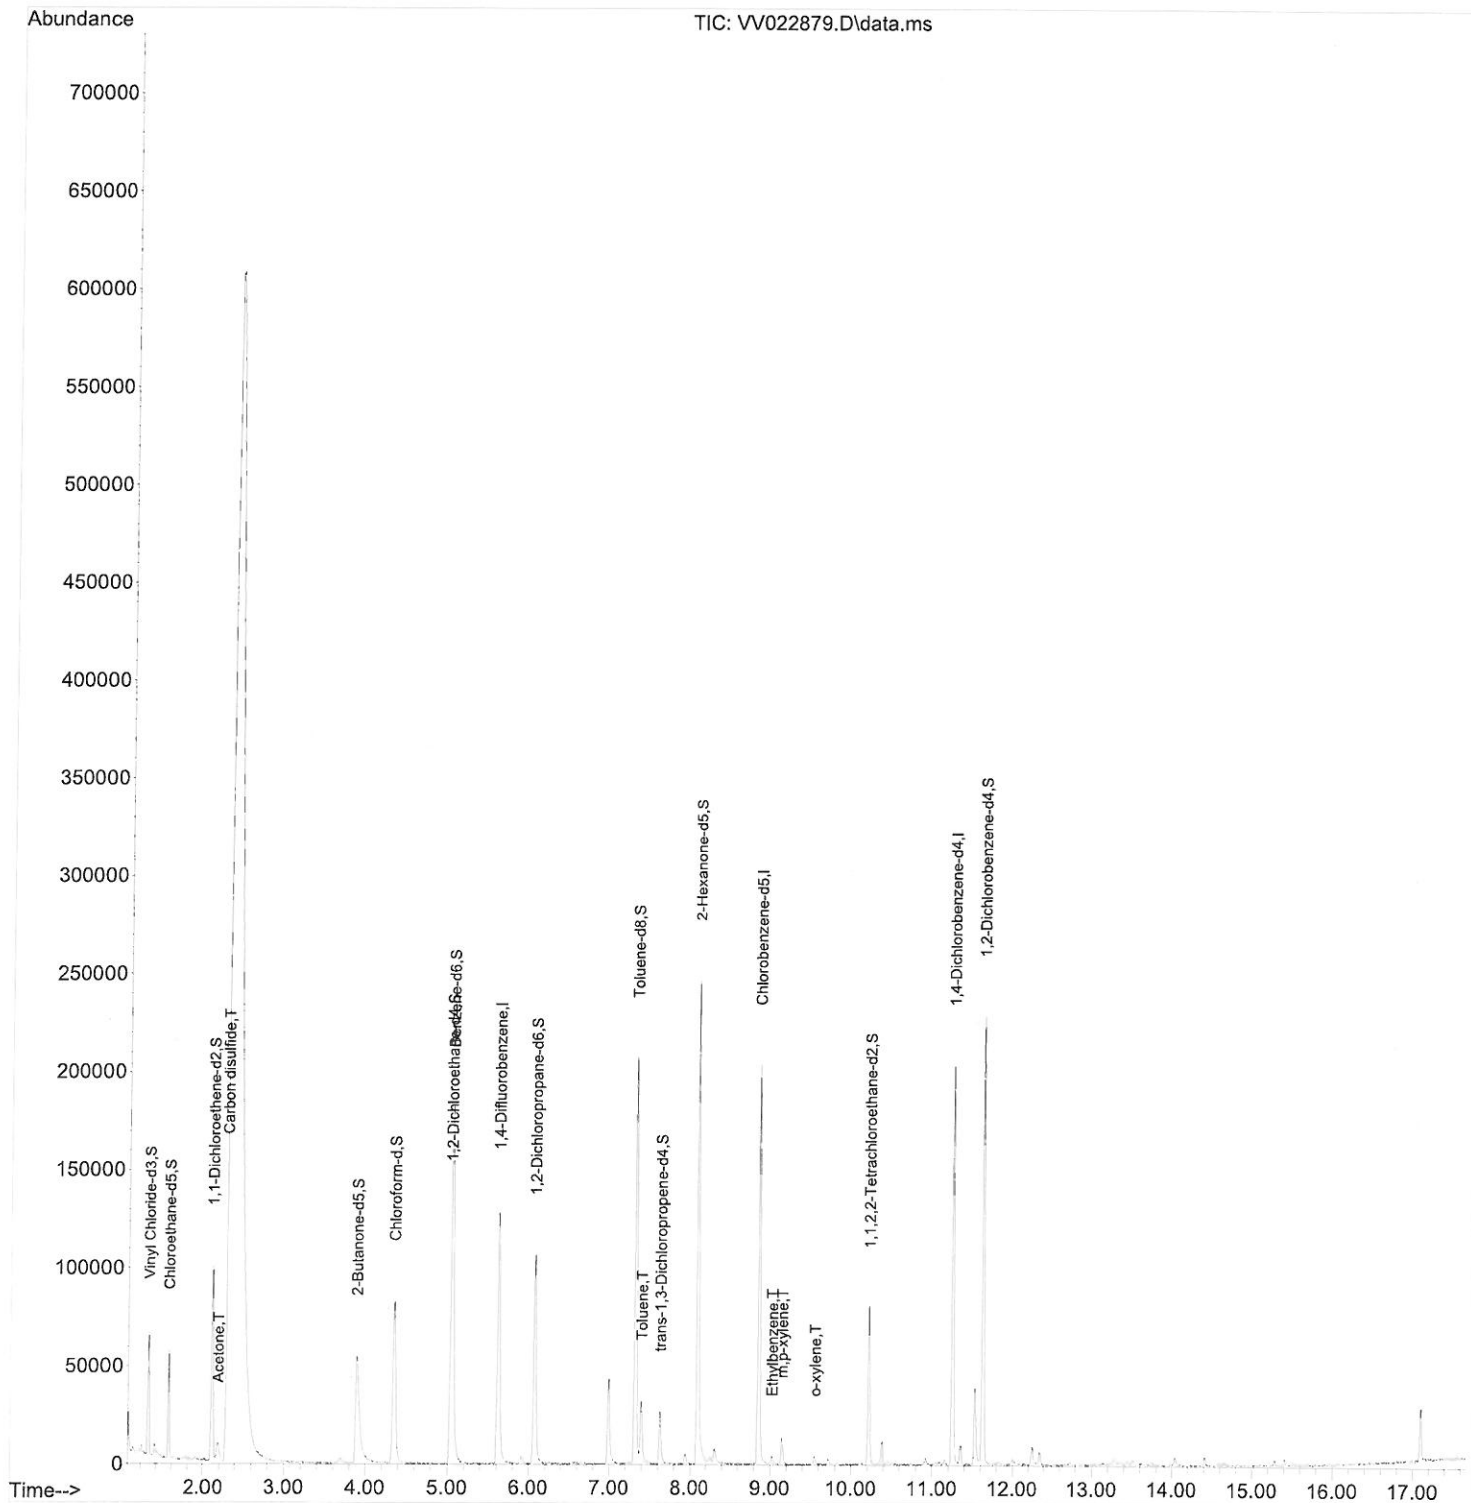

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022879.D
 Acq On : 18 Oct 2021 20:15
 Operator : SY/MD
 Sample : M4200-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGF1

Manual Integrations
 APPROVED

MMDadoda
 10/19/2021 3:47:55 PM

Quant Time: Oct 19 01:46:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

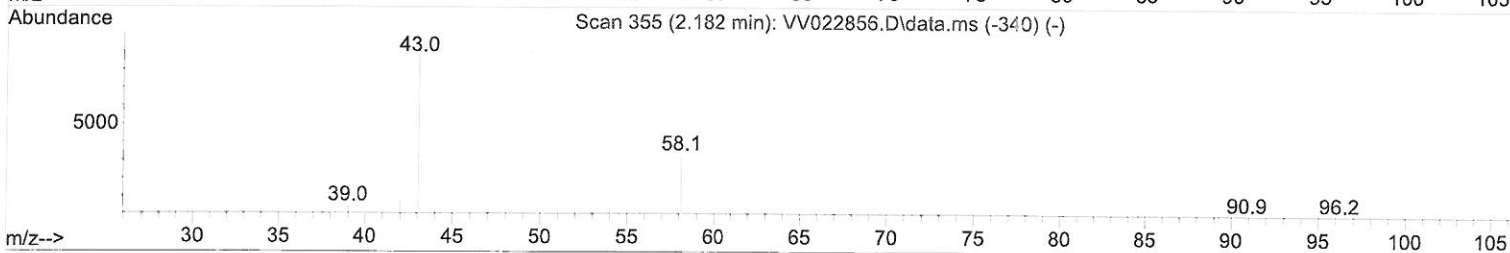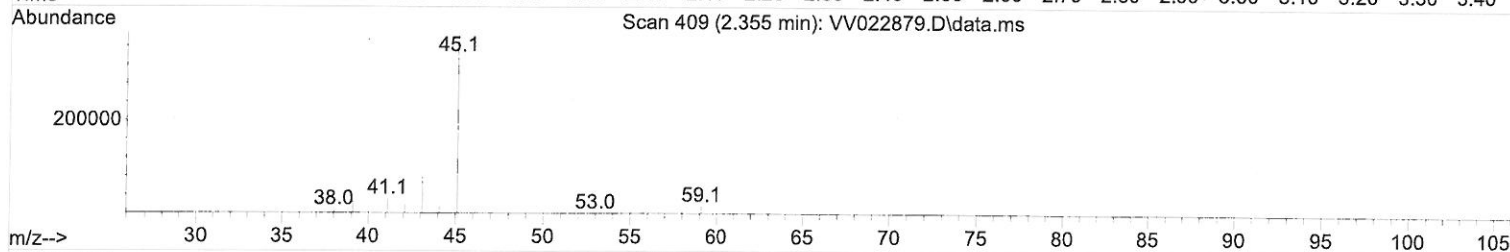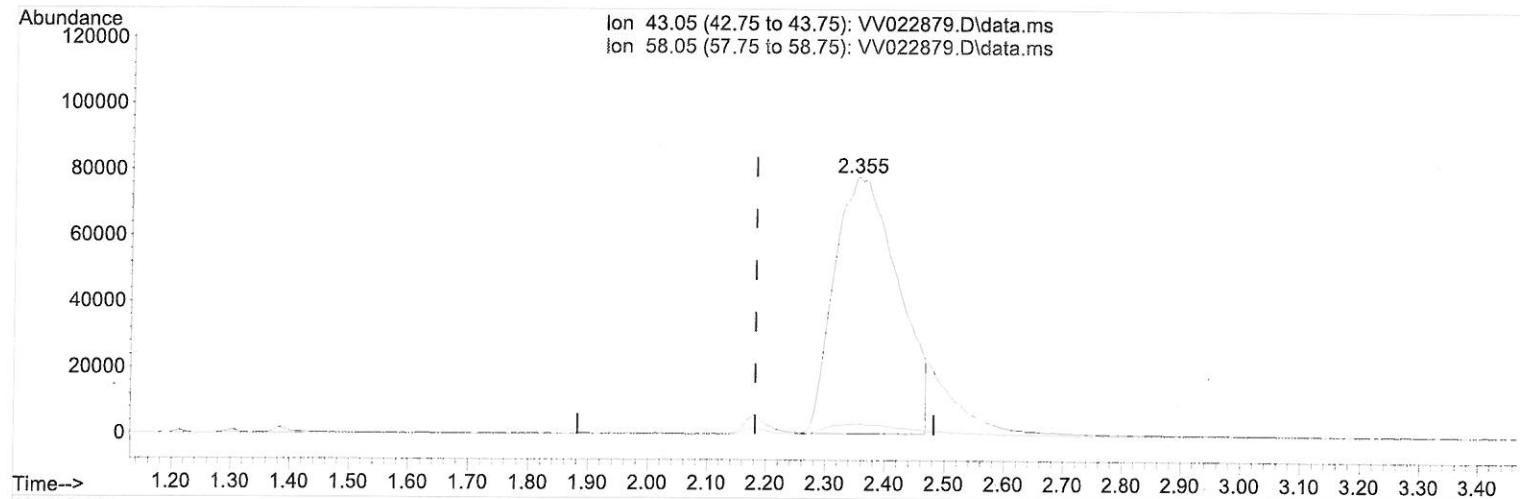

TIC: VV022879.D\data.ms

(13) Acetone (T)

2.355min (+ 0.174) 490.88 ug/L

response 578121

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	1.81
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022879.D
 Acq On : 18 Oct 2021 20:15
 Operator : SY/MD
 Sample : M4200-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGF1

Manual Integrations
 APPROVED

MMDadoda
 10/19/2021 3:47:55 PM

Quant Time: Oct 19 01:46:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

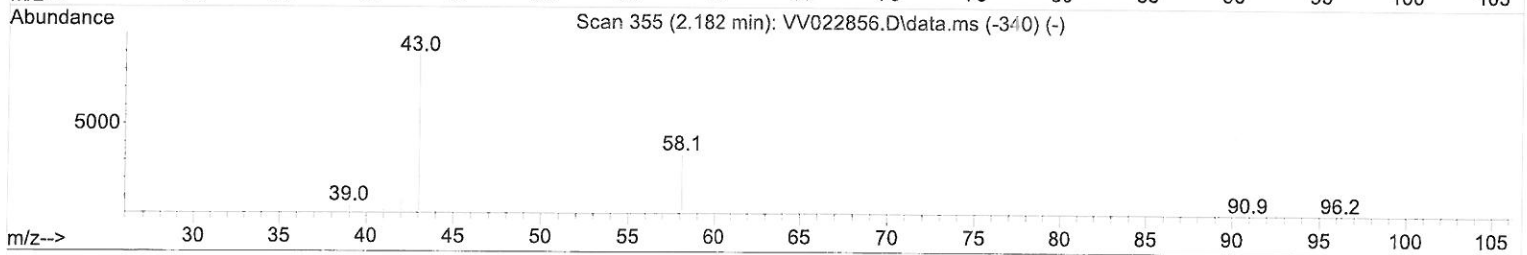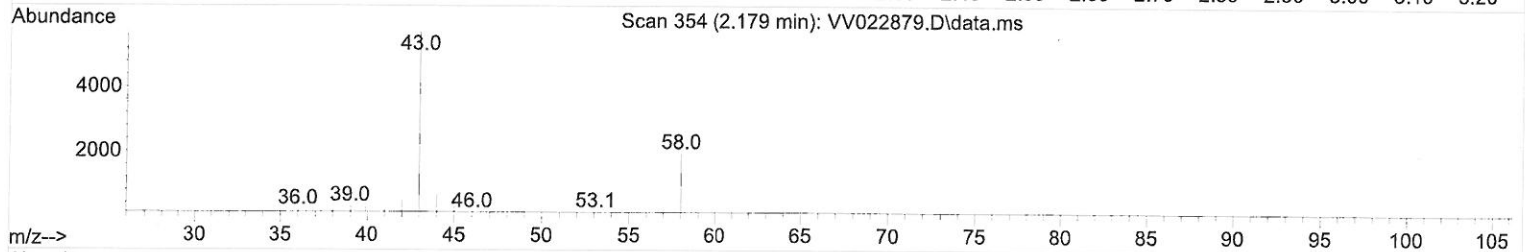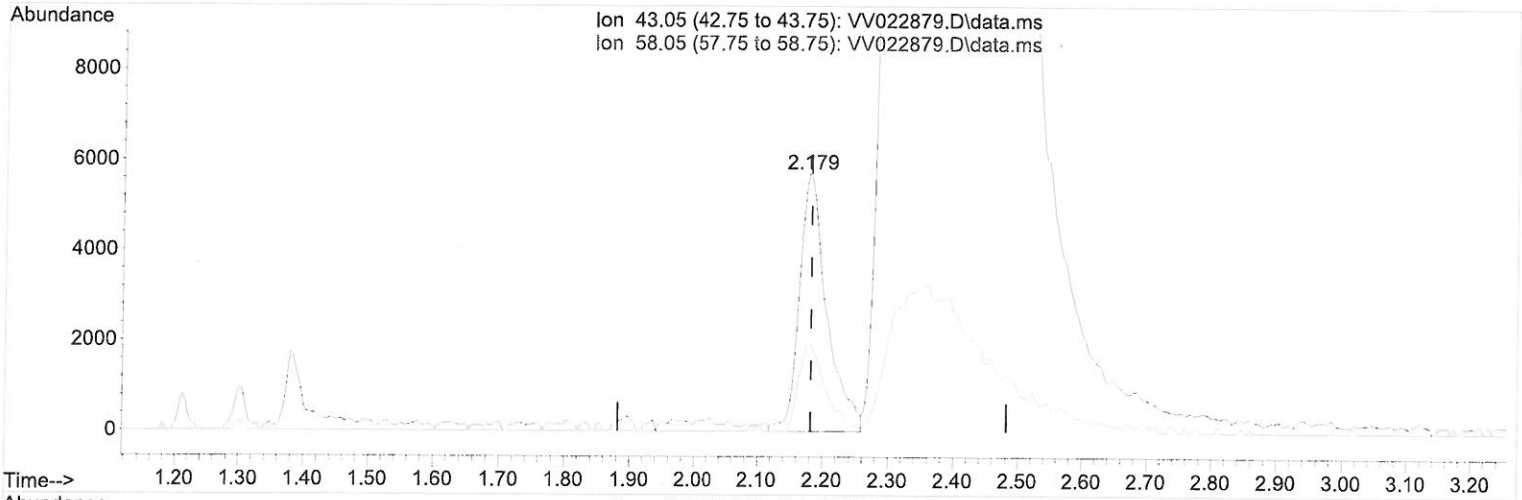

TIC: VV022879.D\data.ms

(13) Acetone (T)

2.179min (-0.003) 14.19 ug/L m

response 16707

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	62.55#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 2 MD
 10/24/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VW022879.D
 Acq On : 18 Oct 2021 20:15
 Operator : SY/MD
 Sample : M4200-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGF1

Manual Integrations
 APPROVED

MMDadoda
 10/19/2021 3:47:55 PM

Quant Time: Oct 19 01:46:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117076	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	119306	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	56183	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	34277	4.255	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	85.200%		
7) Chloroethane-d5	1.564	69	32869	4.541	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	90.800%		
11) 1,1-Dichloroethene-d2	2.105	63	51240	3.243	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.800%		
20) 2-Butanone-d5	3.889	46	105971	50.174	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	100.340%		
24) Chloroform-d	4.349	84	85714	5.164	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.200%		
26) 1,2-Dichloroethane-d4	5.034	65	40966	5.085	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	101.600%		
32) Benzene-d6	5.050	84	166196	4.679	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.600%		
36) 1,2-Dichloropropane-d6	6.072	67	54836	5.214	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	104.200%		
41) Toluene-d8	7.317	98	140124	4.564	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	91.200%		
43) trans-1,3-Dichloroprop...	7.625	79	15738	4.511	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.200%		
46) 2-Hexanone-d5	8.091	63	81739	58.131	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	116.260%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38782	5.443	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	108.800%		
66) 1,2-Dichlorobenzene-d4	11.625	152	60554	5.813	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	116.200%		
Target Compounds						
13) Acetone	2.179	43	16707m	14.186	ug/L	Qvalue
14) Carbon disulfide	2.291	76	2691	0.135	ug/L #	93
42) Toluene	7.394	91	24568	0.753	ug/L	91
52) Ethylbenzene	9.021	91	3005	0.091	ug/L	96
53) m,p-xylene	9.143	106	3734	0.287	ug/L	89
54) o-xylene	9.551	106	1271	0.104	ug/L	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 10/27/21